

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007521.D
 Acq On : 20 Oct 2021 10:40
 Operator : CG/JU
 Sample : M4246-04
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YAT53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	20	rVB	16657	21411	0.36%	0.043%
2	3.658	60	63	70	rVB5	7434	11298	0.19%	0.022%
3	3.799	84	87	100	rBV	197045	307552	5.22%	0.611%
4	4.040	124	128	135	rVB2	26586	43026	0.73%	0.085%
5	4.128	140	143	149	rVB	10584	16762	0.28%	0.033%
6	4.228	157	160	164	rVB2	10657	13170	0.22%	0.026%
7	6.040	463	468	473	rVB7	5421	9632	0.16%	0.019%
8	6.334	514	518	526	rVB4	10434	17037	0.29%	0.034%
9	7.110	642	650	661	rVB	188318	310816	5.28%	0.617%
10	7.281	670	679	689	rBV	653763	1033943	17.55%	2.054%
11	7.481	706	713	721	rBV	654917	1041161	17.67%	2.068%
12	7.952	786	793	801	rBV	662721	1056652	17.93%	2.099%
13	8.204	832	836	842	rBV9	4366	8796	0.15%	0.017%
14	8.375	861	865	870	rBV6	3922	5905	0.10%	0.012%
15	8.522	884	890	894	rBV8	3930	6769	0.11%	0.013%
16	8.657	906	913	921	rBV	548831	853162	14.48%	1.695%
17	9.110	980	990	1002	rBV	788610	1283826	21.79%	2.550%
18	9.581	1063	1070	1076	rVB3	13983	24619	0.42%	0.049%
19	9.834	1105	1113	1124	rBV	579742	956708	16.24%	1.900%
20	10.375	1196	1205	1216	rBV	960782	1567933	26.61%	3.115%
21	10.540	1227	1233	1246	rBV2	84360	138532	2.35%	0.275%
22	10.757	1260	1270	1279	rVB	906823	1522868	25.85%	3.025%
23	10.887	1284	1292	1305	rBV	662078	1106603	18.78%	2.198%
24	12.081	1490	1495	1500	rVB	12846	20619	0.35%	0.041%
25	12.345	1535	1540	1544	rVB2	20408	28868	0.49%	0.057%
26	12.963	1640	1645	1649	rBV6	8165	13870	0.24%	0.028%
27	13.210	1682	1687	1692	rBV4	12560	19765	0.34%	0.039%
28	13.434	1718	1725	1731	rBV	27664	41905	0.71%	0.083%
29	13.498	1731	1736	1743	rVV6	9021	15185	0.26%	0.030%
30	13.563	1743	1747	1751	rVB7	6187	8636	0.15%	0.017%
31	13.628	1751	1758	1763	rBV7	4542	7522	0.13%	0.015%
32	13.998	1814	1821	1827	rBV	1957538	2667158	45.27%	5.298%
33	14.281	1857	1869	1878	rBV	2072259	3037646	51.56%	6.034%
34	14.587	1914	1921	1933	rBV	1372587	2138132	36.29%	4.247%
35	14.769	1941	1952	1960	rBV	185413	281479	4.78%	0.559%
36	15.004	1989	1992	1996	rVB6	7420	9448	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007521.D
 Acq On : 20 Oct 2021 10:40
 Operator : CG/JU
 Sample : M4246-04
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YAT53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	15.404	2056	2060	2065	rVB6	5979	9974	0.17%	0.020%
38	15.581	2083	2090	2099	rBV	2801758	4061234	68.93%	8.067%
39	15.692	2102	2109	2119	rBV	727197	979555	16.63%	1.946%
40	15.822	2126	2131	2137	rVB	36312	55479	0.94%	0.110%
41	15.957	2148	2154	2158	rVB9	3212	6420	0.11%	0.013%
42	16.028	2163	2166	2170	rVB6	5002	6021	0.10%	0.012%
43	16.263	2200	2206	2211	rBV10	5684	13205	0.22%	0.026%
44	17.022	2328	2335	2338	rBV8	6086	10801	0.18%	0.021%
45	17.122	2347	2352	2356	rBV3	9963	18992	0.32%	0.038%
46	17.339	2382	2389	2397	rBV	1780883	2529618	42.93%	5.025%
47	17.439	2399	2406	2418	rBV2	3317826	4836235	82.08%	9.607%
48	18.022	2501	2505	2509	rVB4	21697	27064	0.46%	0.054%
49	18.110	2518	2520	2524	rVB5	6113	6684	0.11%	0.013%
50	18.233	2536	2541	2546	rBV	109153	146520	2.49%	0.291%
51	19.251	2710	2714	2718	rBV	51493	66546	1.13%	0.132%
52	19.316	2721	2725	2729	rBV	50870	69736	1.18%	0.139%
53	19.463	2747	2750	2755	rBV4	58965	78734	1.34%	0.156%
54	19.674	2779	2786	2794	rBV	4229965	5849627	99.28%	11.620%
55	21.145	3033	3036	3044	rBV4	99349	128528	2.18%	0.255%
56	21.427	3079	3084	3090	rBV	2102074	2884054	48.95%	5.729%
57	23.715	3466	3473	3485	rVB2	2866216	5891839	100.00%	11.704%
58	23.874	3494	3500	3511	rVB2	1437484	3016942	51.21%	5.993%




Sum of corrected areas: 50342222

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007521.D
Acq On : 20 Oct 2021 10:40
Operator : CG/JU
Sample : M4246-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT53

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

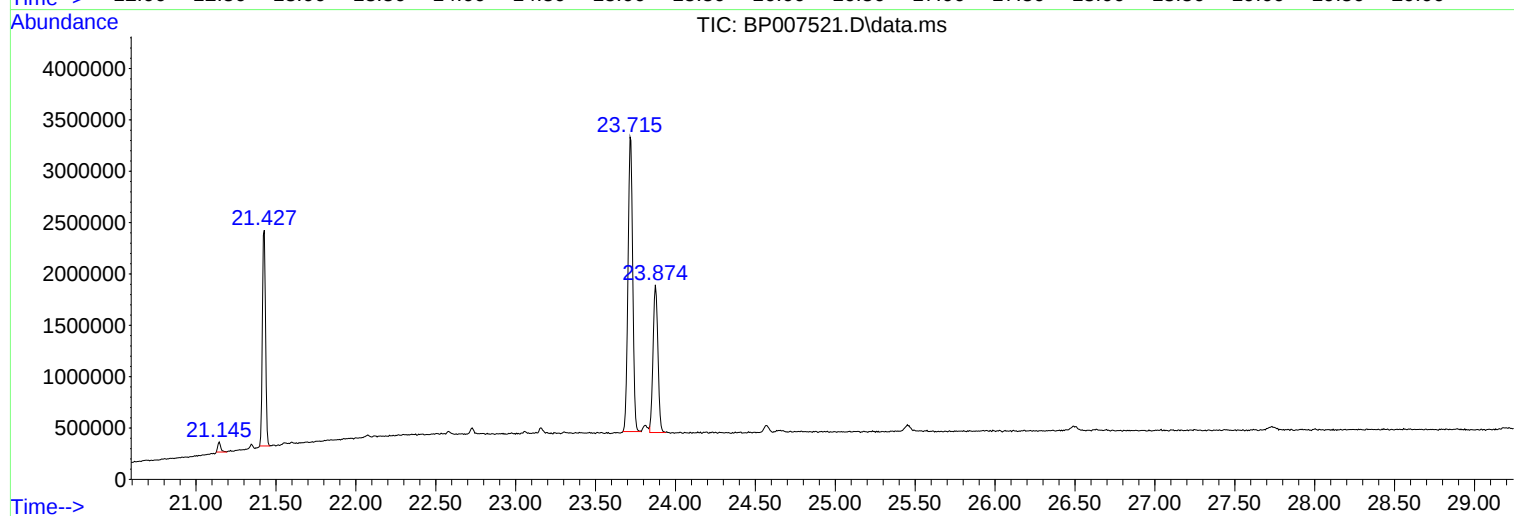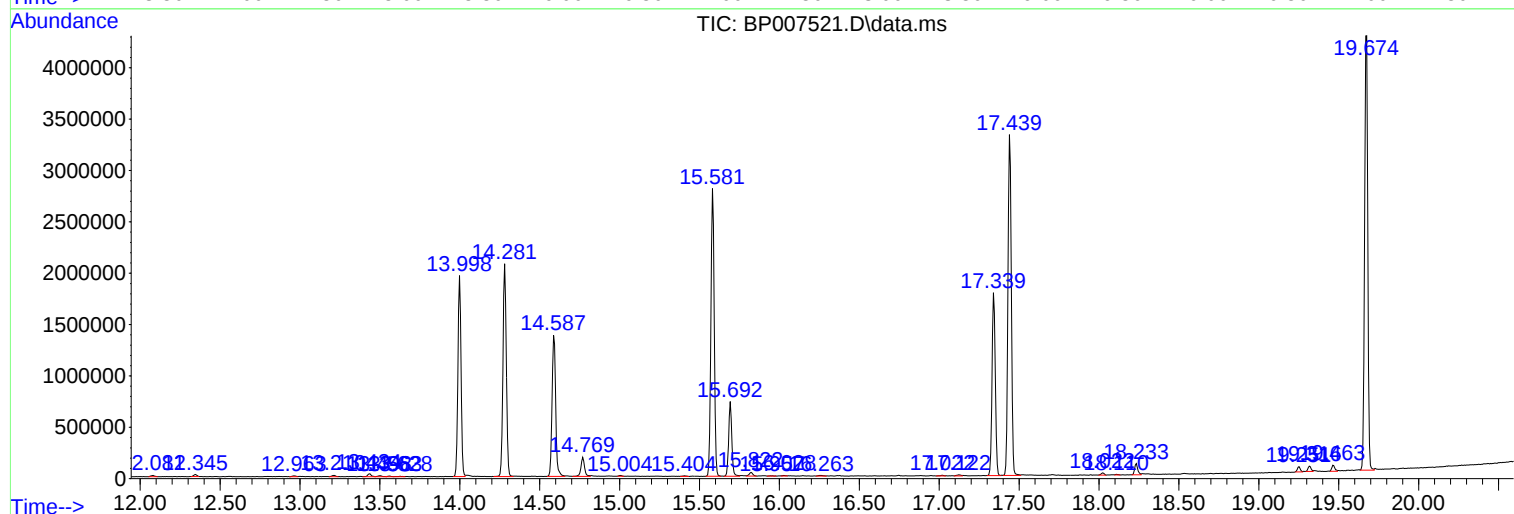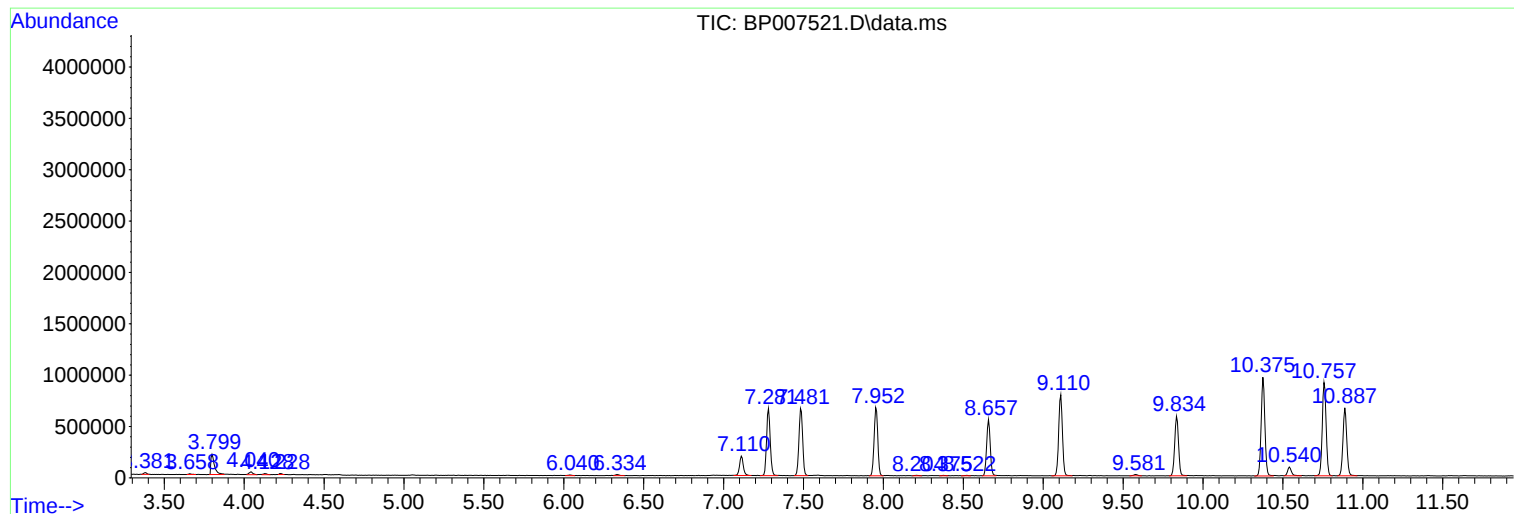

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007521.D
Acq On : 20 Oct 2021 10:40
Operator : CG/JU
Sample : M4246-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT53

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007521.D
Acq On : 20 Oct 2021 10:40
Operator : CG/JU
Sample : M4246-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT53

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
