

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007531.D
 Acq On : 20 Oct 2021 16:25
 Operator : CG/JU
 Sample : M4246-10
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YAT47

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	22	rVB	42022	55839	0.99%	0.115%
2	3.664	59	64	66	rBV6	4356	5811	0.10%	0.012%
3	3.799	84	87	99	rBV	155235	247527	4.38%	0.512%
4	4.040	124	128	135	rVB	27928	43176	0.76%	0.089%
5	4.134	140	144	154	rVB	11071	19388	0.34%	0.040%
6	4.228	156	160	165	rBV4	13468	19844	0.35%	0.041%
7	5.058	297	301	305	rVB3	7117	11313	0.20%	0.023%
8	6.334	512	518	523	rBV5	9423	16973	0.30%	0.035%
9	7.110	643	650	659	rVB	194494	315318	5.58%	0.652%
10	7.281	672	679	687	rBV	605332	943382	16.69%	1.951%
11	7.481	707	713	721	rBV	621828	990798	17.52%	2.049%
12	7.952	786	793	801	rBV	642200	1005190	17.78%	2.078%
13	8.210	828	837	840	rBV10	4328	9714	0.17%	0.020%
14	8.387	861	867	871	rBV8	3682	7322	0.13%	0.015%
15	8.657	906	913	921	rBV	536354	846881	14.98%	1.751%
16	9.110	979	990	1001	rBV	727955	1206525	21.34%	2.495%
17	9.581	1062	1070	1075	rBV	31364	52966	0.94%	0.110%
18	9.834	1105	1113	1121	rBV	555278	922043	16.31%	1.906%
19	10.375	1197	1205	1216	rBV	896103	1474858	26.09%	3.050%
20	10.540	1227	1233	1245	rVB	83821	141346	2.50%	0.292%
21	10.757	1259	1270	1279	rBV	849340	1449791	25.64%	2.998%
22	10.887	1282	1292	1306	rBV	741296	1274069	22.53%	2.634%
23	11.410	1376	1381	1387	rVB10	2869	6522	0.12%	0.013%
24	12.075	1489	1494	1500	rBV	28290	43255	0.77%	0.089%
25	12.340	1534	1539	1547	rVB2	19641	35247	0.62%	0.073%
26	12.557	1574	1576	1584	rVB8	3541	7397	0.13%	0.015%
27	12.957	1640	1644	1648	rBV4	8600	14063	0.25%	0.029%
28	13.210	1682	1687	1692	rBV3	15385	21875	0.39%	0.045%
29	13.434	1720	1725	1731	rVB	21245	30900	0.55%	0.064%
30	13.498	1733	1736	1740	rVV6	4939	5762	0.10%	0.012%
31	13.557	1743	1746	1750	rVB6	5077	6598	0.12%	0.014%
32	13.634	1754	1759	1763	rVB7	5126	7298	0.13%	0.015%
33	13.998	1812	1821	1827	rBV	1680879	2339912	41.39%	4.838%
34	14.281	1858	1869	1877	rBV	1967875	2853415	50.47%	5.900%
35	14.586	1914	1921	1932	rBV	1357834	2046707	36.20%	4.232%
36	14.769	1943	1952	1959	rBV	195789	293701	5.19%	0.607%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007531.D
 Acq On : 20 Oct 2021 16:25
 Operator : CG/JU
 Sample : M4246-10
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YAT47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

37	15.004	1988	1992	1998	rBV8	8981	12573	0.22%	0.026%
38	15.234	2027	2031	2038	rVB10	3822	6928	0.12%	0.014%
39	15.404	2053	2060	2064	rBV9	10272	20307	0.36%	0.042%
40	15.457	2066	2069	2074	rVB6	4589	6826	0.12%	0.014%
41	15.581	2083	2090	2102	rBV	2513620	3714439	65.70%	7.680%
42	15.692	2102	2109	2123	rVV	661961	947333	16.76%	1.959%
43	15.822	2126	2131	2137	rVB2	33212	49929	0.88%	0.103%
44	16.028	2162	2166	2168	rBV5	4697	6785	0.12%	0.014%
45	16.051	2168	2170	2176	rVB5	8241	10836	0.19%	0.022%
46	16.145	2182	2186	2187	rBV4	5960	6411	0.11%	0.013%
47	16.257	2201	2205	2208	rBV5	5650	9184	0.16%	0.019%
48	16.369	2220	2224	2233	rVB5	5728	10992	0.19%	0.023%
49	16.739	2284	2287	2292	rVB7	6126	8147	0.14%	0.017%
50	17.122	2348	2352	2359	rBV4	7051	11660	0.21%	0.024%
51	17.339	2382	2389	2398	rVV	1733423	2404920	42.54%	4.973%
52	17.439	2399	2406	2416	rVV	3177644	4593089	81.24%	9.497%
53	17.516	2417	2419	2425	rVV7	7204	11770	0.21%	0.024%
54	17.580	2425	2430	2434	rVB5	10655	17554	0.31%	0.036%
55	17.710	2448	2452	2455	rBV2	7093	9854	0.17%	0.020%
56	17.775	2461	2463	2468	rVB6	6102	7065	0.12%	0.015%
57	18.022	2501	2505	2510	rVV	48847	67594	1.20%	0.140%
58	18.110	2517	2520	2525	rBV6	6969	7835	0.14%	0.016%
59	18.233	2537	2541	2548	rBV	108997	151286	2.68%	0.313%
60	19.133	2691	2694	2703	rBV	30080	42275	0.75%	0.087%
61	19.251	2709	2714	2719	rBV2	47772	74621	1.32%	0.154%
62	19.316	2721	2725	2729	rBV	55169	77848	1.38%	0.161%
63	19.463	2747	2750	2754	rBV3	46263	51826	0.92%	0.107%
64	19.669	2779	2785	2796	rBV	4014190	5587579	98.83%	11.553%
65	21.145	3032	3036	3040	rBV	156352	225832	3.99%	0.467%
66	21.427	3078	3084	3091	rBV	2111544	2852944	50.46%	5.899%
67	23.715	3466	3473	3483	rVB2	2726700	5653975	100.00%	11.691%
68	23.874	3494	3500	3511	rVB2	1410503	2930732	51.83%	6.060%




Sum of corrected areas: 48363675

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007531.D
Acq On : 20 Oct 2021 16:25
Operator : CG/JU
Sample : M4246-10
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT47

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

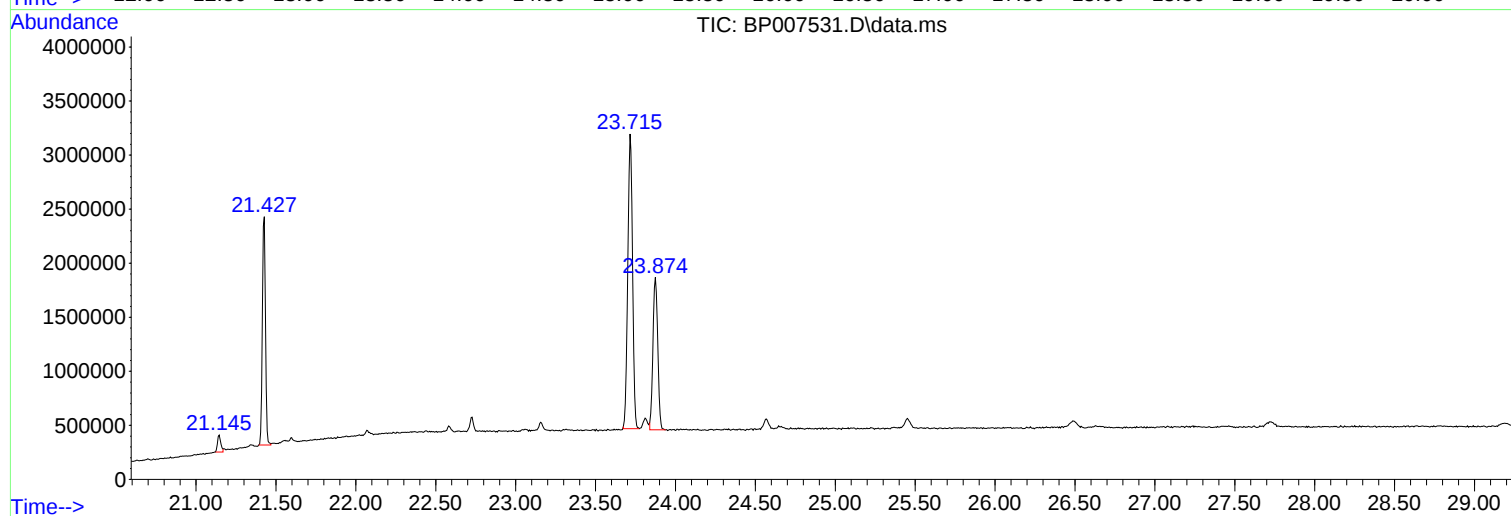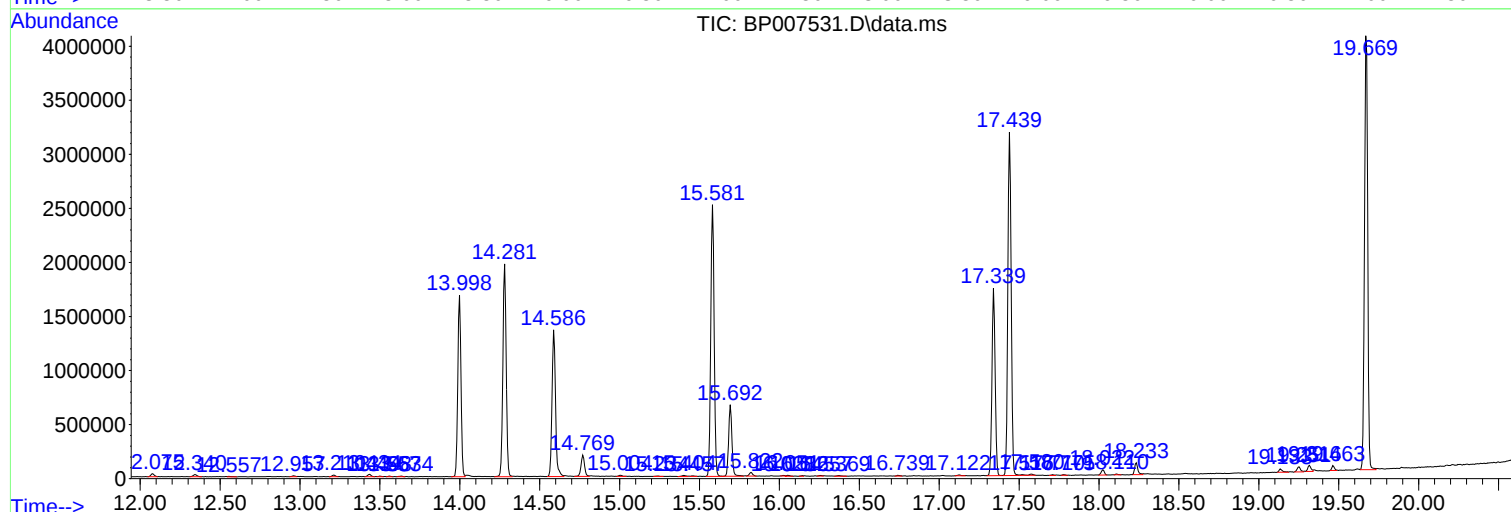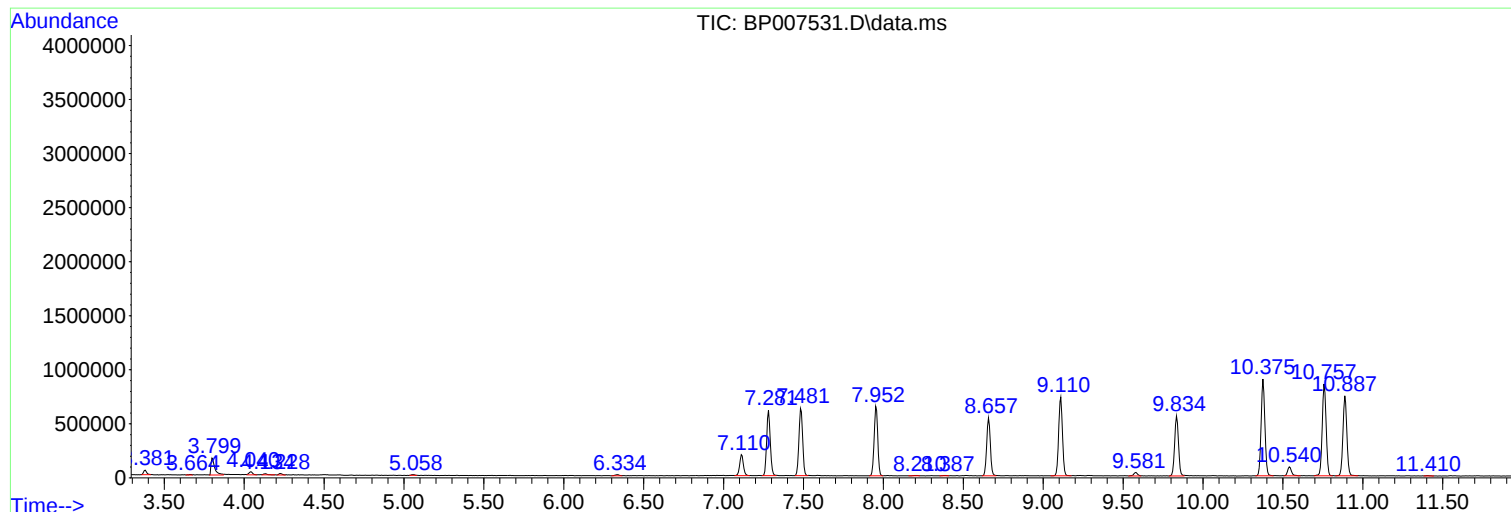

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007531.D
Acq On : 20 Oct 2021 16:25
Operator : CG/JU
Sample : M4246-10
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT47

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007531.D
Acq On : 20 Oct 2021 16:25
Operator : CG/JU
Sample : M4246-10
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YAT47

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
