

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
 Data File : BP007536.D
 Acq On : 20 Oct 2021 19:16
 Operator : CG/JU
 Sample : PB140016BL
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK016

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	22	rVB	48351	67602	1.48%	0.137%
2	3.793	82	86	108	rBV	683353	1038413	22.68%	2.103%
3	4.128	139	143	149	rBV	11079	16009	0.35%	0.032%
4	5.128	310	313	317	rVB6	4038	5607	0.12%	0.011%
5	7.111	643	650	660	rBV	799601	1240312	27.09%	2.512%
6	7.281	672	679	689	rVB	595925	972308	21.23%	1.969%
7	7.481	707	713	722	rVB	797499	1252239	27.35%	2.536%
8	7.952	785	793	801	rBV	739879	1157425	25.28%	2.344%
9	8.658	904	913	924	rBV	951403	1559804	34.07%	3.159%
10	9.105	981	989	1001	rBV	713560	1184846	25.88%	2.399%
11	9.834	1102	1113	1128	rBV	546922	924320	20.19%	1.872%
12	10.375	1197	1205	1216	rBV	953785	1583509	34.58%	3.207%
13	10.757	1261	1270	1279	rVV	963701	1653673	36.12%	3.349%
14	10.887	1283	1292	1302	rBV	922462	1565151	34.18%	3.169%
15	11.551	1401	1405	1411	rBV9	4942	7523	0.16%	0.015%
16	12.346	1533	1540	1546	rVV2	18031	31595	0.69%	0.064%
17	13.563	1740	1747	1752	rBV7	4653	7528	0.16%	0.015%
18	13.998	1814	1821	1835	rBV	1608153	2278193	49.75%	4.613%
19	14.281	1859	1869	1880	rBV	1854177	2764222	60.37%	5.597%
20	14.587	1913	1921	1932	rBV	1587186	2261678	49.39%	4.580%
21	14.769	1945	1952	1967	rBV	797664	1133303	24.75%	2.295%
22	15.581	2083	2090	2099	rBV	2384212	3448051	75.30%	6.982%
23	15.692	2102	2109	2122	rVV	505009	725002	15.83%	1.468%
24	15.822	2126	2131	2135	rVB2	27331	40941	0.89%	0.083%
25	16.145	2181	2186	2192	rVB10	4175	7768	0.17%	0.016%
26	16.257	2200	2205	2208	rBV6	5428	9295	0.20%	0.019%
27	17.016	2330	2334	2339	rVB8	5499	9201	0.20%	0.019%
28	17.122	2347	2352	2359	rBV3	9951	20065	0.44%	0.041%
29	17.339	2382	2389	2397	rBV	1913686	2761770	60.32%	5.593%
30	17.439	2399	2406	2422	rVV	2720558	3847035	84.02%	7.790%
31	17.575	2424	2429	2435	rVB8	7604	16724	0.37%	0.034%
32	17.710	2449	2452	2456	rBV4	5020	6566	0.14%	0.013%
33	18.016	2500	2504	2508	rBV7	12490	18050	0.39%	0.037%
34	18.228	2538	2540	2546	rVB6	7378	11136	0.24%	0.023%
35	19.245	2710	2713	2719	rVB2	36031	47746	1.04%	0.097%
36	19.316	2721	2725	2732	rVV	39973	56869	1.24%	0.115%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007536.D
Acq On : 20 Oct 2021 19:16
Operator : CG/JU
Sample : PB140016BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Title : SVOA CALIBRATION

37	19.669	2779	2785	2795	rBV	3378490	4578875	100.00%	9.272%
38	21.422	3078	3083	3091	rBV	2287767	3203019	69.95%	6.486%
39	23.716	3466	3473	3483	rVB2	2284307	4559809	99.58%	9.234%
40	23.874	3493	3500	3512	rVB2	1565533	3309989	72.29%	6.703%




Sum of corrected areas: 49383171

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007536.D
Acq On : 20 Oct 2021 19:16
Operator : CG/JU
Sample : PB140016BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

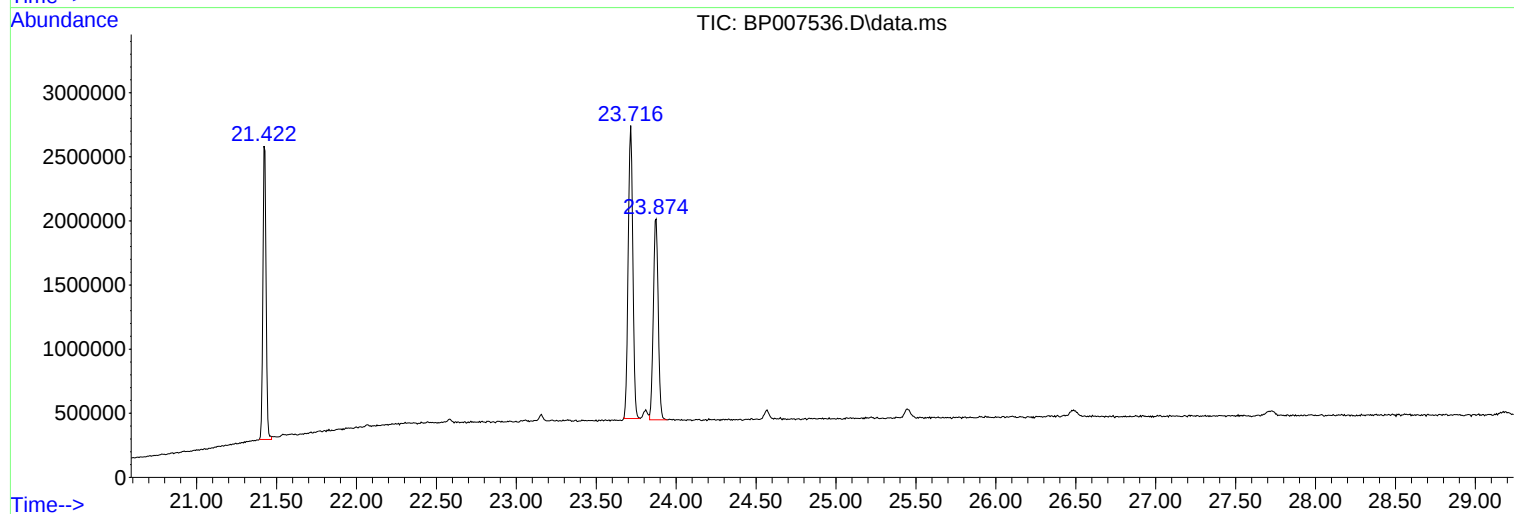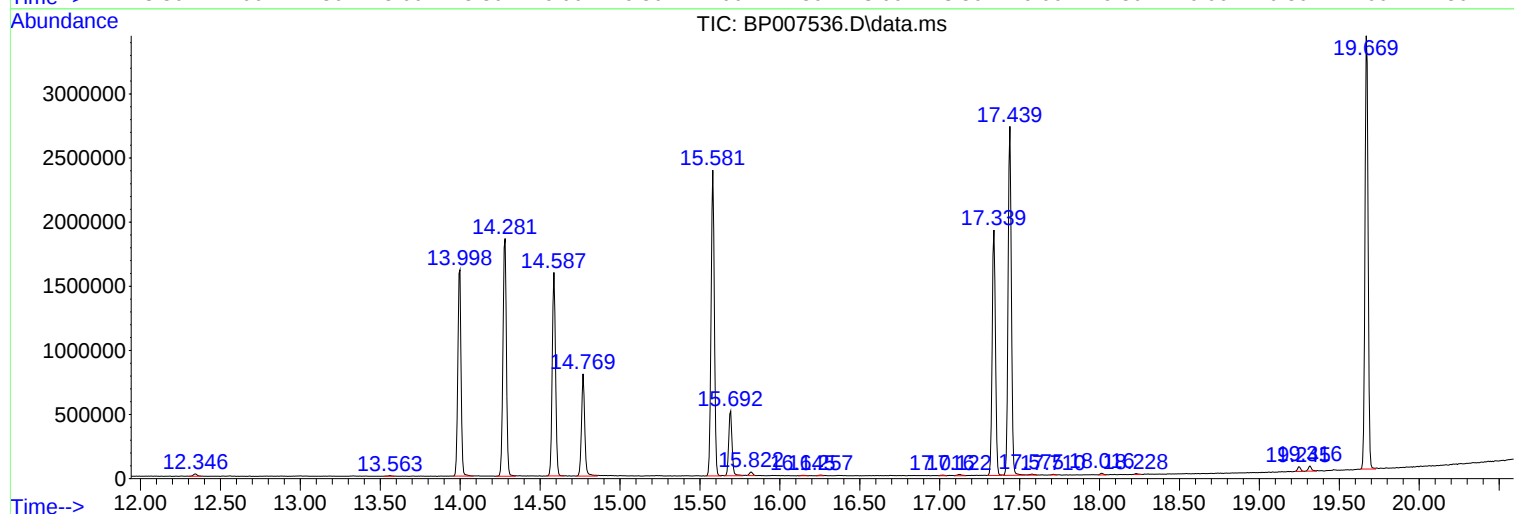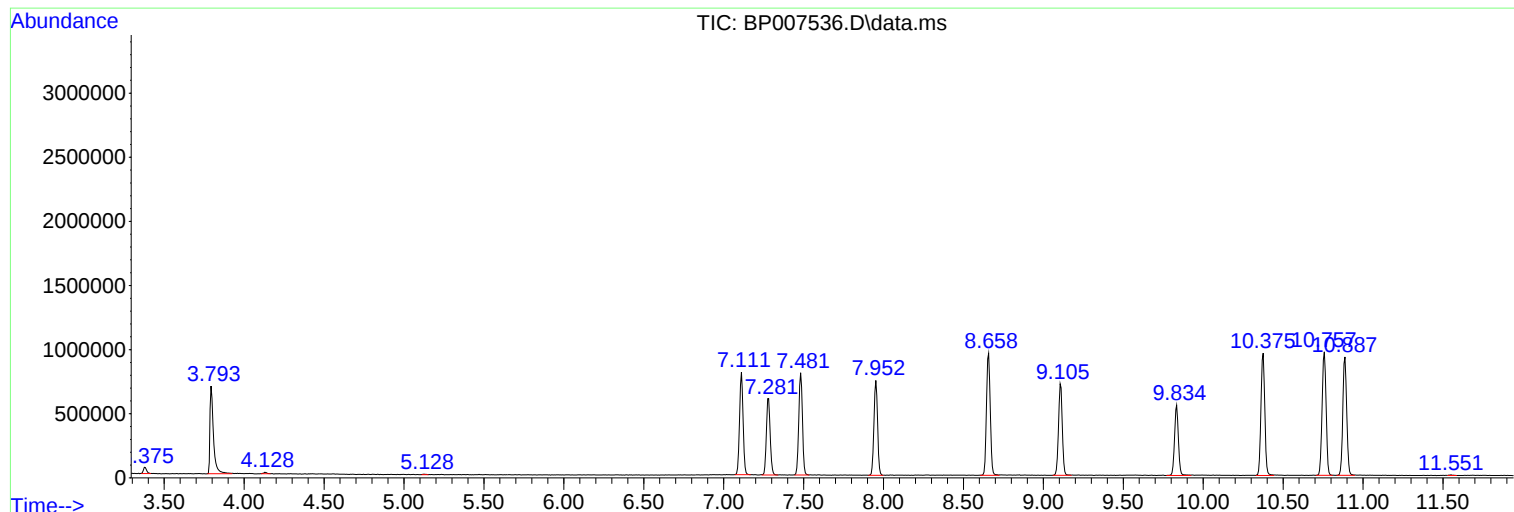

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007536.D
Acq On : 20 Oct 2021 19:16
Operator : CG/JU
Sample : PB140016BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101821\
Data File : BP007536.D
Acq On : 20 Oct 2021 19:16
Operator : CG/JU
Sample : PB140016BL
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
