

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101824\
 Data File : BP022454.D
 Acq On : 18 Oct 2024 10:46
 Operator : RC/JU
 Sample : PB164170BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	47	rVB	22050	32314	0.89%	0.089%
2	3.605	101	105	125	rBV	277143	486092	13.32%	1.343%
3	3.928	155	160	165	rVB	6640	10160	0.28%	0.028%
4	6.852	651	657	673	rVB	397995	628303	17.22%	1.735%
5	7.004	676	683	691	rBV	300589	456354	12.51%	1.260%
6	7.204	708	717	730	rBV	376968	621227	17.03%	1.716%
7	7.657	787	794	804	rBV	466934	733930	20.12%	2.027%
8	8.363	905	914	928	rBV2	489543	849857	23.30%	2.347%
9	8.804	979	989	1000	rBV	428192	675782	18.52%	1.866%
10	9.216	1054	1059	1065	rVB3	4313	7403	0.20%	0.020%
11	9.516	1102	1110	1121	rBV	351235	608171	16.67%	1.680%
12	10.051	1194	1201	1220	rBV	527915	935810	25.65%	2.585%
13	10.416	1255	1263	1274	rBV	635571	1075037	29.47%	2.969%
14	10.557	1279	1287	1301	rBV	512519	917757	25.16%	2.535%
15	11.687	1474	1479	1484	rBV6	4167	6320	0.17%	0.017%
16	12.016	1528	1535	1542	rVB4	7500	15883	0.44%	0.044%
17	13.686	1810	1819	1832	rBV	1273169	1712843	46.95%	4.731%
18	13.792	1832	1837	1842	rVB8	2135	4331	0.12%	0.012%
19	13.969	1859	1867	1878	rBV	1139396	1804628	49.47%	4.984%
20	14.281	1912	1920	1929	rBV	1314813	1829763	50.16%	5.054%
21	14.504	1952	1958	1974	rBV	466805	815944	22.37%	2.254%
22	14.698	1988	1991	1996	rVB7	3893	6275	0.17%	0.017%
23	15.286	2083	2091	2103	rBV	1857318	2420017	66.34%	6.684%
24	15.416	2106	2113	2126	rVV	543860	813058	22.29%	2.246%
25	15.528	2129	2132	2138	rVB4	7675	13428	0.37%	0.037%
26	16.863	2355	2359	2365	rVB6	3177	5070	0.14%	0.014%
27	17.069	2387	2394	2405	rBV	1796007	2586822	70.91%	7.145%
28	17.180	2405	2413	2425	rVV2	1766338	2853090	78.21%	7.880%
29	17.469	2458	2462	2465	rBV6	2589	3949	0.11%	0.011%
30	17.663	2492	2495	2501	rVB6	3164	5085	0.14%	0.014%
31	18.016	2551	2555	2563	rBV9	7604	14447	0.40%	0.040%
32	18.369	2609	2615	2616	rBV6	3632	6591	0.18%	0.018%
33	19.110	2736	2741	2745	rBV2	27010	37966	1.04%	0.105%
34	19.180	2749	2753	2757	rVV	25984	36814	1.01%	0.102%
35	19.557	2811	2817	2825	rBV	2667810	3648108	100.00%	10.076%
36	21.510	3143	3149	3164	rVB2	2026833	3204713	87.85%	8.851%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101824\
Data File : BP022454.D
Acq On : 18 Oct 2024 10:46
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.545	3656	3665	3679	rVB	1530152	3411184	93.51%	9.421%
38	24.768	3694	3703	3717	rVB	993040	2912060	79.82%	8.043%




Sum of corrected areas: 36206586

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101824\
Data File : BP022454.D
Acq On : 18 Oct 2024 10:46
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

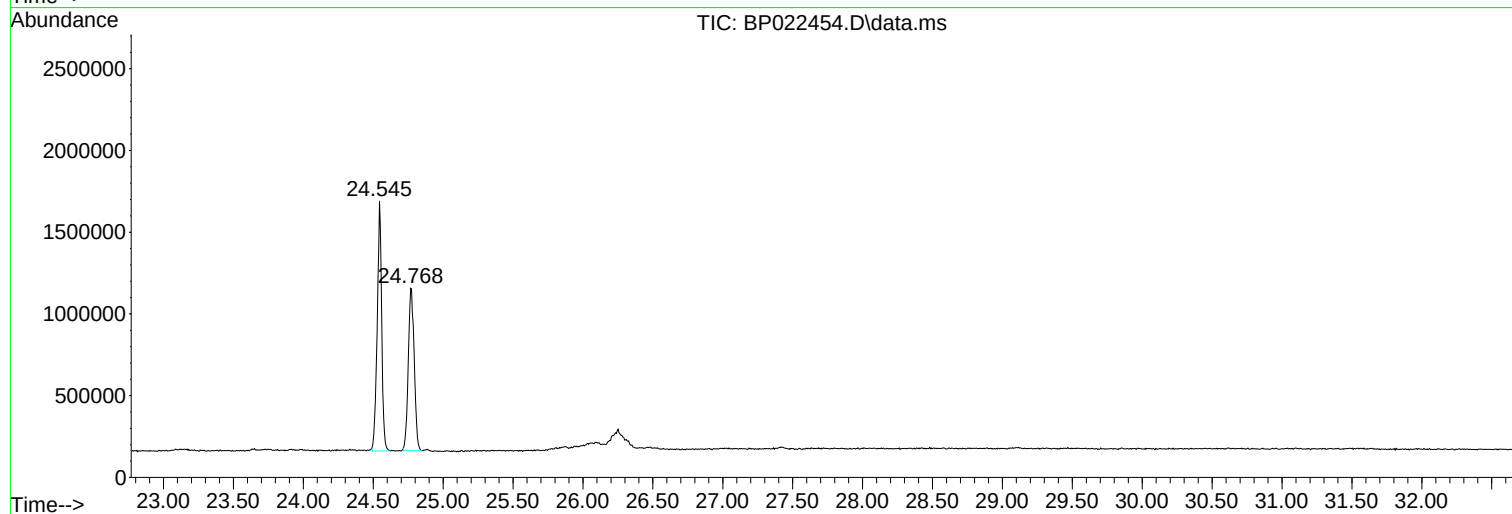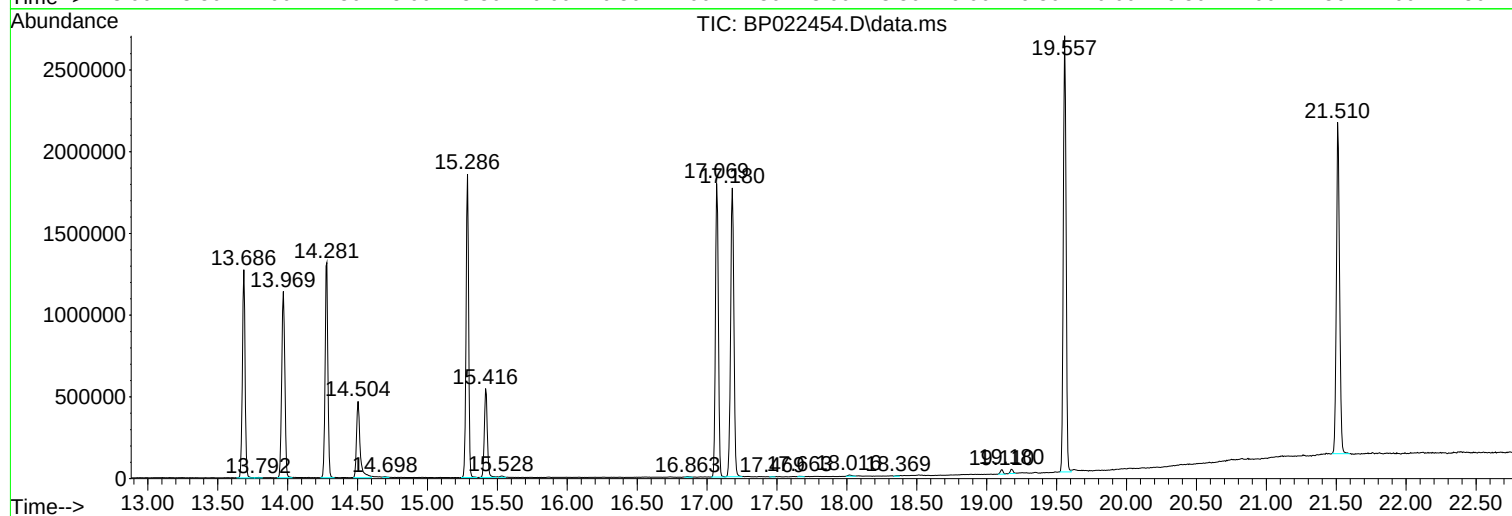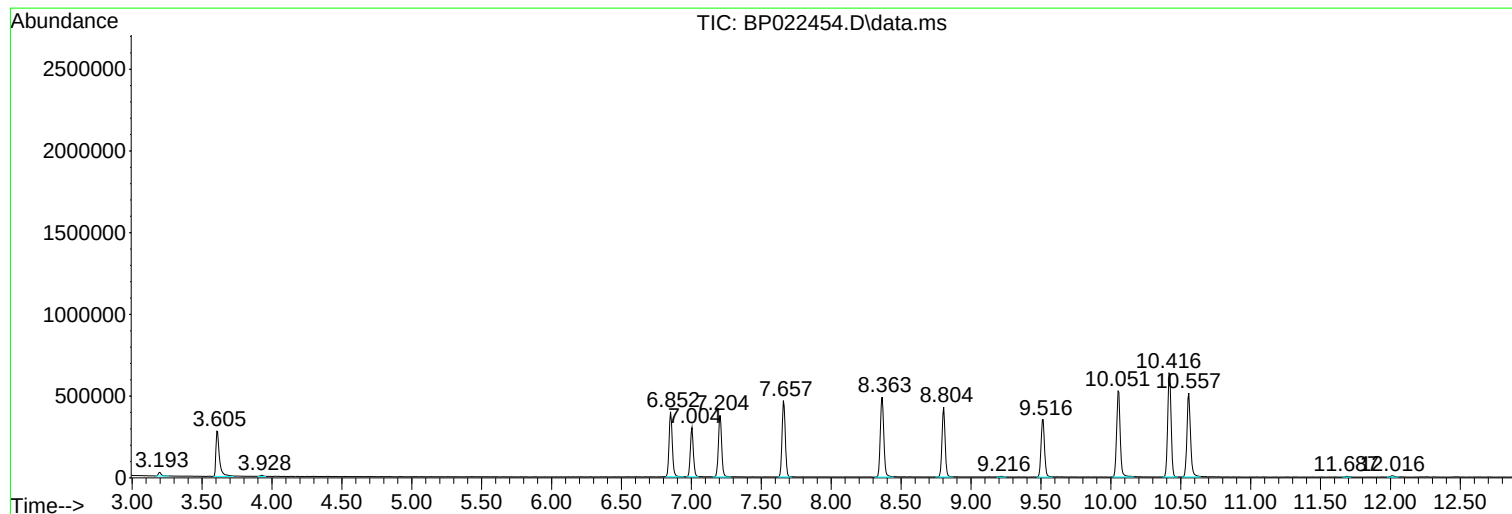

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101824\
Data File : BP022454.D
Acq On : 18 Oct 2024 10:46
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101824\
Data File : BP022454.D
Acq On : 18 Oct 2024 10:46
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc