

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000905.D
 Acq On : 19 Oct 2019 11:26
 Operator : JU
 Sample : PB124015TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB29

Quant Time: Oct 19 20:27:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	124184	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	473013	20.00	ng/ul	-0.01
36) Acenaphthene-d10	9.79	164	267761	20.00	ng/ul	-0.01
62) Phenanthrene-d10	11.29	188	512169	20.00	ng/ul	-0.01
78) Chrysene-d12	13.96	240	491060	20.00	ng/ul	-0.02
86) Perylene-d12	15.43	264	560553	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.41	96	211	0.07	ng/uL	0.02
5) Phenol-d5	6.38	99	336072	35.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	166743	34.82	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	292878	36.29	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	272830	37.28	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	137115	38.13	ng/ul	-0.01
22) 2-Nitrophenol-d4	7.63	143	154654	40.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	266038	36.30	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	359553	44.12	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	721750	38.51	ng/ul	-0.01
47) Acenaphthylene-d8	9.63	160	855225	37.09	ng/ul	0.00
52) 4-Nitrophenol-d4	9.91	143	95159	32.96	ng/ul	0.00
58) Fluorene-d10	10.31	176	598318	37.31	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	10.39	200	57188	23.45	ng/ul	-0.01
71) Anthracene-d10	11.34	188	891514	37.58	ng/ul	-0.01
79) Pyrene-d10	12.73	212	978889	35.25	ng/ul	-0.01
90) Benzo(a)pyrene-d12	15.35	264	1072489	38.75	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	7.13	70	5672	1.165	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000905.D
Acq On : 19 Oct 2019 11:26
Operator : JU
Sample : PB124015TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB29

Quant Time: Oct 19 20:27:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

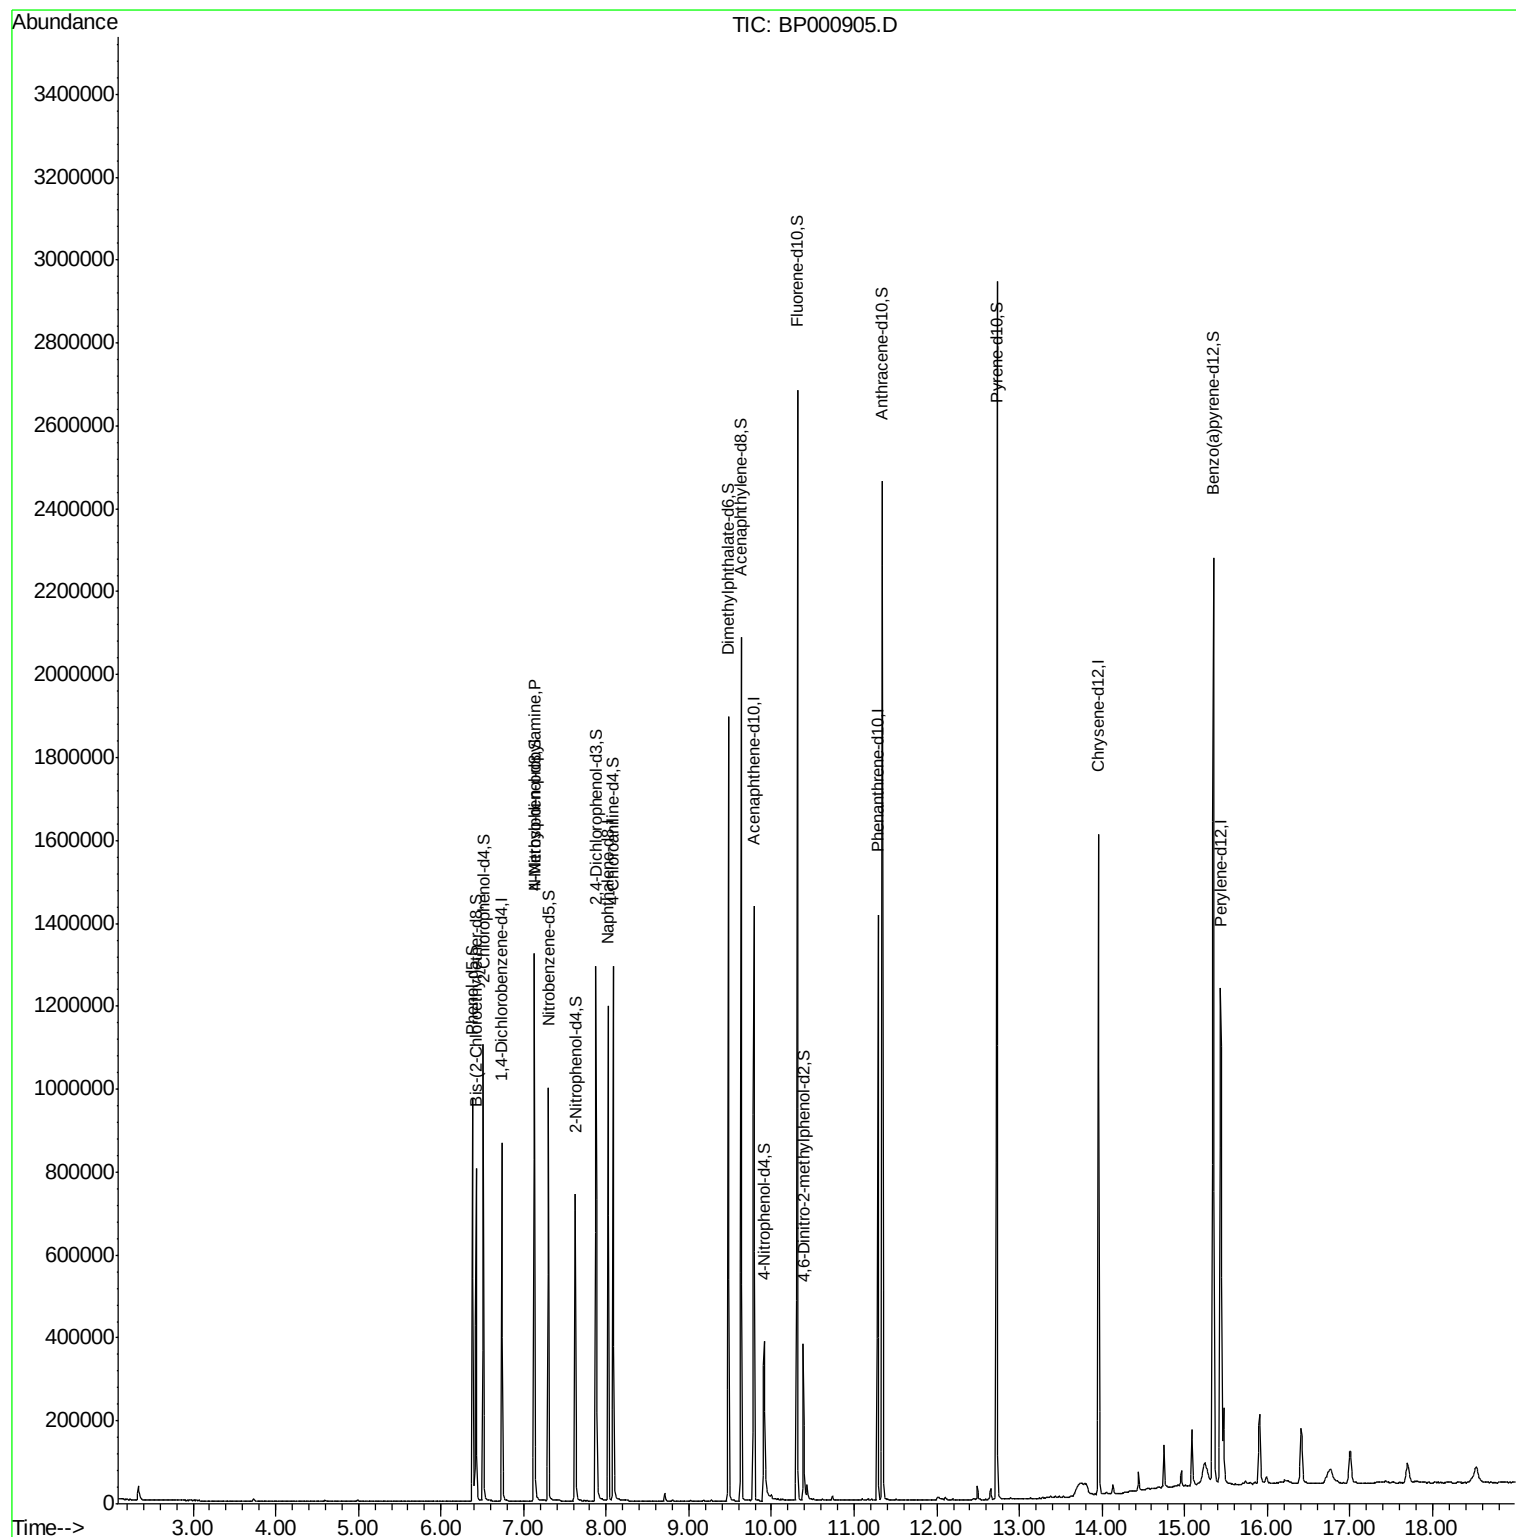

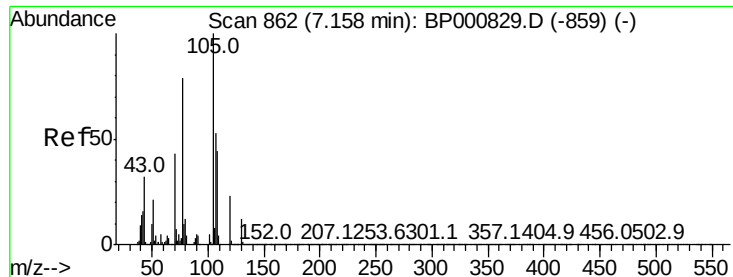

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.165 ng/ul
 RT: 7.13 min Scan# 857
 Delta R.T. -0.03 min
 Lab File: BP000905.D
 Acq: 19 Oct 2019 11:26

Instrument :
 BNA_P
 ClientSampleId :
 SLEB29

Tot Ion: 70 Resp: 5672
 Ion Ratio Lower Upper
 70 100
 42 286.8 33.5 50.3#
 101 0.3 9.6 14.4#
 130 0.1 21.8 32.8#

