

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000908.D
 Acq On : 19 Oct 2019 12:38
 Operator : JU
 Sample : K5321-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AA4

Quant Time: Oct 19 20:27:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	121912	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	469906	20.00	ng/ul	-0.01
36) Acenaphthene-d10	9.79	164	269395	20.00	ng/ul	-0.01
62) Phenanthrene-d10	11.28	188	518278	20.00	ng/ul	-0.02
78) Chrysene-d12	13.96	240	486739	20.00	ng/ul	-0.02
86) Perylene-d12	15.43	264	546952	20.00	ng/ul	-0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.34	96	15868	5.40	ng/uL	-0.05
5) Phenol-d5	6.39	99	60700	6.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	147784	31.43	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	212709	26.85	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	124450	17.32	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	125780	35.21	ng/ul	-0.01
22) 2-Nitrophenol-d4	7.63	143	142644	37.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	230740	31.70	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	27015	3.34	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	711494	37.73	ng/ul	-0.01
47) Acenaphthylene-d8	9.63	160	833158	35.91	ng/ul	0.00
52) 4-Nitrophenol-d4	9.92	143	17415	6.00	ng/ul	0.00
58) Fluorene-d10	10.31	176	608291	37.70	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	10.39	200	66921	27.11	ng/ul	-0.01
71) Anthracene-d10	11.34	188	933114	38.87	ng/ul	-0.01
79) Pyrene-d10	12.73	212	1013620	36.83	ng/ul	-0.01
90) Benzo(a)pyrene-d12	15.35	264	1080462	40.01	ng/ul	-0.02


Target Compounds					Ovalue	
45) Dimethylphthalate	9.50	163	49032	2.609	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000908.D
Acq On : 19 Oct 2019 12:38
Operator : JU
Sample : K5321-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AA4

Quant Time: Oct 19 20:27:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

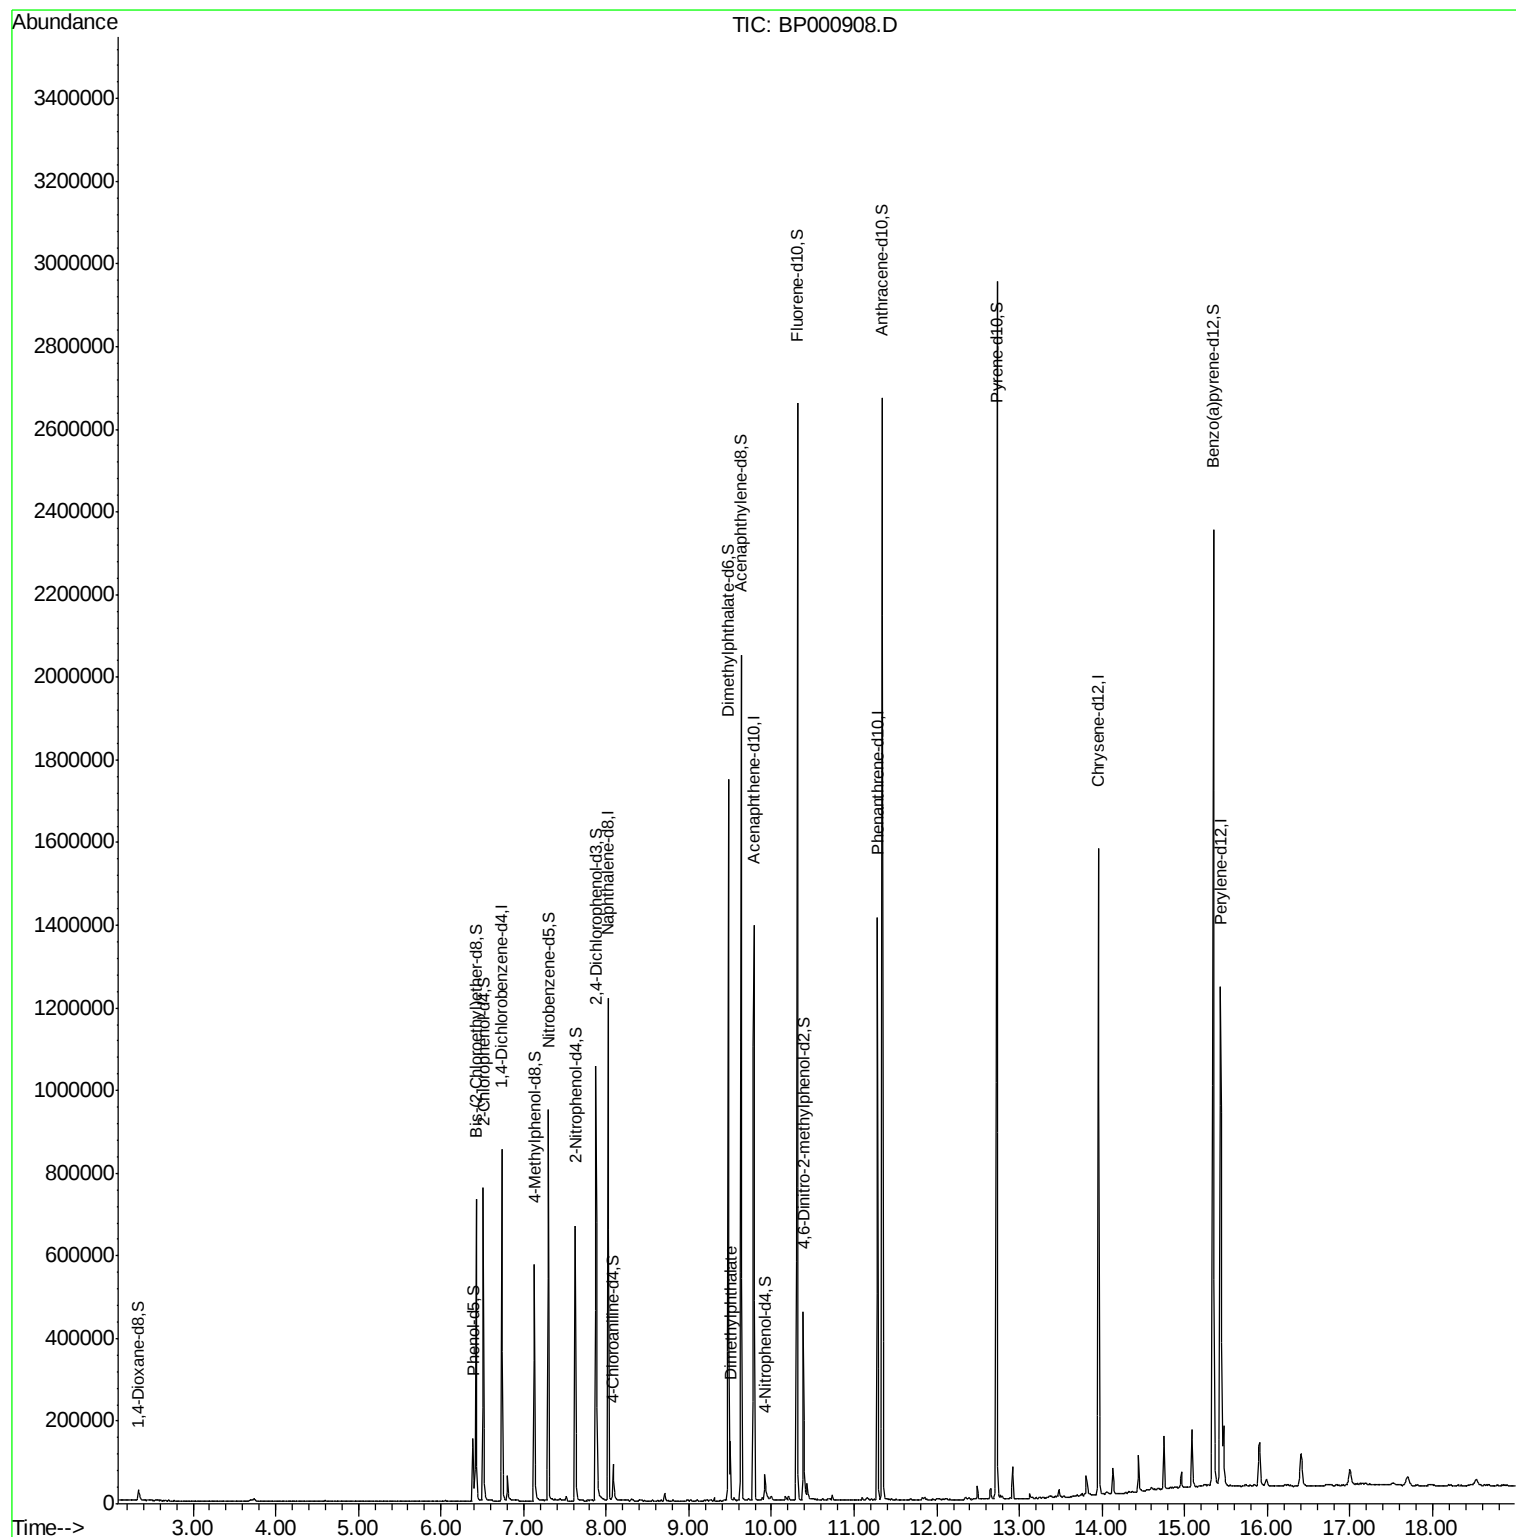

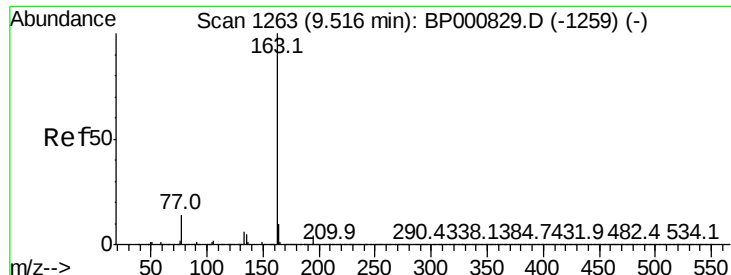

#45

Dimethylphthalate

Concen: 2.609 ng/ul

RT: 9.50 min Scan# 1260

Delta R.T. -0.02 min

Lab File: BP000908.D

Acq: 19 Oct 2019 12:38

Instrument :

BNA_P

ClientSampleId :

E0AA4


Tot Ion:163 Resp: 49032

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 10.3 8.1 12.1

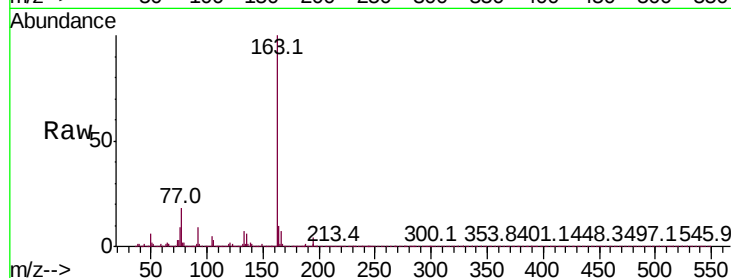

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

