

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000912.D
 Acq On : 19 Oct 2019 14:15
 Operator : JU
 Sample : K5321-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB1

Quant Time: Oct 19 20:28:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	145313	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	544717	20.00	ng/ul	-0.01
36) Acenaphthene-d10	9.79	164	304383	20.00	ng/ul	-0.01
62) Phenanthrene-d10	11.28	188	572832	20.00	ng/ul	-0.02
78) Chrysene-d12	13.96	240	527457	20.00	ng/ul	-0.02
86) Perylene-d12	15.43	264	608514	20.00	ng/ul	-0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.34	96	17338	4.95	ng/uL	-0.05
5) Phenol-d5	6.39	99	70875	6.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	150431	26.84	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	222992	23.61	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	138735	16.20	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	126269	30.49	ng/ul	-0.01
22) 2-Nitrophenol-d4	7.63	143	141720	32.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.87	165	233949	27.72	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	34290	3.65	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	676343	31.74	ng/ul	-0.01
47) Acenaphthylene-d8	9.63	160	812961	31.02	ng/ul	0.00
52) 4-Nitrophenol-d4	9.92	143	20057	6.11	ng/ul	0.00
58) Fluorene-d10	10.31	176	578183	31.71	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	10.39	200	70283	25.76	ng/ul	-0.01
71) Anthracene-d10	11.34	188	901604	33.98	ng/ul	-0.01
79) Pyrene-d10	12.73	212	969611	32.51	ng/ul	-0.01
90) Benzo(a)pyrene-d12	15.35	264	1042790	34.71	ng/ul	-0.02


Target Compounds					Ovalue	
45) Dimethylphthalate	9.50	163	168176	7.921	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000912.D
Acq On : 19 Oct 2019 14:15
Operator : JU
Sample : K5321-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB1

Quant Time: Oct 19 20:28:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

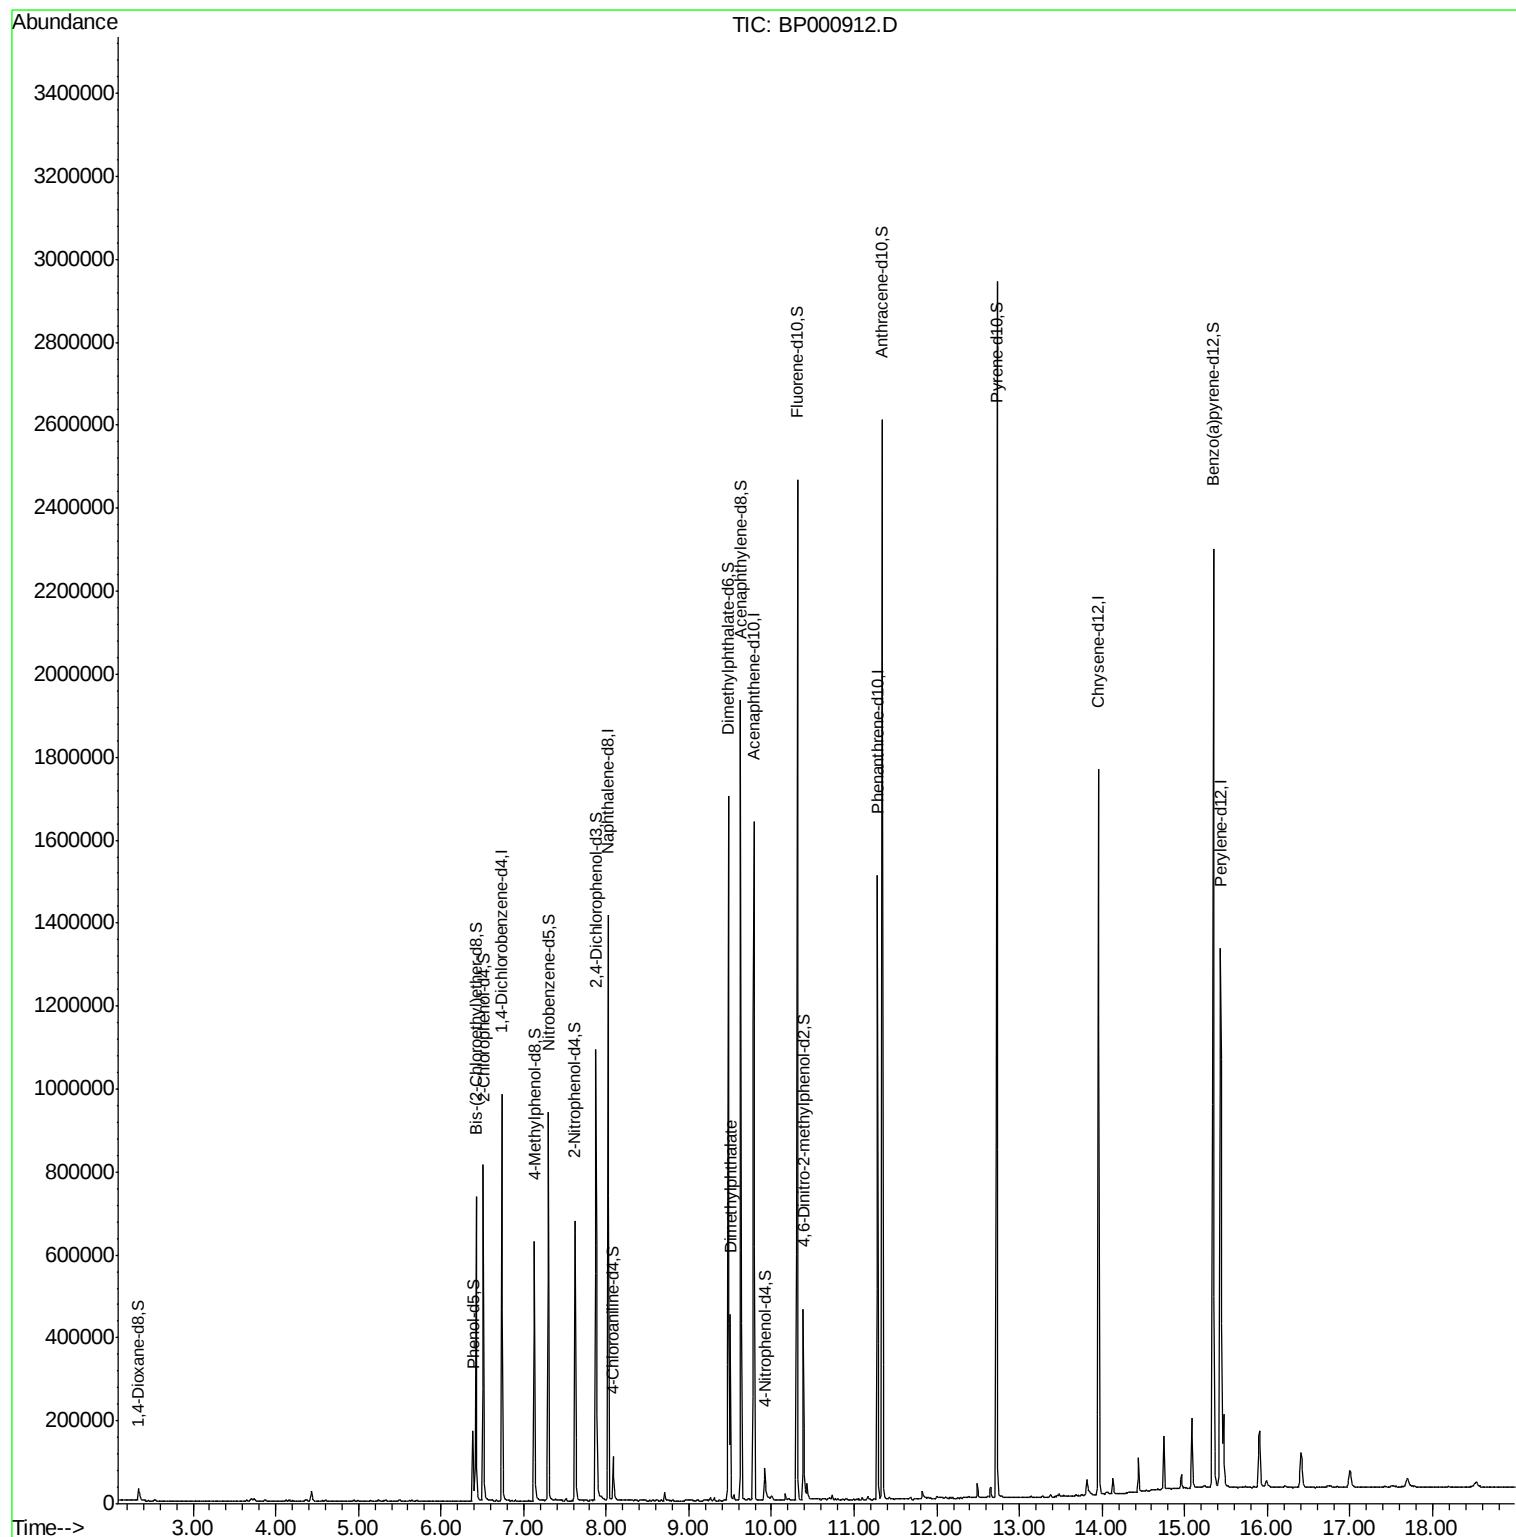

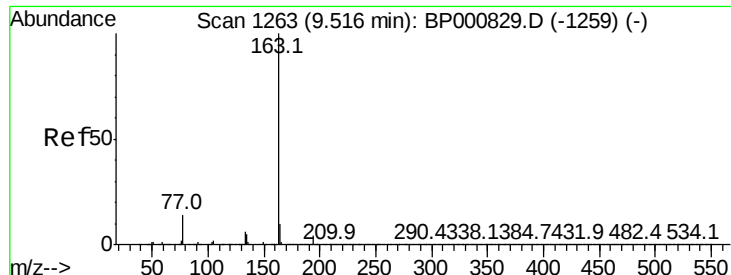

#45

Dimethylphthalate

Concen: 7.921 ng/ul

RT: 9.50 min Scan# 1260

Delta R.T. -0.02 min

Lab File: BP000912.D

Acq: 19 Oct 2019 14:15

Instrument :

BNA_P

ClientSampleId :

E0AB1


Tot Ion:163 Resp: 168176

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.1 8.1 12.1

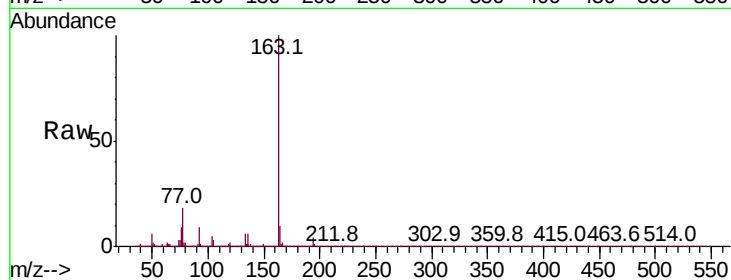

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

