

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000914.D
 Acq On : 19 Oct 2019 15:03
 Operator : JU
 Sample : K5321-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB2

Quant Time: Oct 19 20:28:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	133772	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	506203	20.00	ng/ul	-0.01
36) Acenaphthene-d10	9.79	164	282327	20.00	ng/ul	-0.01
62) Phenanthrene-d10	11.28	188	526611	20.00	ng/ul	-0.02
78) Chrysene-d12	13.96	240	489780	20.00	ng/ul	-0.02
86) Perylene-d12	15.43	264	582732	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.34	96	15972	4.95	ng/uL	-0.05
5) Phenol-d5	6.39	99	61372	5.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	134957	26.16	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	197383	22.70	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	118058	14.98	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	114460	29.75	ng/ul	-0.01
22) 2-Nitrophenol-d4	7.63	143	125930	30.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	208123	26.54	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	29972	3.44	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	603973	30.56	ng/ul	-0.01
47) Acenaphthylene-d8	9.63	160	724610	29.80	ng/ul	-0.01
52) 4-Nitrophenol-d4	9.92	143	16263	5.34	ng/ul	0.00
58) Fluorene-d10	10.31	176	519164	30.70	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	10.39	200	60880	24.28	ng/ul	-0.01
71) Anthracene-d10	11.34	188	807423	33.10	ng/ul	-0.01
79) Pyrene-d10	12.72	212	884584	31.94	ng/ul	-0.02
90) Benzo(a)pyrene-d12	15.35	264	982769	34.16	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	9.50	163	52848	2.684	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000914.D
Acq On : 19 Oct 2019 15:03
Operator : JU
Sample : K5321-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB2

Quant Time: Oct 19 20:28:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

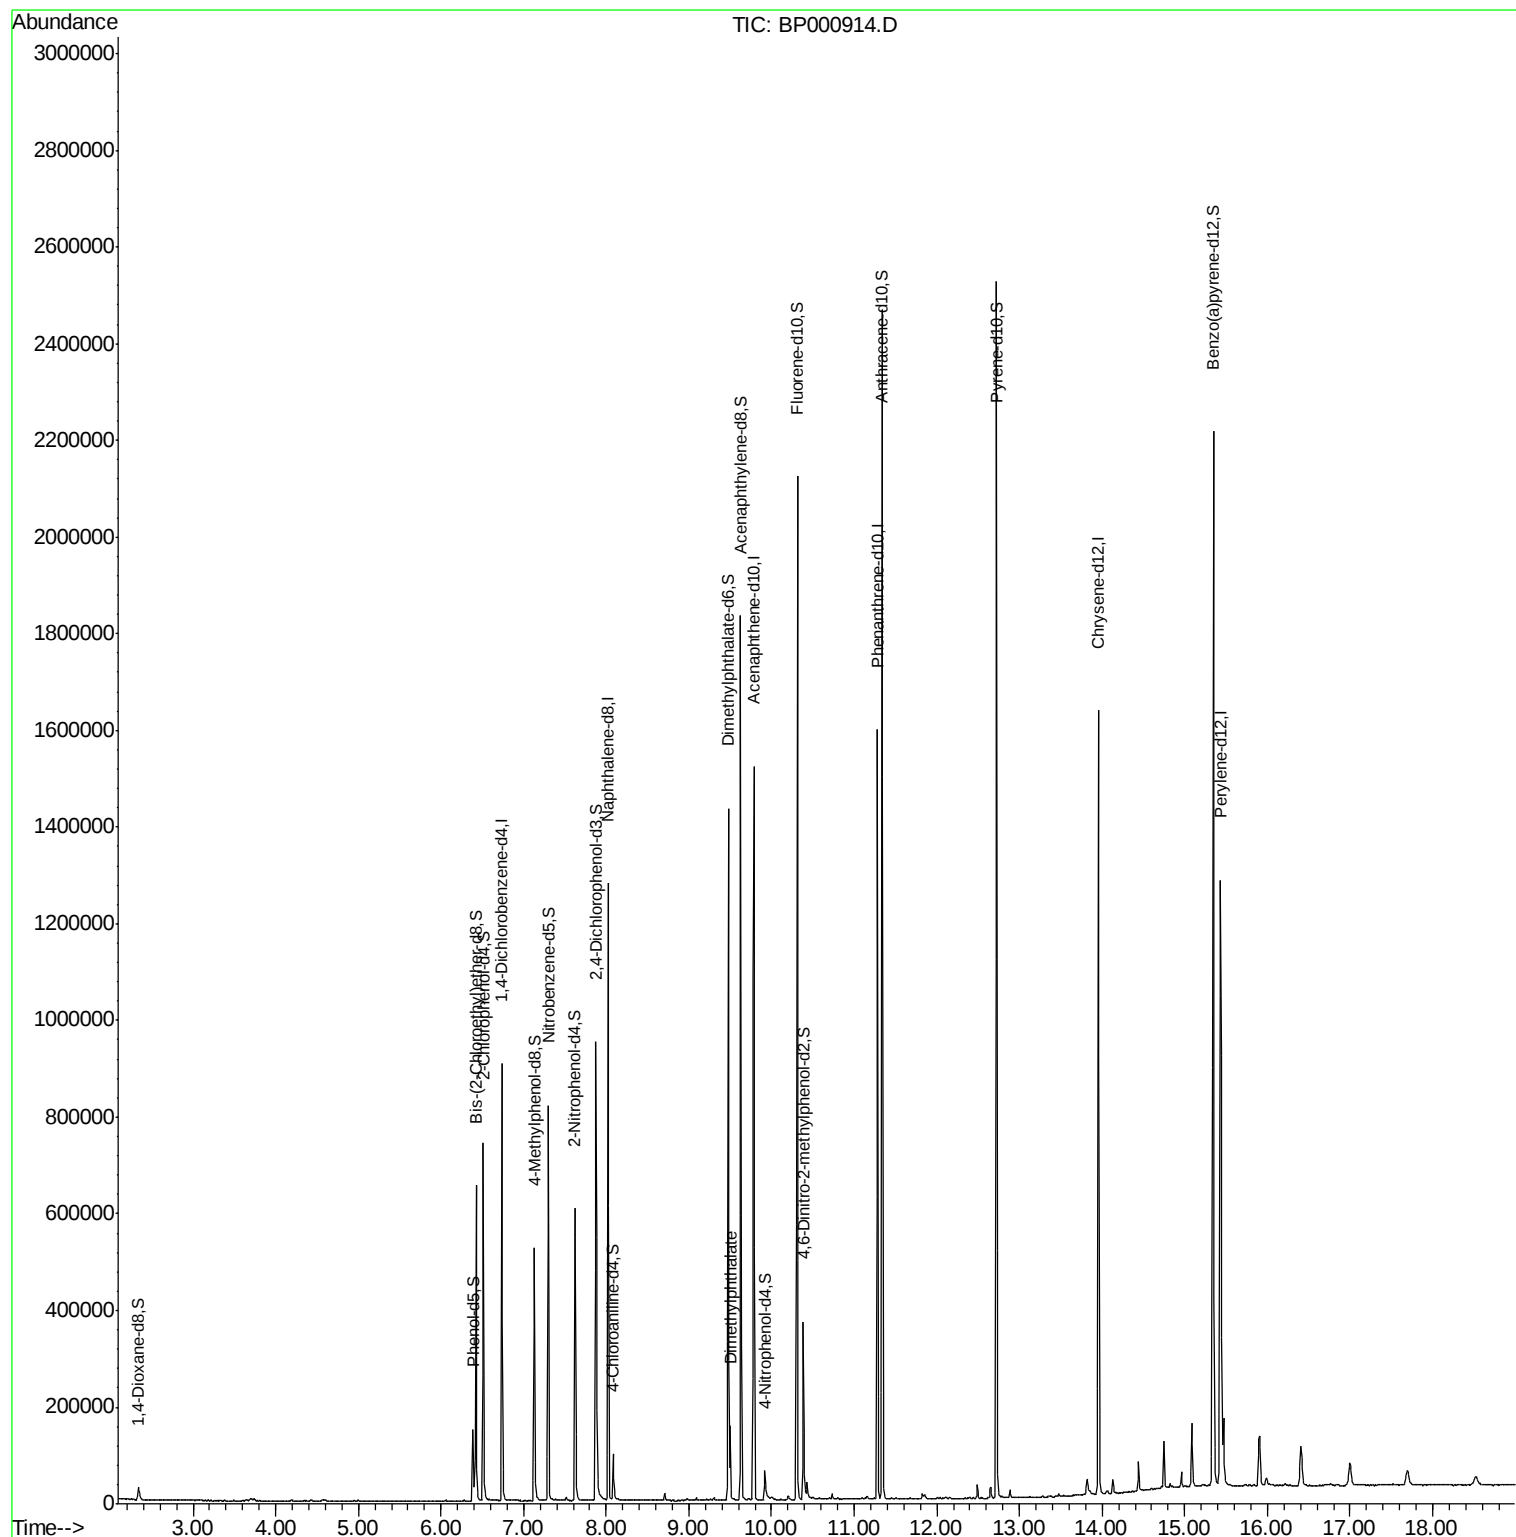

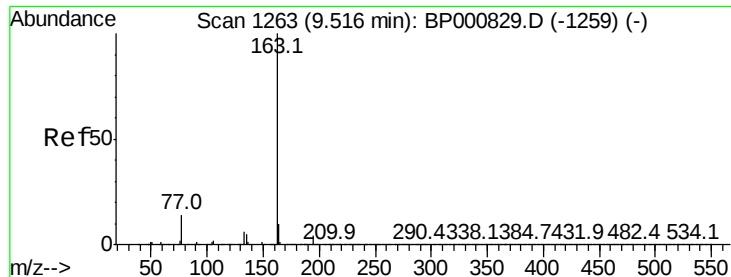

#45
 Dimethylphthalate
 Concen: 2.684 ng/ul
 RT: 9.50 min Scan# 1260
 Delta R.T. -0.02 min
 Lab File: BP000914.D
 Acq: 19 Oct 2019 15:03

Instrument :
 BNA_P
 ClientSampleId :
 E0AB2

Tot Ion:163	Resp:	52848
Ion Ratio	Lower	Upper
163	100	
194	4.2	3.3 4.9
164	10.1	8.1 12.1

