

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000915.D
 Acq On : 19 Oct 2019 15:27
 Operator : JU
 Sample : K5321-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AA2

Quant Time: Oct 19 20:28:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	145045	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	549496	20.00	ng/ul	-0.01
36) Acenaphthene-d10	9.79	164	321286	20.00	ng/ul	-0.01
62) Phenanthrene-d10	11.28	188	621987	20.00	ng/ul	-0.02
78) Chrysene-d12	13.96	240	582376	20.00	ng/ul	-0.02
86) Perylene-d12	15.43	264	618584	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.40	96	359	0.10	ng/uL	0.01
5) Phenol-d5	6.39	99	61536	5.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	141348	25.27	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	204816	21.73	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	121425	14.21	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	124043	29.70	ng/ul	-0.01
22) 2-Nitrophenol-d4	7.63	143	136394	30.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	225408	26.48	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	21404	2.26	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	742897	33.03	ng/ul	-0.01
47) Acenaphthylene-d8	9.63	160	839587	30.35	ng/ul	-0.01
52) 4-Nitrophenol-d4	9.92	143	17037	4.92	ng/ul	0.00
58) Fluorene-d10	10.31	176	615396	31.98	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	10.39	200	70776	23.89	ng/ul	-0.01
71) Anthracene-d10	11.34	188	968976	33.63	ng/ul	-0.01
79) Pyrene-d10	12.73	212	1042230	31.65	ng/ul	-0.01
90) Benzo(a)pyrene-d12	15.35	264	1040747	34.08	ng/ul	-0.02


Target Compounds				Ovalue
45) Dimethylphthalate	9.50	163	73437	3.277 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000915.D
Acq On : 19 Oct 2019 15:27
Operator : JU
Sample : K5321-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AA2

Quant Time: Oct 19 20:28:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

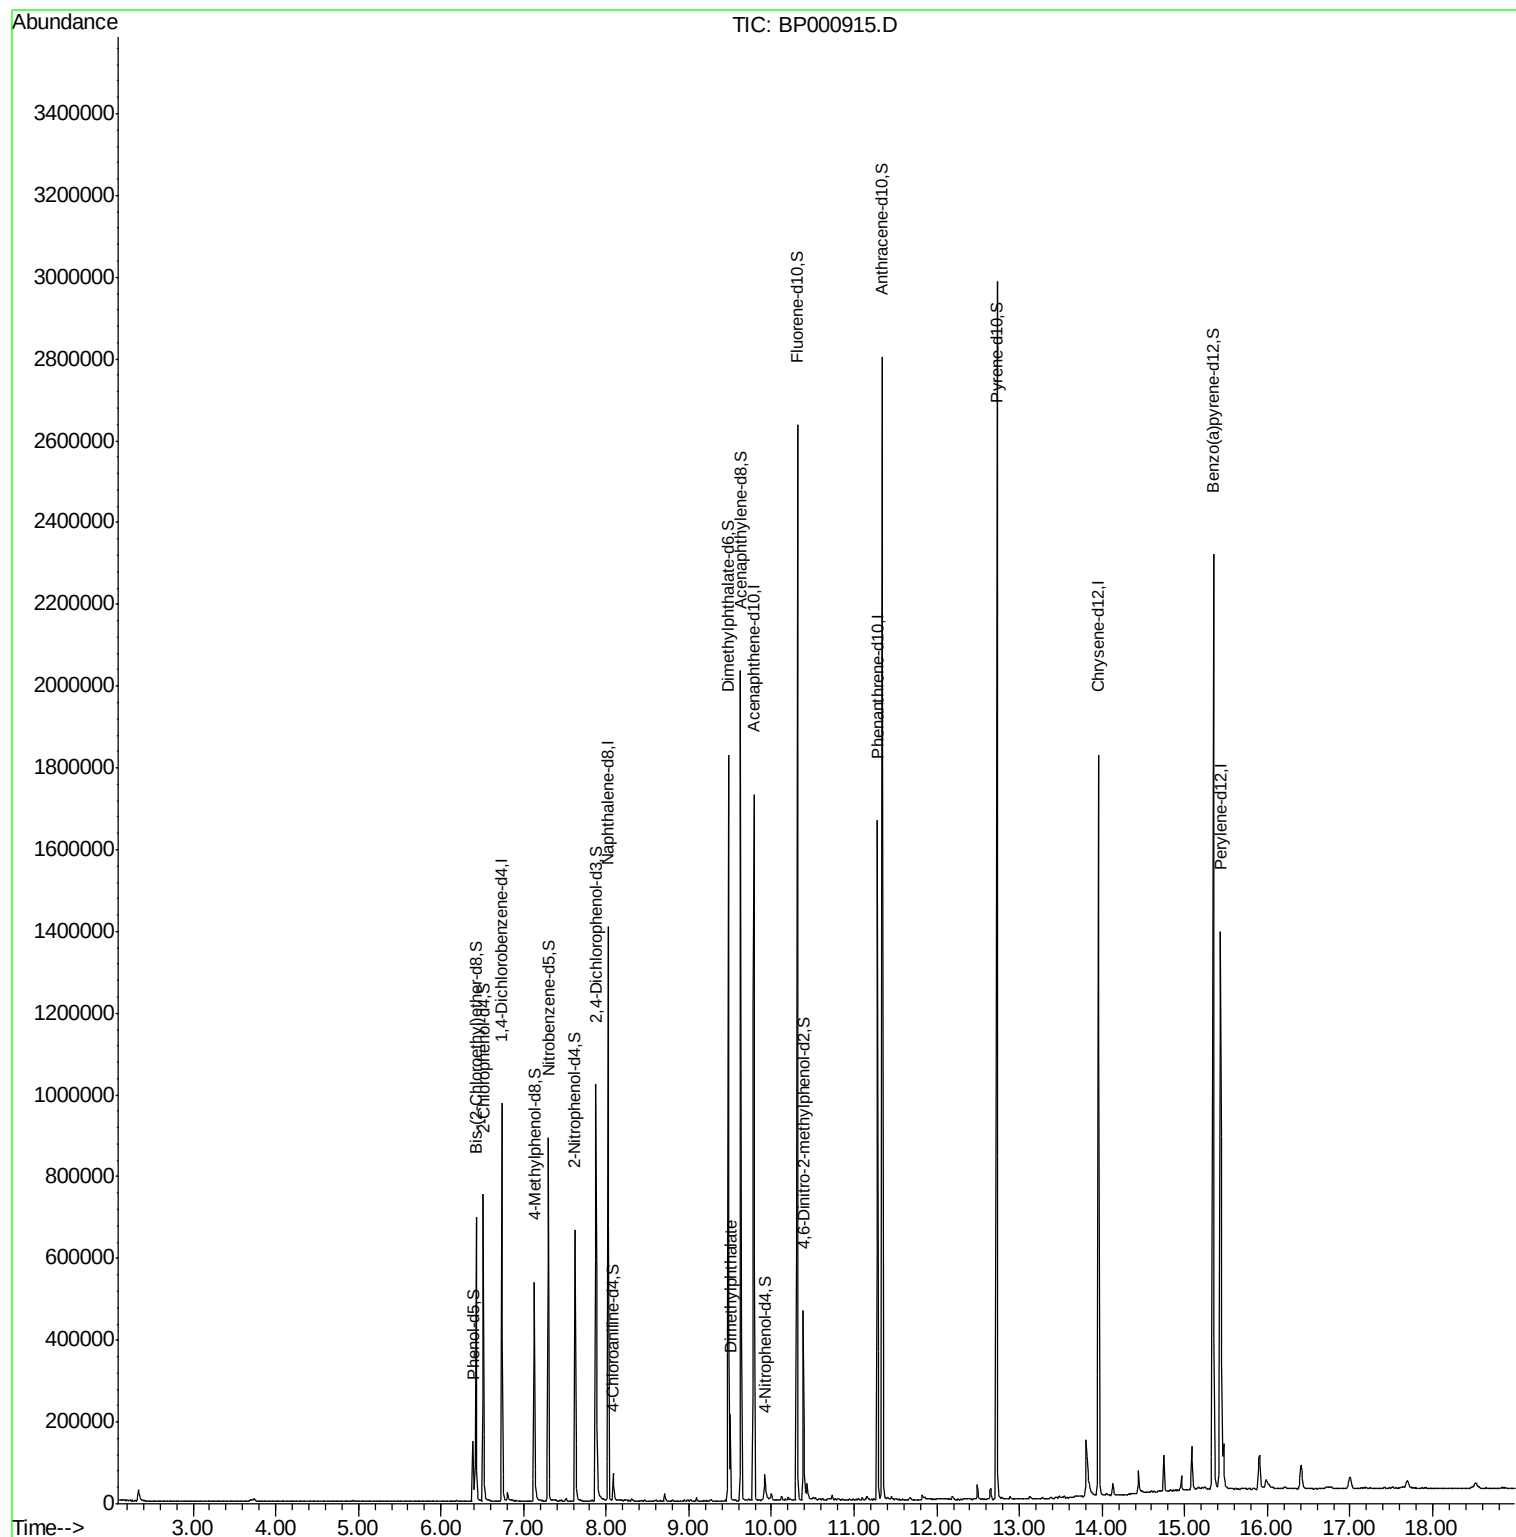

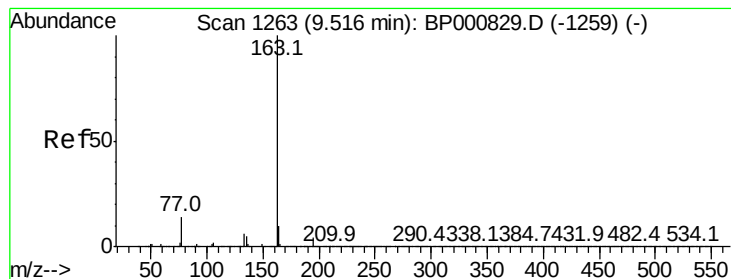

#45

Dimethylphthalate

Concen: 3.277 ng/ul

RT: 9.50 min Scan# 1260

Delta R.T. -0.02 min

Lab File: BP000915.D

Acq: 19 Oct 2019 15:27

Instrument :

BNA_P

ClientSampleId :

E0AA2

Tot Ion:163 Resp: 73437

Ion Ratio Lower Upper

163 100

194 3.9 3.3 4.9

164 10.3 8.1 12.1

