

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000925.D
 Acq On : 19 Oct 2019 19:27
 Operator : JU
 Sample : PB123974BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK74

Quant Time: Oct 19 20:30:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	133725	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	497790	20.00	ng/ul	-0.01
36) Acenaphthene-d10	9.79	164	284529	20.00	ng/ul	-0.01
62) Phenanthrene-d10	11.28	188	541673	20.00	ng/ul	-0.02
78) Chrysene-d12	13.96	240	529412	20.00	ng/ul	-0.02
86) Perylene-d12	15.43	264	609020	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.42	96	128	0.04	ng/uL	0.03
5) Phenol-d5	6.38	99	323459	31.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	159425	30.91	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	287014	33.03	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	264441	33.56	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	132450	35.00	ng/ul	-0.01
22) 2-Nitrophenol-d4	7.63	143	147858	36.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	256122	33.21	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	347036	40.46	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	693642	34.83	ng/ul	-0.01
47) Acenaphthylene-d8	9.63	160	823082	33.59	ng/ul	-0.01
52) 4-Nitrophenol-d4	9.90	143	93674	30.53	ng/ul	-0.01
58) Fluorene-d10	10.31	176	575702	33.78	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	10.39	200	67167	26.04	ng/ul	-0.01
71) Anthracene-d10	11.34	188	871961	34.75	ng/ul	-0.01
79) Pyrene-d10	12.72	212	950026	31.73	ng/ul	-0.02
90) Benzo(a)pyrene-d12	15.35	264	1031822	34.32	ng/ul	-0.02

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	7.13	70	5351	1.021	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000925.D
Acq On : 19 Oct 2019 19:27
Operator : JU
Sample : PB123974BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK74

Quant Time: Oct 19 20:30:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

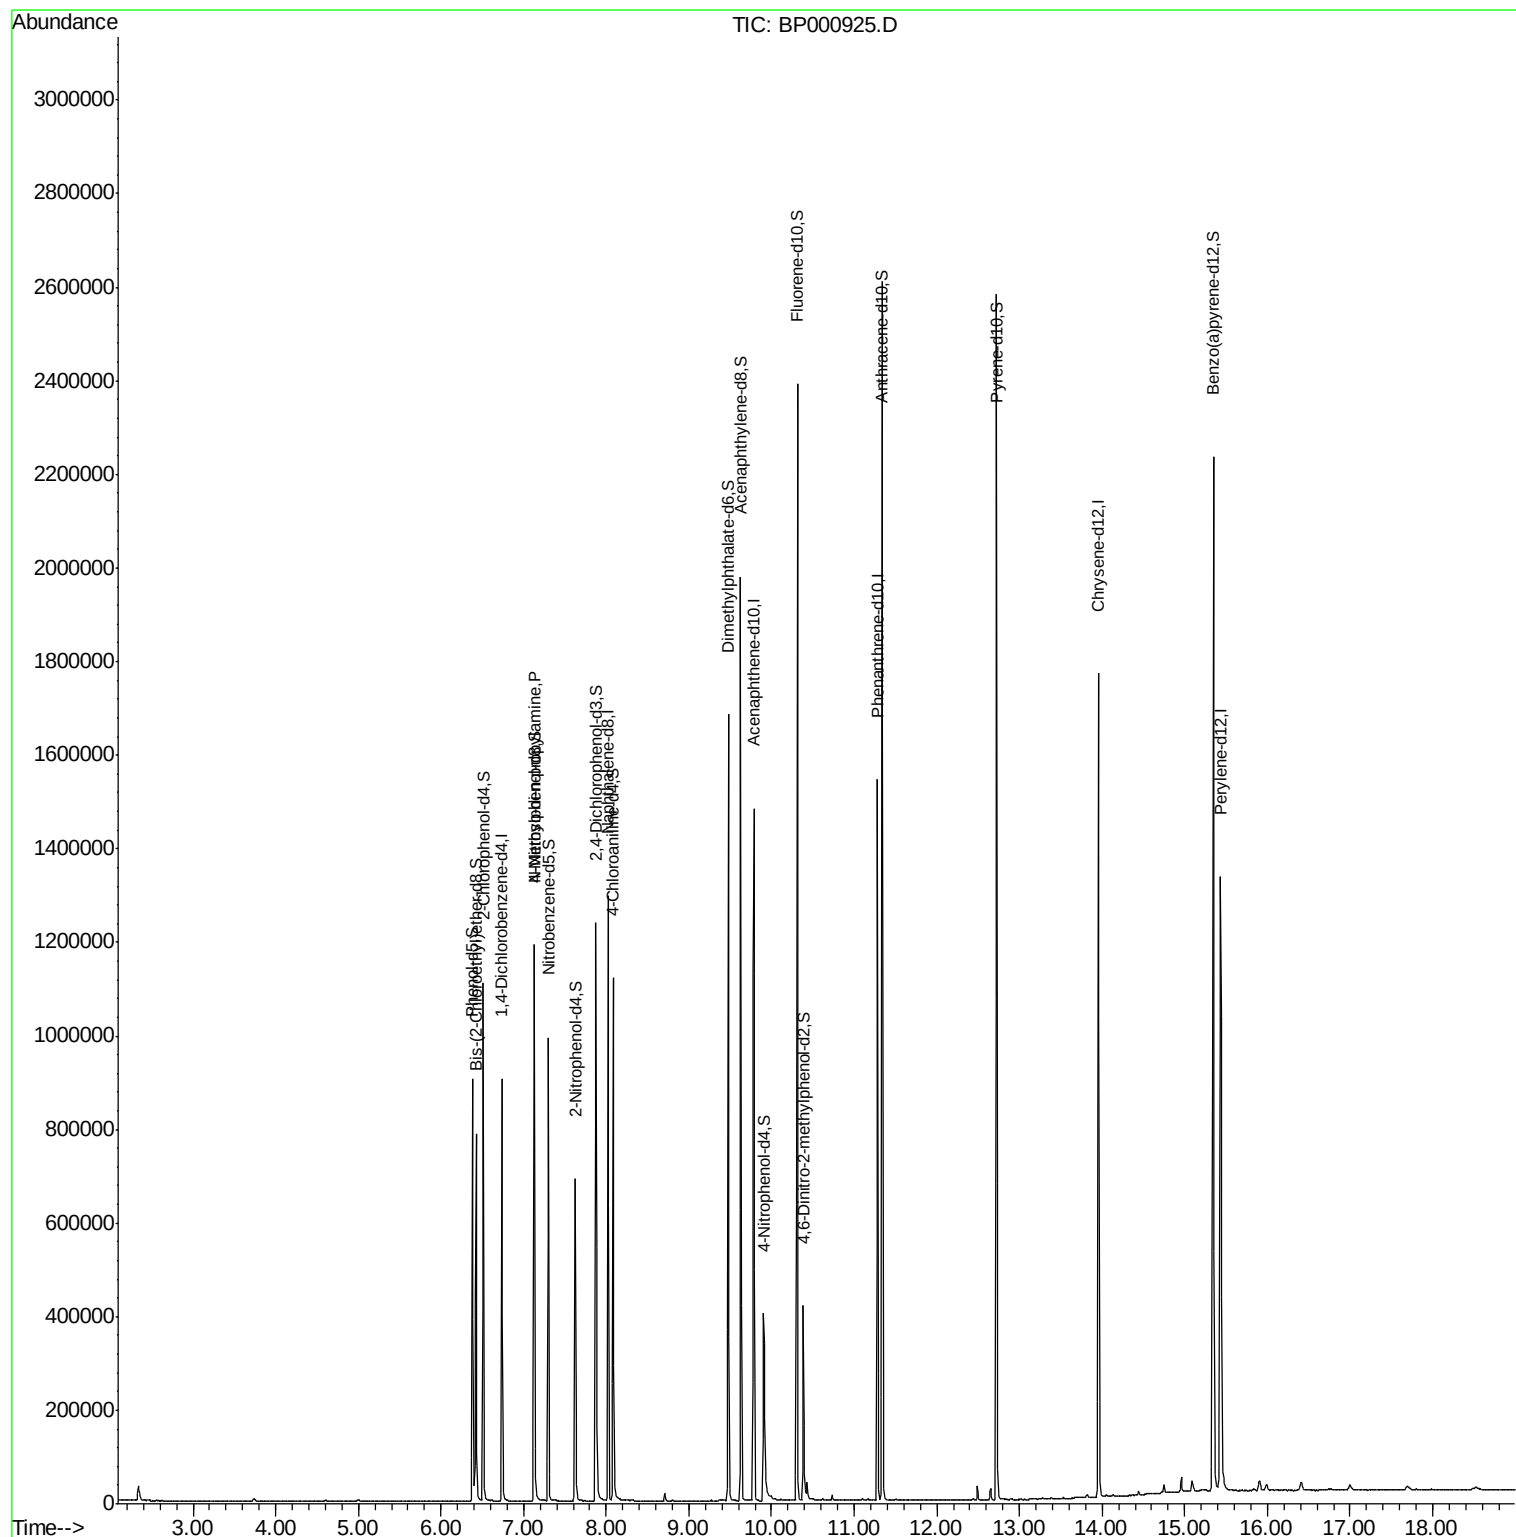

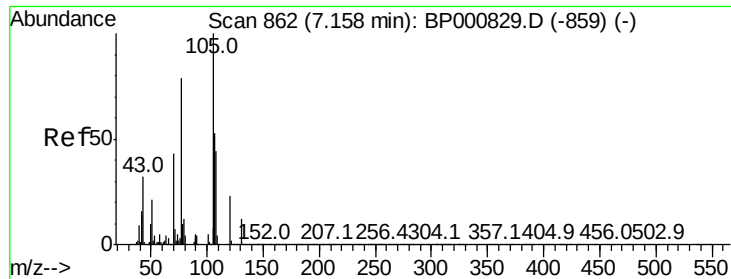

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.021 ng/ul
 RT: 7.13 min Scan# 857
 Delta R.T. -0.03 min
 Lab File: BP000925.D
 Acq: 19 Oct 2019 19:27

Instrument :
 BNA_P
 ClientSampleId :
 SBLK74

Tot Ion:	70	Resp:	5351
Ion	Ratio	Lower	Upper
70	100		
42	272.3	33.5	50.3#
101	0.5	9.6	14.4#
130	0.2	21.8	32.8#

