

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000907.D
 Acq On : 19 Oct 2019 12:14
 Operator : JU
 Sample : K5321-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB5

Quant Time: Oct 19 22:18:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 19 22:14:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	132548	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	500172	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.79	164	293359	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.28	188	559667	20.00	ng/ul	0.00
78) Chrysene-d12	13.96	240	524086	20.00	ng/ul	0.00
86) Perylene-d12	15.43	264	563321	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.34	96	18087	5.66	ng/uL	0.00
5) Phenol-d5	6.39	99	74772	7.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	153852	30.10	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	230435	26.75	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	141748	18.15	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	132969	34.97	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	147296	36.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	242478	31.29	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	26586	3.09	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	751724	36.61	ng/ul	0.00
47) Acenaphthylene-d8	9.63	160	873800	34.59	ng/ul	0.00
52) 4-Nitrophenol-d4	9.92	143	20376	6.44	ng/ul	0.00
58) Fluorene-d10	10.31	176	624065	35.52	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	67437	25.30	ng/ul	0.00
71) Anthracene-d10	11.34	188	970358	37.43	ng/ul	0.00
79) Pyrene-d10	12.73	212	1047711	35.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.35	264	1056745	38.00	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	9.50	163	58655	2.867	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000907.D
Acq On : 19 Oct 2019 12:14
Operator : JU
Sample : K5321-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB5

Quant Time: Oct 19 22:18:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 19 22:14:11 2019
Response via : Initial Calibration

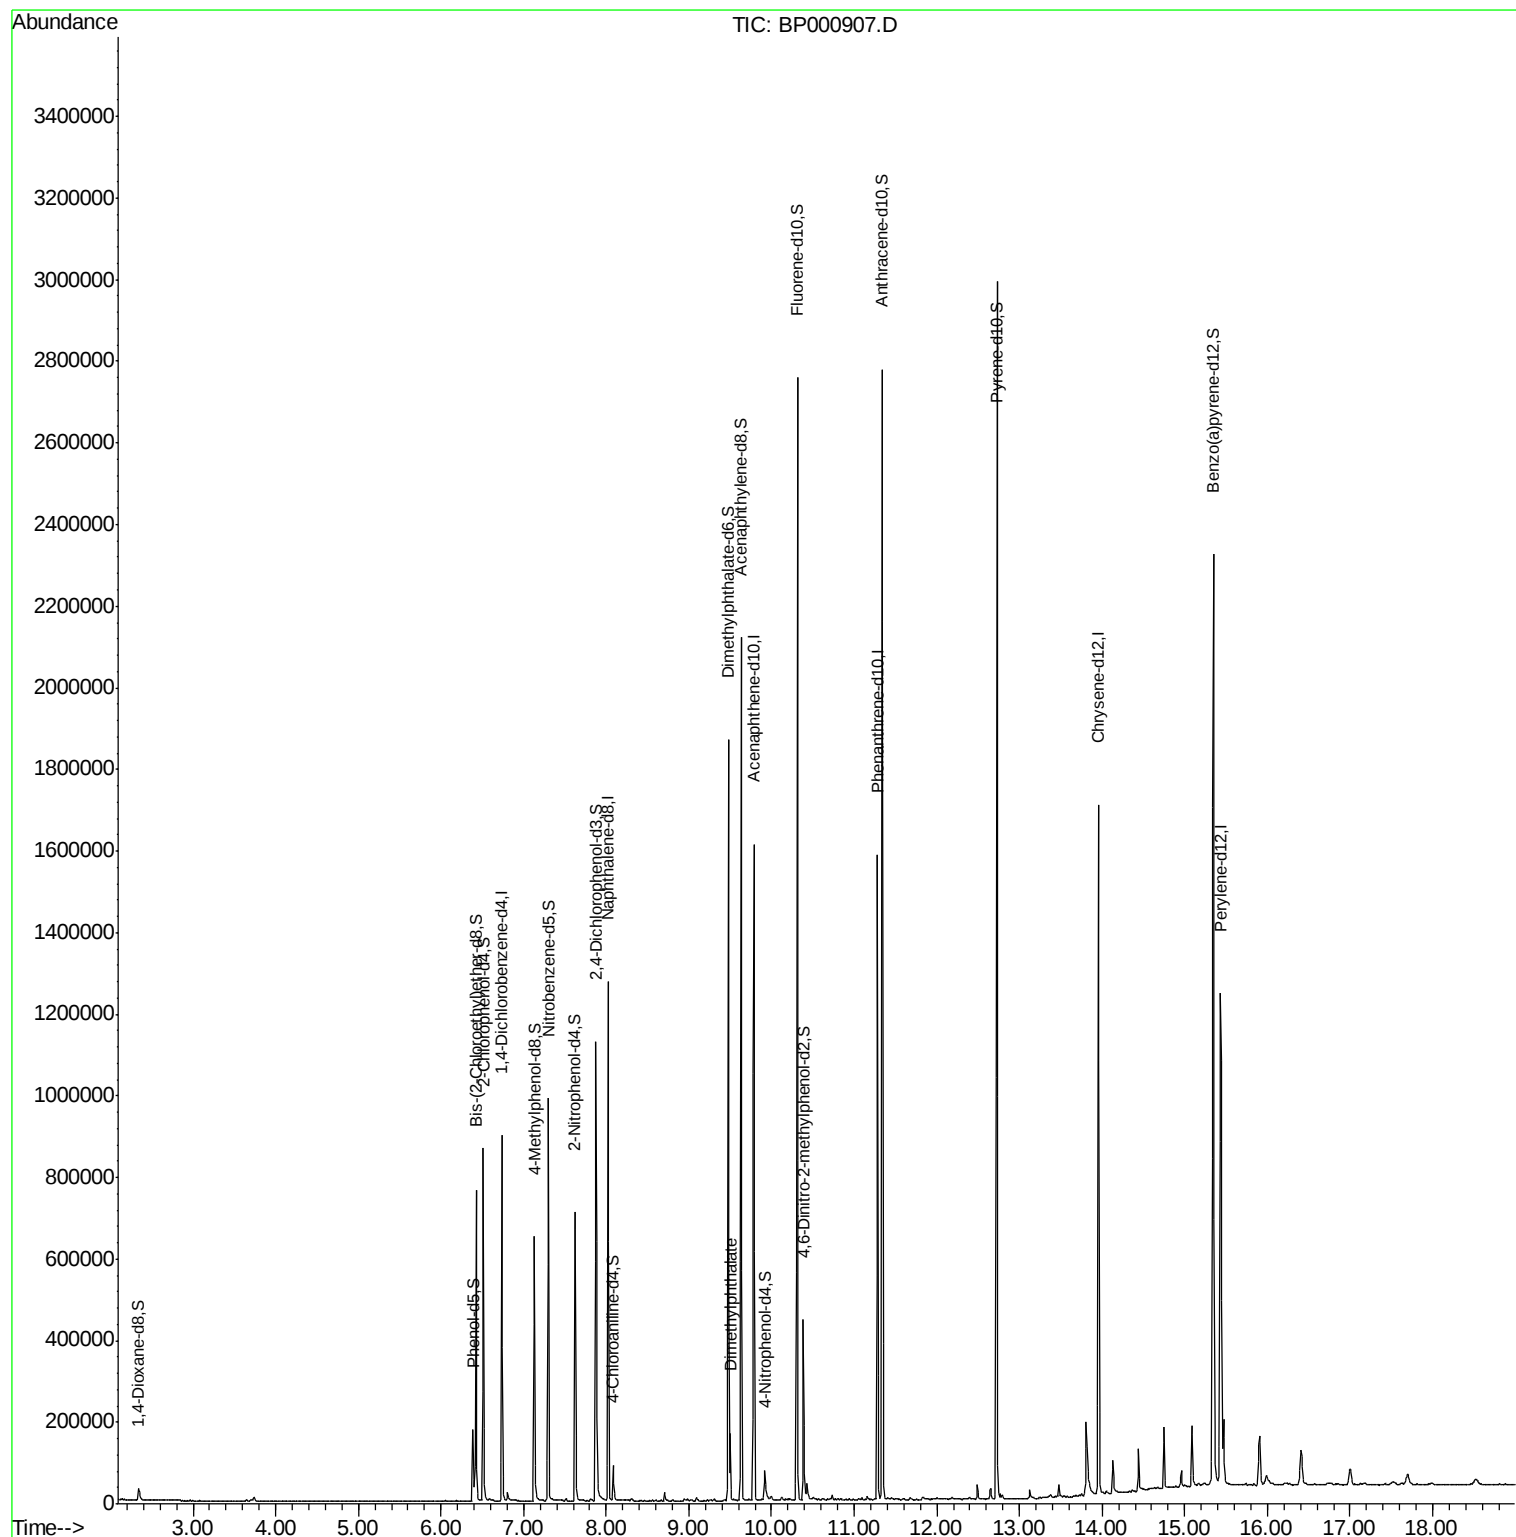

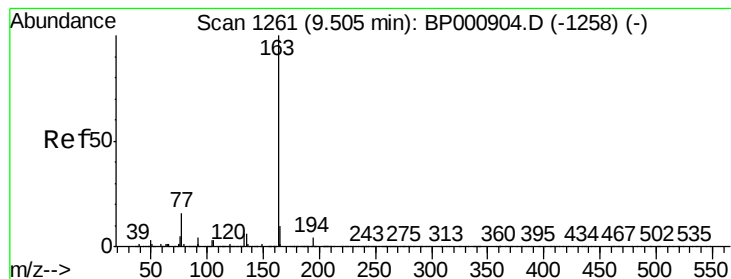

#45

Dimethylphthalate

Concen: 2.867 ng/ul

RT: 9.50 min Scan# 1260

Delta R.T. -0.01 min

Lab File: BP000907.D

Acq: 19 Oct 2019 12:14

Instrument :

BNA_P

ClientSampleId :

E0AB5


Tot Ion:163 Resp: 58655

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.6 8.1 12.1

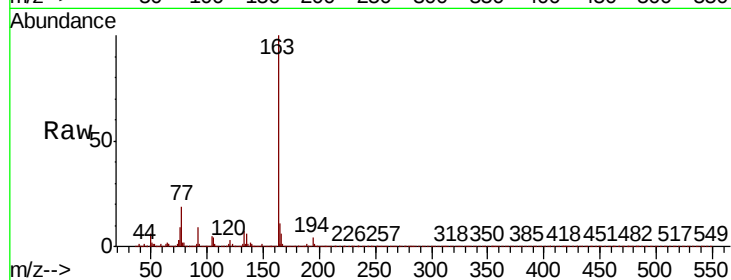

Abundance Ion 163.00 (162.70 to 163.70): E

100000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

