

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000917.D
 Acq On : 19 Oct 2019 16:15
 Operator : JU
 Sample : K5321-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AA3

Quant Time: Oct 19 22:45:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 19 22:14:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	139609	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	518250	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.79	164	292356	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.28	188	549363	20.00	ng/ul	0.00
78) Chrysene-d12	13.96	240	525264	20.00	ng/ul	0.00
86) Perylene-d12	15.43	264	619283	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.34	96	16285	4.84	ng/uL	0.00
5) Phenol-d5	6.38	99	58355	5.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	128144	23.80	ng/ul	0.00
9) 2-Chlorophenol-d4	6.51	132	188947	20.83	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	114473	13.91	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	108138	27.45	ng/ul	0.00
22) 2-Nitrophenol-d4	7.62	143	117608	28.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	196086	24.42	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	20545	2.30	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	597585	29.20	ng/ul	0.00
47) Acenaphthylene-d8	9.63	160	697508	27.71	ng/ul	0.00
52) 4-Nitrophenol-d4	9.92	143	16251	5.16	ng/ul	0.00
58) Fluorene-d10	10.30	176	508472	29.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	59053	22.57	ng/ul	0.00
71) Anthracene-d10	11.34	188	832900	32.73	ng/ul	0.00
79) Pyrene-d10	12.72	212	905998	30.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.35	264	1002043	32.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	9.50	163	139790	6.855	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000917.D
Acq On : 19 Oct 2019 16:15
Operator : JU
Sample : K5321-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AA3

Quant Time: Oct 19 22:45:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 19 22:14:11 2019
Response via : Initial Calibration

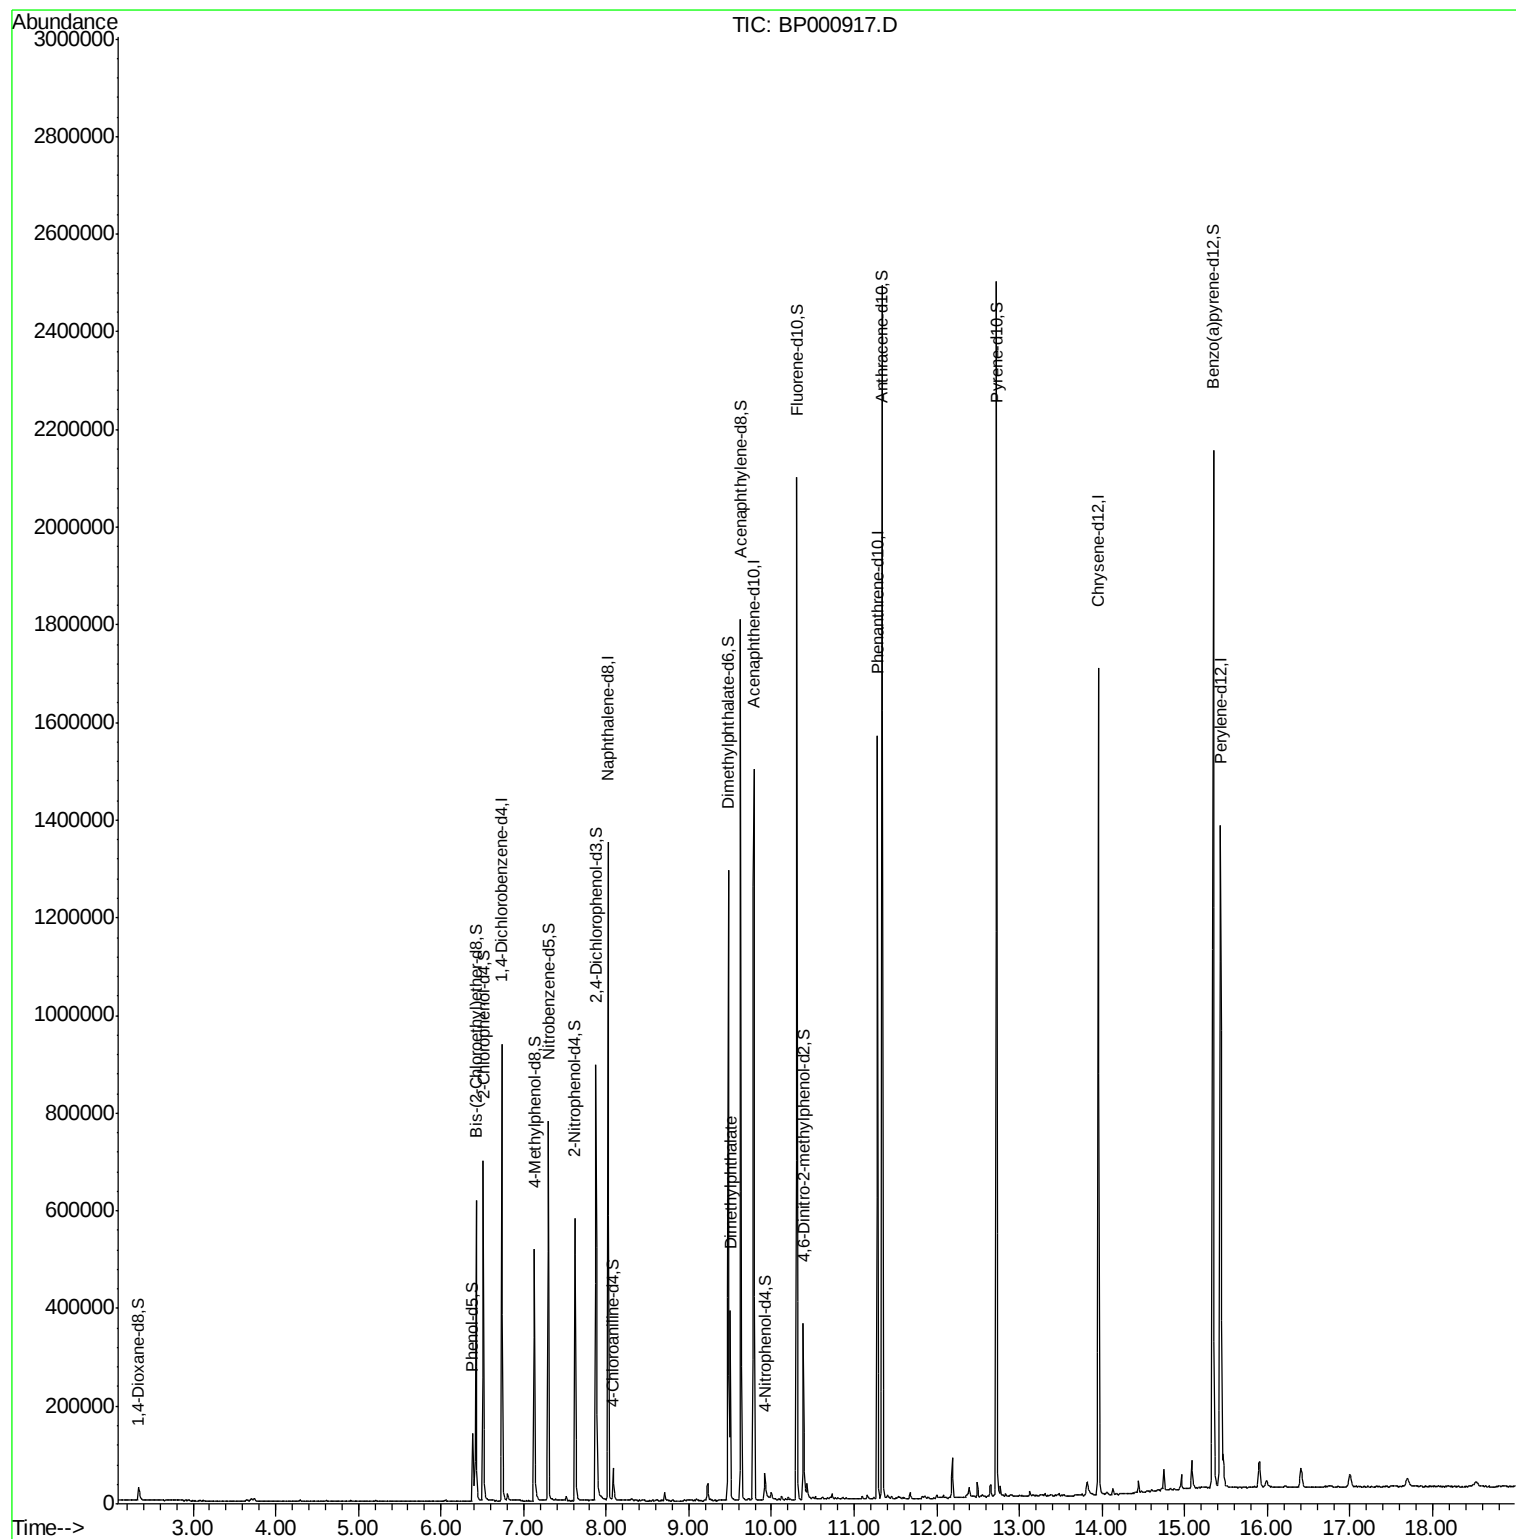

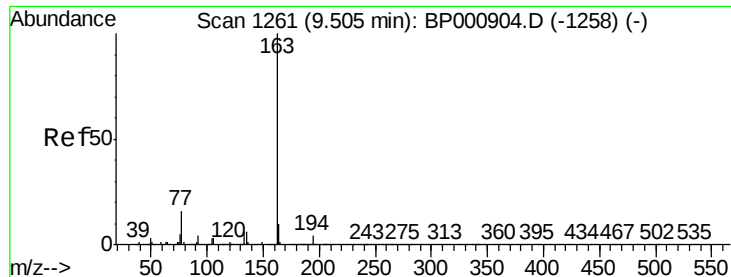

#45

Dimethylphthalate

Concen: 6.855 ng/ul

RT: 9.50 min Scan# 1260

Delta R.T. -0.01 min

Lab File: BP000917.D

Acq: 19 Oct 2019 16:15

Instrument :

BNA_P

ClientSampleId :

E0AA3


Tot Ion:163 Resp: 139790

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.3 8.1 12.1

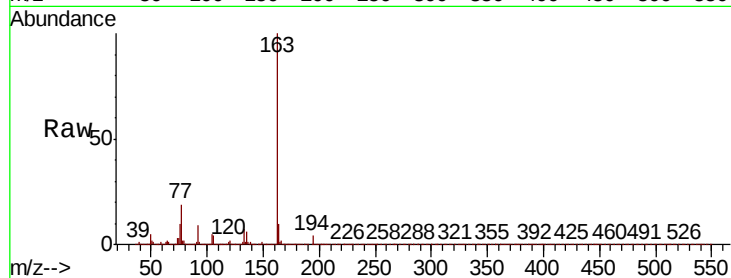

Abundance Ion 163.00 (162.70 to 163.70): E

250000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

