

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000910.D
 Acq On : 19 Oct 2019 13:27
 Operator : JU
 Sample : K5321-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.346	40	44	57	rBV	25383	38537	1.39%	0.138%
2	3.740	276	281	287	rVB	9195	14603	0.53%	0.052%
3	4.434	395	399	405	rBV	3561	4494	0.16%	0.016%
4	6.387	727	731	734	rBV2	169030	188293	6.81%	0.673%
5	6.422	734	737	749	rVV	777758	642026	23.22%	2.294%
6	6.510	749	752	763	rVV	790437	703297	25.43%	2.513%
7	6.740	788	791	800	rBV	999008	778578	28.15%	2.782%
8	6.810	800	803	811	rVB2	4099	5609	0.20%	0.020%
9	7.128	854	857	873	rBV	626633	533320	19.29%	1.906%
10	7.298	882	886	899	rBV	981491	766106	27.70%	2.738%
11	7.516	920	923	926	rBV	11932	9691	0.35%	0.035%
12	7.628	938	942	957	rBV	732709	643828	23.28%	2.301%
13	7.810	970	973	978	rBV	6153	6439	0.23%	0.023%
14	7.875	981	984	1006	rVV	1123203	1016832	36.77%	3.634%
15	8.022	1006	1009	1013	rVV	1381060	1053701	38.10%	3.766%
16	8.087	1017	1020	1028	rVB	113577	100984	3.65%	0.361%
17	8.304	1054	1057	1063	rVB	2767	2925	0.11%	0.010%
18	8.704	1122	1125	1130	rBV	18408	17748	0.64%	0.063%
19	9.210	1209	1211	1216	rVB2	2614	3315	0.12%	0.012%
20	9.257	1216	1219	1224	rVV4	2537	3613	0.13%	0.013%
21	9.304	1224	1227	1230	rVB	6297	4823	0.17%	0.017%
22	9.481	1253	1257	1259	rBV	1798058	1446380	52.30%	5.169%
23	9.498	1259	1260	1264	rVV	215432	150391	5.44%	0.537%
24	9.539	1265	1267	1274	rVB7	3409	4323	0.16%	0.015%
25	9.633	1279	1283	1286	rBV	2174891	1877476	67.89%	6.710%
26	9.722	1293	1298	1301	rBV3	4535	5455	0.20%	0.019%
27	9.786	1305	1309	1312	rBV	1708759	1345012	48.64%	4.807%
28	9.881	1323	1325	1328	rBV2	4800	4133	0.15%	0.015%
29	9.916	1328	1331	1339	rVV	66114	91308	3.30%	0.326%
30	9.998	1342	1345	1351	rVB6	7723	11846	0.43%	0.042%
31	10.204	1377	1380	1382	rBV2	6946	7113	0.26%	0.025%
32	10.275	1389	1392	1394	rBV3	3791	3613	0.13%	0.013%
33	10.310	1394	1398	1401	rBV	2665498	2217400	80.18%	7.924%
34	10.386	1407	1411	1417	rBV	480437	434203	15.70%	1.552%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000910.D
 Acq On : 19 Oct 2019 13:27
 Operator : JU
 Sample : K5321-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	10.433	1417	1419	1428	rVV	40356	48295	1.75%	0.173%
36	10.504	1428	1431	1434	rVB	5645	5769	0.21%	0.021%
37	10.622	1448	1451	1453	rBV2	2994	3077	0.11%	0.011%
38	10.681	1458	1461	1463	rVV2	8323	7958	0.29%	0.028%
39	10.733	1467	1470	1474	rVB	12905	12100	0.44%	0.043%
40	10.798	1479	1481	1485	rVB5	2500	2949	0.11%	0.011%
41	10.892	1494	1497	1501	rBV6	2497	3487	0.13%	0.012%
42	11.098	1529	1532	1535	rVB	6114	5336	0.19%	0.019%
43	11.139	1535	1539	1541	rBV3	5021	6037	0.22%	0.022%
44	11.157	1541	1542	1548	rVB2	7541	7979	0.29%	0.029%
45	11.280	1560	1563	1567	rBV	1636667	1464373	52.95%	5.233%
46	11.339	1569	1573	1577	rBV	2763168	2400355	86.80%	8.578%
47	11.675	1628	1630	1634	rVB5	2797	3733	0.13%	0.013%
48	11.822	1653	1655	1664	rBV3	9173	17070	0.62%	0.061%
49	11.998	1682	1685	1689	rBV5	4602	6129	0.22%	0.022%
50	12.098	1700	1702	1707	rVB5	2369	3323	0.12%	0.012%
51	12.392	1749	1752	1755	rVB	8346	6156	0.22%	0.022%
52	12.439	1758	1760	1765	rVB5	2846	2984	0.11%	0.011%
53	12.492	1765	1769	1774	rBV	33951	29706	1.07%	0.106%
54	12.651	1793	1796	1800	rVB	26650	23428	0.85%	0.084%
55	12.727	1804	1809	1812	rVV	3010175	2765415	100.00%	9.883%
56	12.769	1814	1816	1818	rVV	17994	15821	0.57%	0.057%
57	12.792	1818	1820	1827	rVB	15305	14290	0.52%	0.051%
58	13.133	1873	1878	1881	rBV	26669	29232	1.06%	0.104%
59	13.280	1900	1903	1907	rVB	3277	3413	0.12%	0.012%
60	13.363	1912	1917	1918	rBV4	5759	8498	0.31%	0.030%
61	13.427	1926	1928	1931	rBV4	3848	3545	0.13%	0.013%
62	13.457	1931	1933	1934	rBV	3502	2955	0.11%	0.011%
63	13.474	1934	1936	1939	rVV	39457	36382	1.32%	0.130%
64	13.545	1944	1948	1951	rVB2	3913	5958	0.22%	0.021%
65	13.686	1970	1972	1976	rBV5	3959	3821	0.14%	0.014%
66	13.722	1976	1978	1980	rBV2	3688	2915	0.11%	0.010%
67	13.810	1989	1993	2011	rBV2	169855	280146	10.13%	1.001%
68	13.957	2014	2018	2022	rBV	1794842	1512080	54.68%	5.404%
69	14.051	2031	2034	2035	rBV	8707	8055	0.29%	0.029%
70	14.133	2044	2048	2060	rBV	92687	87660	3.17%	0.313%
71	14.327	2079	2081	2083	rVB3	5502	4294	0.16%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000910.D
 Acq On : 19 Oct 2019 13:27
 Operator : JU
 Sample : K5321-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

72	14.439	2097	2100	2104	rBV	105028	100533	3.64%	0.359%
73	14.751	2149	2153	2160	rBV	116448	117878	4.26%	0.421%
74	14.957	2185	2188	2192	rVB	35641	35248	1.27%	0.126%
75	15.086	2206	2210	2219	rBV	121881	141002	5.10%	0.504%
76	15.345	2248	2254	2263	rBV	2203777	2605958	94.23%	9.313%
77	15.433	2264	2269	2273	rVV	1268223	1513951	54.75%	5.410%
78	15.468	2273	2275	2283	rVB	112758	127021	4.59%	0.454%
79	15.904	2344	2349	2356	rBV	83327	127075	4.60%	0.454%
80	15.986	2360	2363	2367	rVV4	14046	21003	0.76%	0.075%
81	16.410	2429	2435	2444	rVB	56385	110840	4.01%	0.396%
82	16.998	2530	2535	2543	rVB2	29208	59931	2.17%	0.214%
83	17.698	2650	2654	2664	rVB3	17586	39698	1.44%	0.142%


Sum of corrected areas: 27982277

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000910.D
Acq On : 19 Oct 2019 13:27
Operator : JU
Sample : K5321-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
E0AB3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

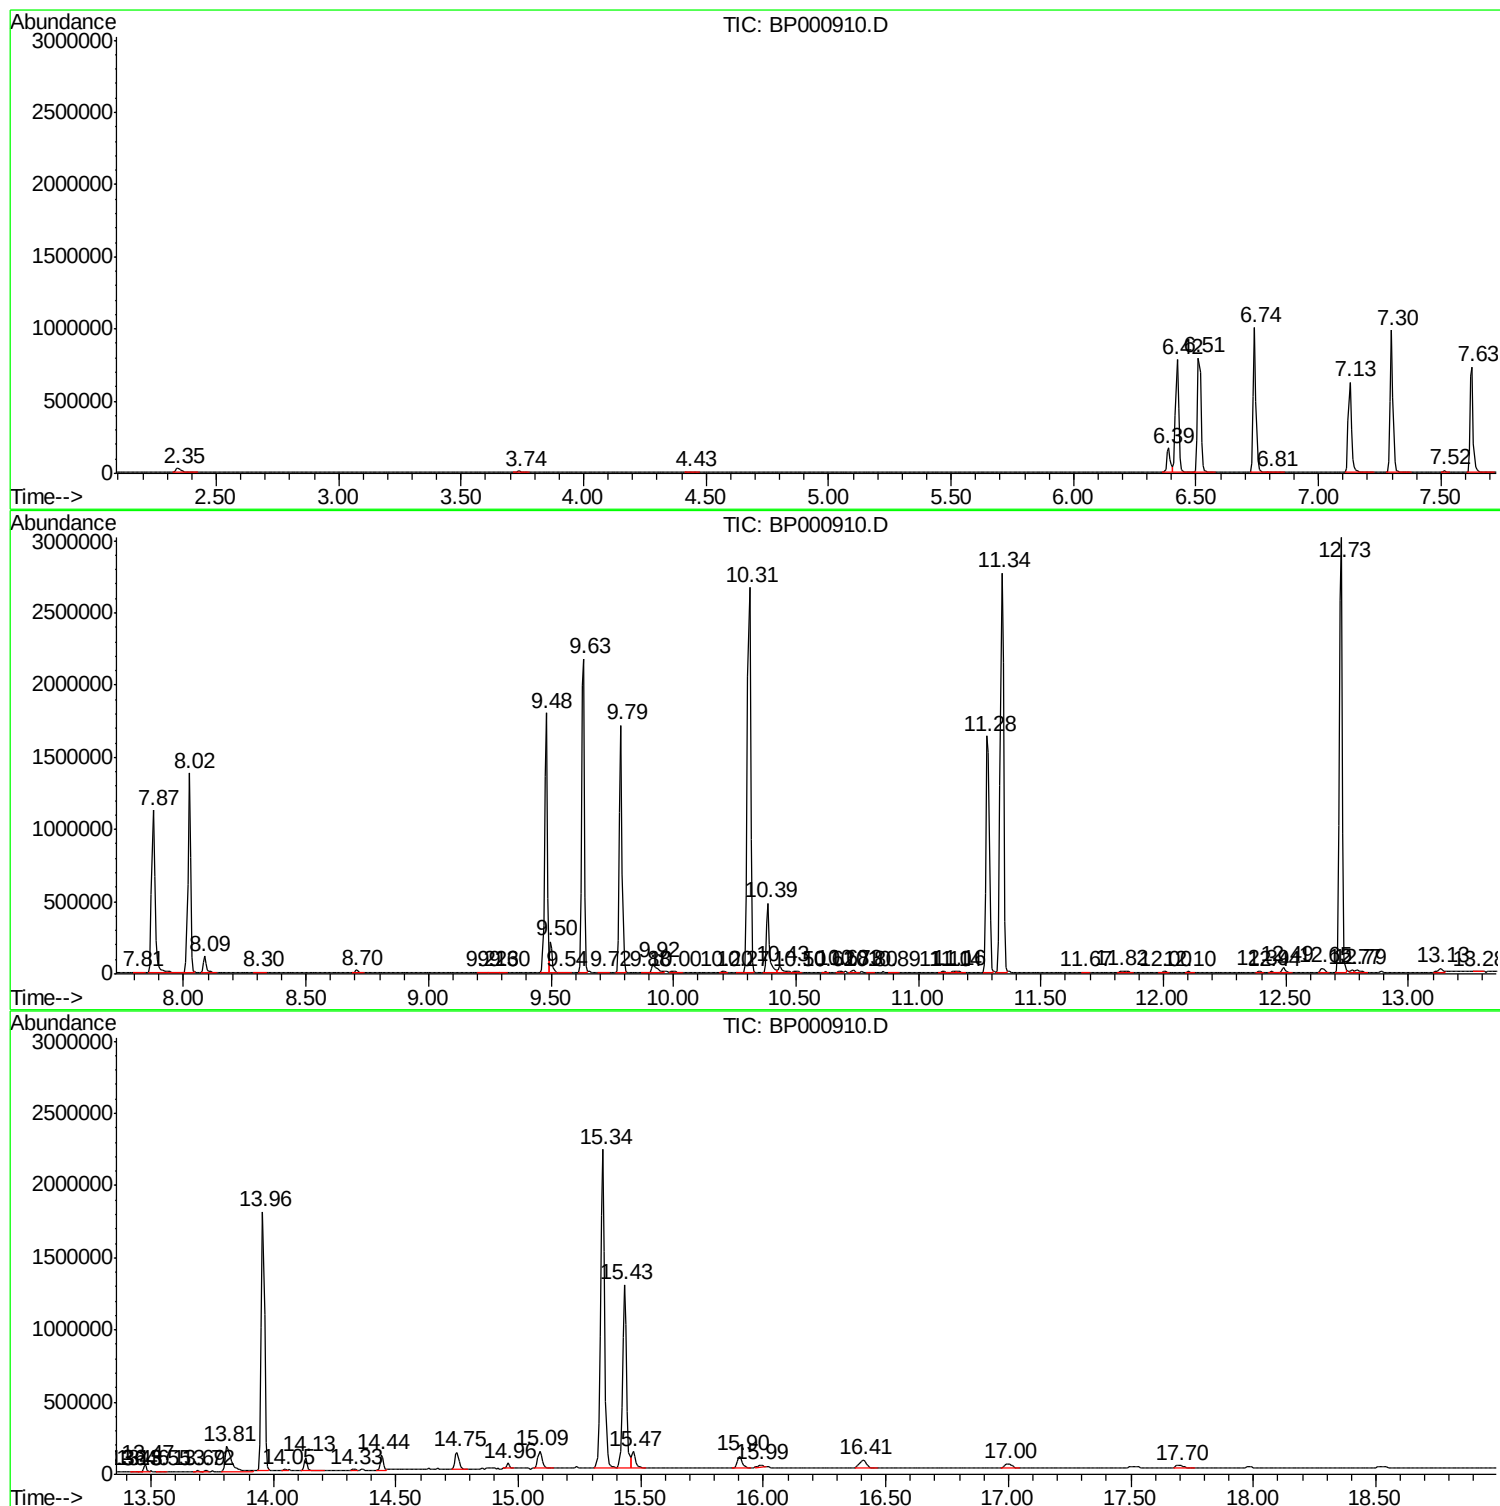

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000910.D
Acq On : 19 Oct 2019 13:27
Operator : JU
Sample : K5321-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB3










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic13.81 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.81	3.71 ng/ul	280146	Chrysene-d12	13.96

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentadecane	210	C15H30	000295-48-7	95
2		Ethanol, 2-(octadecyloxy)-	314	C20H42O2	002136-72-3	89
3		Cyclopentadecane	210	C15H30	000295-48-7	74
4		9-Nonadecene	266	C19H38	031035-07-1	70
5		Heptafluorobutanoic acid, heptad...	452	C21H35F7O2	1000282-97-3	60

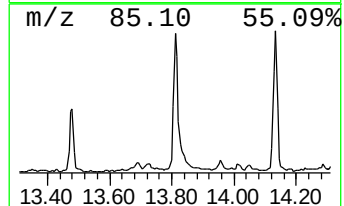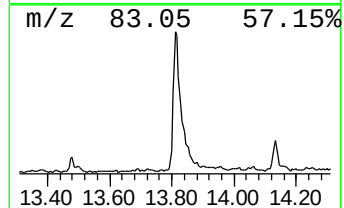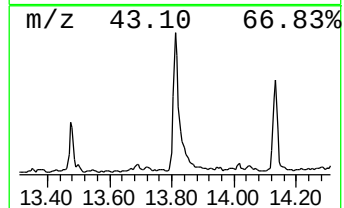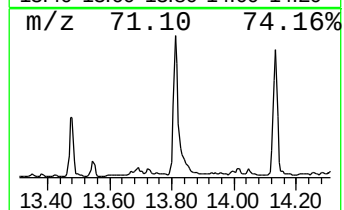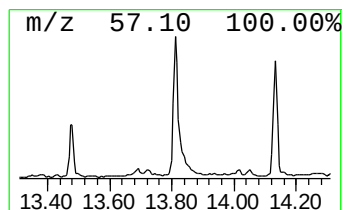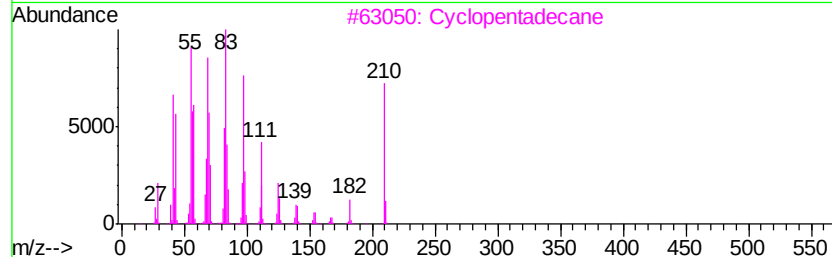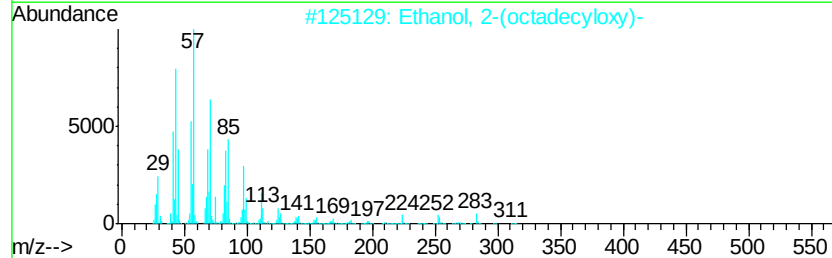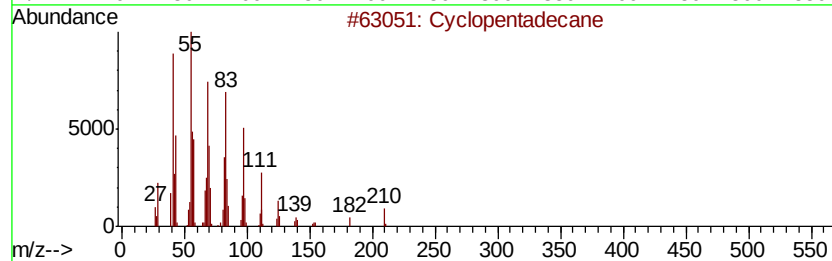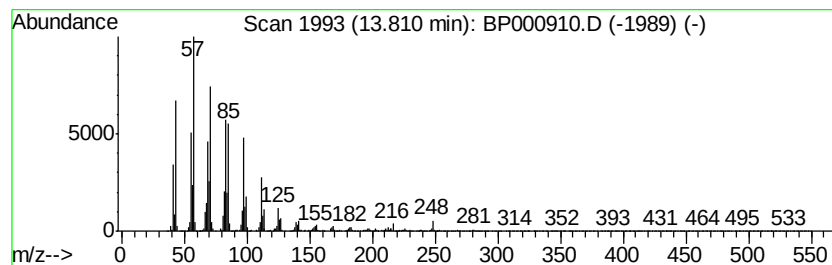

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000910.D
Acq On : 19 Oct 2019 13:27
Operator : JU
Sample : K5321-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Cyc...	13.81	3.7	ng/ul	280146	5	13.96	1512080	20.0