

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000911.D
 Acq On : 19 Oct 2019 13:51
 Operator : JU
 Sample : K5321-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	39	43	54	rVB	27208	39762	1.32%	0.135%
2	3.705	270	275	276	rBV3	2185	3384	0.11%	0.012%
3	3.734	276	280	285	rVB	5222	7819	0.26%	0.027%
4	6.387	727	731	734	rBV	163121	180050	5.99%	0.613%
5	6.422	734	737	749	rVB	769187	639066	21.26%	2.176%
6	6.510	749	752	763	rBV	800584	696766	23.18%	2.372%
7	6.740	787	791	801	rBV	1029206	807584	26.86%	2.750%
8	6.810	801	803	810	rVB	3378	4439	0.15%	0.015%
9	7.128	854	857	872	rBV	617239	521645	17.35%	1.776%
10	7.299	882	886	898	rBV	993380	772776	25.70%	2.631%
11	7.516	919	923	927	rVB	15551	13269	0.44%	0.045%
12	7.628	938	942	952	rBV	729455	648540	21.57%	2.208%
13	7.875	981	984	1006	rBV	1128275	1015531	33.78%	3.458%
14	8.022	1006	1009	1012	rBV	1498139	1089867	36.25%	3.711%
15	8.087	1017	1020	1036	rVB	98561	94488	3.14%	0.322%
16	8.704	1123	1125	1134	rBV	18937	19240	0.64%	0.066%
17	9.481	1253	1257	1259	rBV	1917878	1497331	49.81%	5.098%
18	9.498	1259	1260	1266	rVB	230594	159814	5.32%	0.544%
19	9.634	1279	1283	1286	rBV	2161008	1944765	64.69%	6.622%
20	9.722	1293	1298	1301	rVB3	4198	4983	0.17%	0.017%
21	9.787	1305	1309	1312	rBV	1848835	1429524	47.55%	4.867%
22	9.916	1328	1331	1342	rBV	73793	102114	3.40%	0.348%
23	9.998	1342	1345	1351	rVB5	7113	11436	0.38%	0.039%
24	10.204	1377	1380	1382	rBV2	4126	4619	0.15%	0.016%
25	10.310	1394	1398	1401	rBV	2796828	2318215	77.11%	7.893%
26	10.387	1407	1411	1417	rBV	526924	479899	15.96%	1.634%
27	10.434	1417	1419	1428	rVB	40612	46318	1.54%	0.158%
28	10.622	1448	1451	1454	rBV	3621	3590	0.12%	0.012%
29	10.681	1458	1461	1463	rBV2	5598	5446	0.18%	0.019%
30	10.734	1468	1470	1473	rVB	13826	10684	0.36%	0.036%
31	10.851	1485	1490	1493	rBV3	3190	3244	0.11%	0.011%
32	11.098	1529	1532	1535	rVB2	6250	5529	0.18%	0.019%
33	11.157	1540	1542	1549	rVB2	8476	9684	0.32%	0.033%
34	11.287	1560	1564	1567	rBV	1755546	1604179	53.36%	5.462%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000911.D
 Acq On : 19 Oct 2019 13:51
 Operator : JU
 Sample : K5321-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	11.339	1569	1573	1577	rBV	2972823	2592930	86.25%	8.828%
36	11.822	1652	1655	1657	rBV2	6607	6423	0.21%	0.022%
37	11.851	1658	1660	1664	rVB	4655	5177	0.17%	0.018%
38	12.439	1758	1760	1765	rBV4	3477	3662	0.12%	0.012%
39	12.492	1765	1769	1775	rVV	36136	32147	1.07%	0.109%
40	12.651	1792	1796	1801	rVB	30701	26726	0.89%	0.091%
41	12.728	1804	1809	1812	rBV	3407571	3006381	100.00%	10.236%
42	12.792	1818	1820	1826	rVB6	4342	4727	0.16%	0.016%
43	13.134	1874	1878	1881	rBV3	5997	7017	0.23%	0.024%
44	13.281	1900	1903	1910	rVB4	3717	3980	0.13%	0.014%
45	13.428	1926	1928	1931	rBV4	3819	3533	0.12%	0.012%
46	13.475	1934	1936	1940	rVV2	8190	8746	0.29%	0.030%
47	13.539	1944	1947	1950	rVB3	3328	4494	0.15%	0.015%
48	13.816	1990	1994	2008	rVB3	41064	77668	2.58%	0.264%
49	13.957	2014	2018	2022	rBV	1954078	1757323	58.45%	5.983%
50	14.063	2032	2036	2039	rVB3	5026	7132	0.24%	0.024%
51	14.133	2044	2048	2058	rBV	39086	43643	1.45%	0.149%
52	14.439	2097	2100	2111	rBV	63705	71397	2.37%	0.243%
53	14.751	2149	2153	2159	rBV	100003	100069	3.33%	0.341%
54	14.957	2184	2188	2191	rBV	39167	39473	1.31%	0.134%
55	15.086	2206	2210	2219	rBV	120479	143854	4.78%	0.490%
56	15.345	2248	2254	2263	rBV	2431276	2957169	98.36%	10.069%
57	15.433	2264	2269	2273	rVV	1439552	1735551	57.73%	5.909%
58	15.469	2273	2275	2287	rVB	125915	143395	4.77%	0.488%
59	15.904	2344	2349	2357	rBV	96970	138378	4.60%	0.471%
60	15.992	2360	2364	2374	rVB2	15542	27758	0.92%	0.095%
61	16.404	2429	2434	2443	rVB	59315	110556	3.68%	0.376%
62	16.998	2530	2535	2544	rVB2	33803	69839	2.32%	0.238%
63	17.698	2649	2654	2662	rVB5	20265	45696	1.52%	0.156%


Sum of corrected areas: 29370444

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000911.D
Acq On : 19 Oct 2019 13:51
Operator : JU
Sample : K5321-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

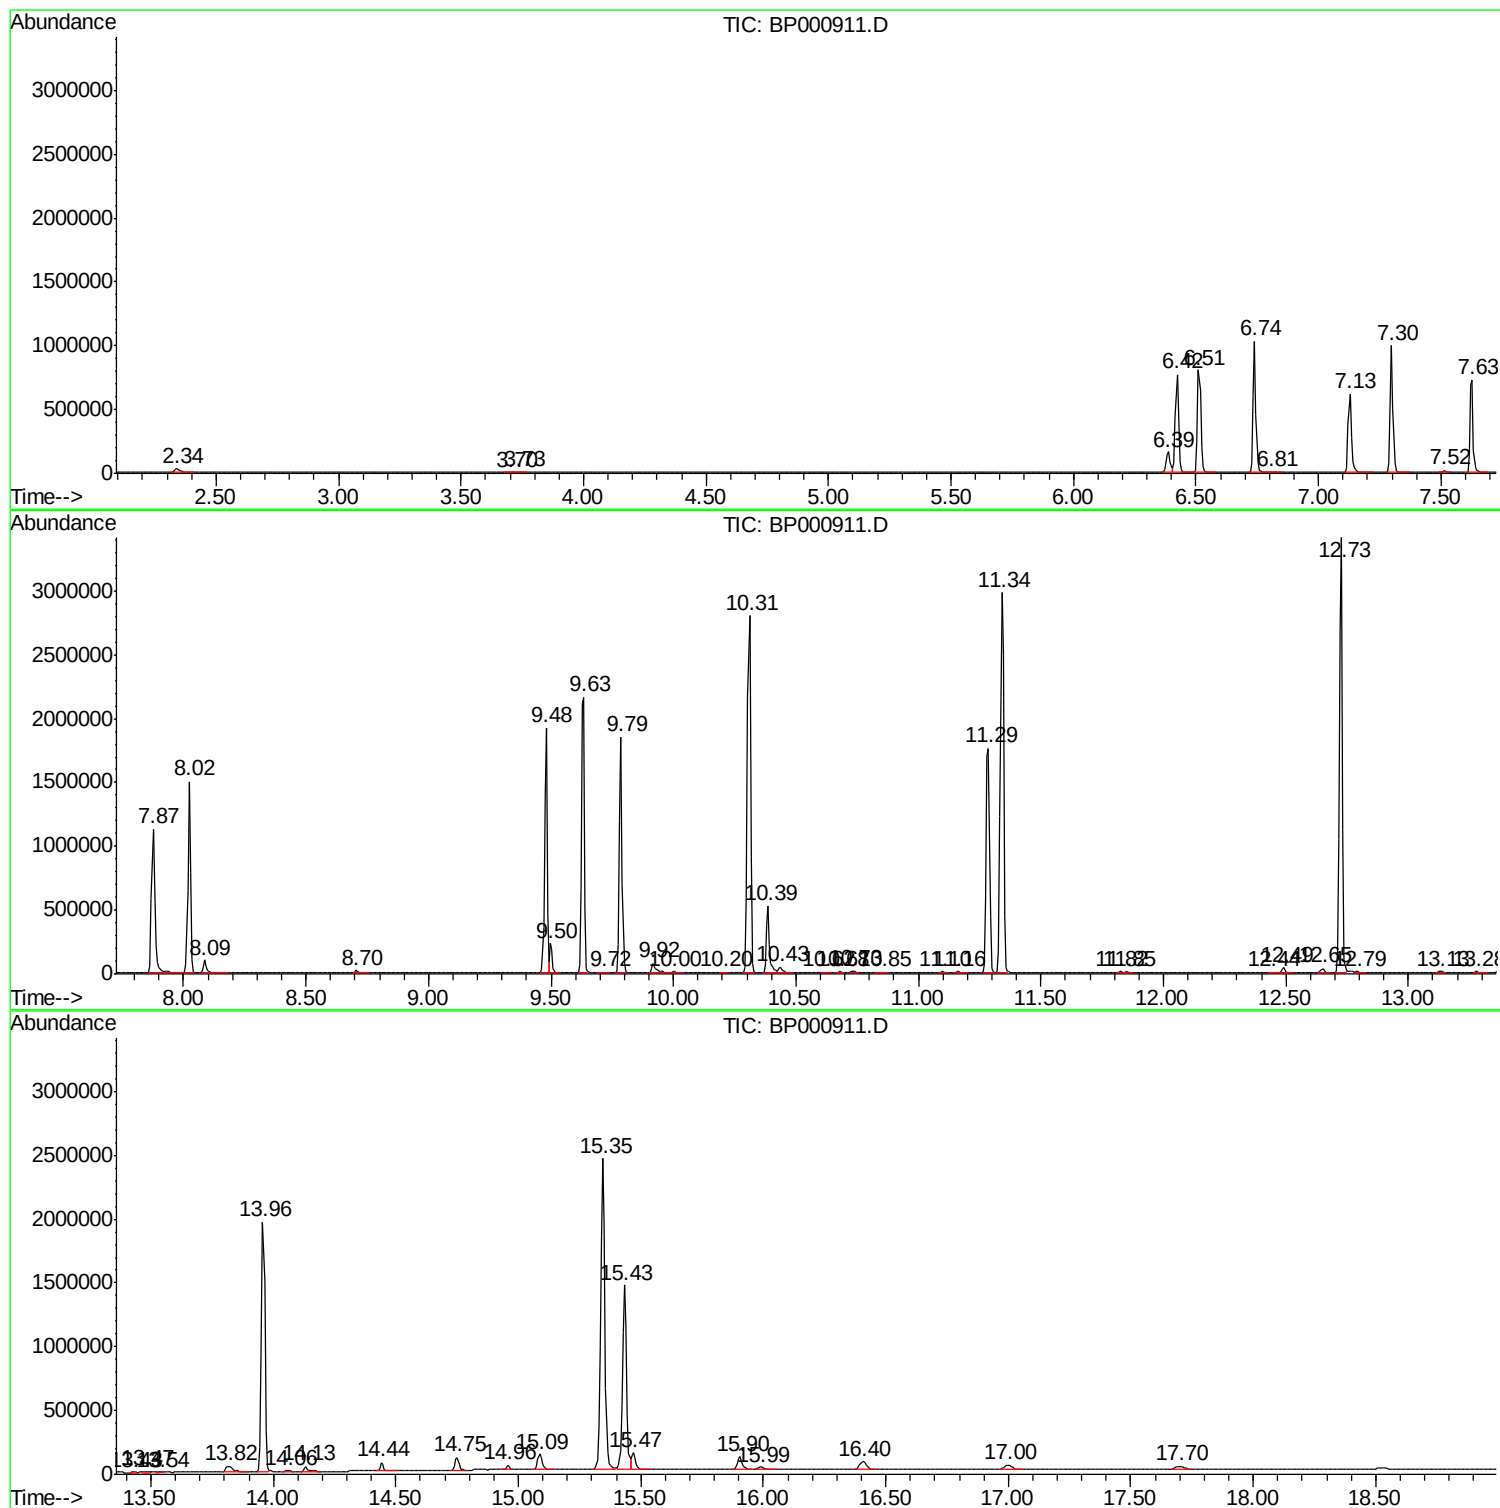

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000911.D
Acq On : 19 Oct 2019 13:51
Operator : JU
Sample : K5321-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000911.D
Acq On : 19 Oct 2019 13:51
Operator : JU
Sample : K5321-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc