

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000915.D
 Acq On : 19 Oct 2019 15:27
 Operator : JU
 Sample : K5321-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AA2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	39	43	53	rVB	27163	40150	1.45%	0.145%
2	3.699	269	274	277	rBV	3931	6464	0.23%	0.023%
3	3.734	277	280	287	rVB	7633	11404	0.41%	0.041%
4	4.940	482	485	492	rVB	2139	2913	0.11%	0.011%
5	6.187	694	697	701	rBV2	2818	2870	0.10%	0.010%
6	6.387	727	731	734	rBV	146812	163410	5.90%	0.592%
7	6.422	734	737	749	rVB	695778	579766	20.93%	2.099%
8	6.511	749	752	762	rBV	750189	642614	23.20%	2.327%
9	6.740	787	791	799	rBV	972425	785043	28.34%	2.843%
10	6.805	799	802	809	rVB	19165	21146	0.76%	0.077%
11	7.128	853	857	869	rBV	536585	492054	17.77%	1.782%
12	7.299	882	886	892	rBV	887788	697285	25.18%	2.525%
13	7.387	898	901	905	rVB3	3391	3206	0.12%	0.012%
14	7.516	920	923	926	rVB	5319	4940	0.18%	0.018%
15	7.622	938	941	954	rBV	662900	589522	21.28%	2.135%
16	7.875	981	984	1005	rBV	1017592	932530	33.67%	3.377%
17	8.022	1005	1009	1012	rBV	1401735	1058487	38.22%	3.833%
18	8.087	1017	1020	1027	rVB	66499	60488	2.18%	0.219%
19	8.305	1054	1057	1062	rVB	4952	4919	0.18%	0.018%
20	8.704	1122	1125	1133	rBV	18231	17384	0.63%	0.063%
21	8.940	1162	1165	1169	rBV2	3920	3640	0.13%	0.013%
22	8.981	1169	1172	1176	rVV	3576	4228	0.15%	0.015%
23	9.093	1188	1191	1197	rVB	7736	7322	0.26%	0.027%
24	9.481	1253	1257	1259	rBV	1824613	1463476	52.84%	5.300%
25	9.499	1259	1260	1265	rVB	208903	139477	5.04%	0.505%
26	9.628	1279	1282	1286	rBV	2026138	1804358	65.15%	6.534%
27	9.722	1293	1298	1303	rBV5	3571	4493	0.16%	0.016%
28	9.787	1305	1309	1312	rBV	1725728	1366259	49.33%	4.947%
29	9.916	1325	1331	1340	rBV	64831	98202	3.55%	0.356%
30	9.999	1342	1345	1350	rVB2	14190	15070	0.54%	0.055%
31	10.122	1362	1366	1371	rBV2	10017	9087	0.33%	0.033%
32	10.204	1376	1380	1382	rBV2	6047	6950	0.25%	0.025%
33	10.310	1394	1398	1401	rBV	2628852	2203996	79.57%	7.981%
34	10.387	1407	1411	1417	rBV	462388	430265	15.53%	1.558%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000915.D
 Acq On : 19 Oct 2019 15:27
 Operator : JU
 Sample : K5321-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AA2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	10.434	1417	1419	1428	rVV	40573	48116	1.74%	0.174%
36	10.499	1428	1430	1433	rVV3	5293	5694	0.21%	0.021%
37	10.528	1433	1435	1439	rVB	4197	3855	0.14%	0.014%
38	10.734	1467	1470	1473	rVB2	12631	11354	0.41%	0.041%
39	10.799	1478	1481	1484	rVB3	3537	2884	0.10%	0.010%
40	10.987	1510	1513	1518	rBV7	1968	2903	0.10%	0.011%
41	11.099	1529	1532	1535	rVB	5646	4488	0.16%	0.016%
42	11.140	1536	1539	1540	rBV2	3788	3293	0.12%	0.012%
43	11.157	1540	1542	1547	rVB2	7518	7885	0.28%	0.029%
44	11.281	1560	1563	1567	rBV	1658388	1517142	54.78%	5.494%
45	11.340	1569	1573	1577	rBV	2791847	2402933	86.76%	8.701%
46	11.404	1581	1584	1587	rVV3	5287	4570	0.16%	0.017%
47	11.451	1590	1592	1598	rVB	7243	7363	0.27%	0.027%
48	11.504	1598	1601	1605	rBV2	3358	3582	0.13%	0.013%
49	11.675	1628	1630	1634	rVB5	7134	7206	0.26%	0.026%
50	11.822	1652	1655	1659	rBV3	11296	15556	0.56%	0.056%
51	12.187	1714	1717	1720	rBV	6960	6240	0.23%	0.023%
52	12.440	1757	1760	1765	rBV7	3565	4319	0.16%	0.016%
53	12.493	1765	1769	1776	rVB	35458	31509	1.14%	0.114%
54	12.651	1792	1796	1801	rVB	26754	25075	0.91%	0.091%
55	12.728	1804	1809	1812	rBV	2978262	2769729	100.00%	10.030%
56	12.887	1833	1836	1840	rBV	7652	6255	0.23%	0.023%
57	13.128	1872	1877	1881	rBV6	6315	10754	0.39%	0.039%
58	13.281	1900	1903	1907	rVB4	3807	3298	0.12%	0.012%
59	13.381	1917	1920	1925	rVB7	3151	3707	0.13%	0.013%
60	13.475	1934	1936	1939	rBV	5590	5225	0.19%	0.019%
61	13.534	1944	1946	1950	rVB2	3742	5313	0.19%	0.019%
62	13.810	1989	1993	2011	rBV2	136862	266700	9.63%	0.966%
63	13.957	2014	2018	2022	rBV	1810252	1634236	59.00%	5.918%
64	14.051	2032	2034	2039	rVB2	5032	6713	0.24%	0.024%
65	14.134	2044	2048	2051	rBV	28745	28155	1.02%	0.102%
66	14.440	2097	2100	2104	rBV	56951	52922	1.91%	0.192%
67	14.745	2149	2152	2157	rBV	86231	87087	3.14%	0.315%
68	14.957	2184	2188	2191	rBV	34867	34740	1.25%	0.126%
69	15.087	2206	2210	2218	rBV	107398	128151	4.63%	0.464%
70	15.345	2248	2254	2263	rBV	2284578	2645757	95.52%	9.581%
71	15.434	2263	2269	2273	rVV	1361863	1622831	58.59%	5.877%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000915.D
Acq On : 19 Oct 2019 15:27
Operator : JU
Sample : K5321-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AA2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

72	15.469	2273	2275	2284	rVB	109352	120680	4.36%	0.437%
73	15.904	2343	2349	2357	rBV	82394	133677	4.83%	0.484%
74	15.986	2360	2363	2373	rVB6	18551	40611	1.47%	0.147%
75	16.404	2429	2434	2447	rVB	57603	108613	3.92%	0.393%
76	16.998	2530	2535	2544	rVB	29863	62292	2.25%	0.226%
77	17.698	2648	2654	2665	rVB5	18855	48360	1.75%	0.175%


Sum of corrected areas: 27615191

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000915.D
Acq On : 19 Oct 2019 15:27
Operator : JU
Sample : K5321-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AA2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

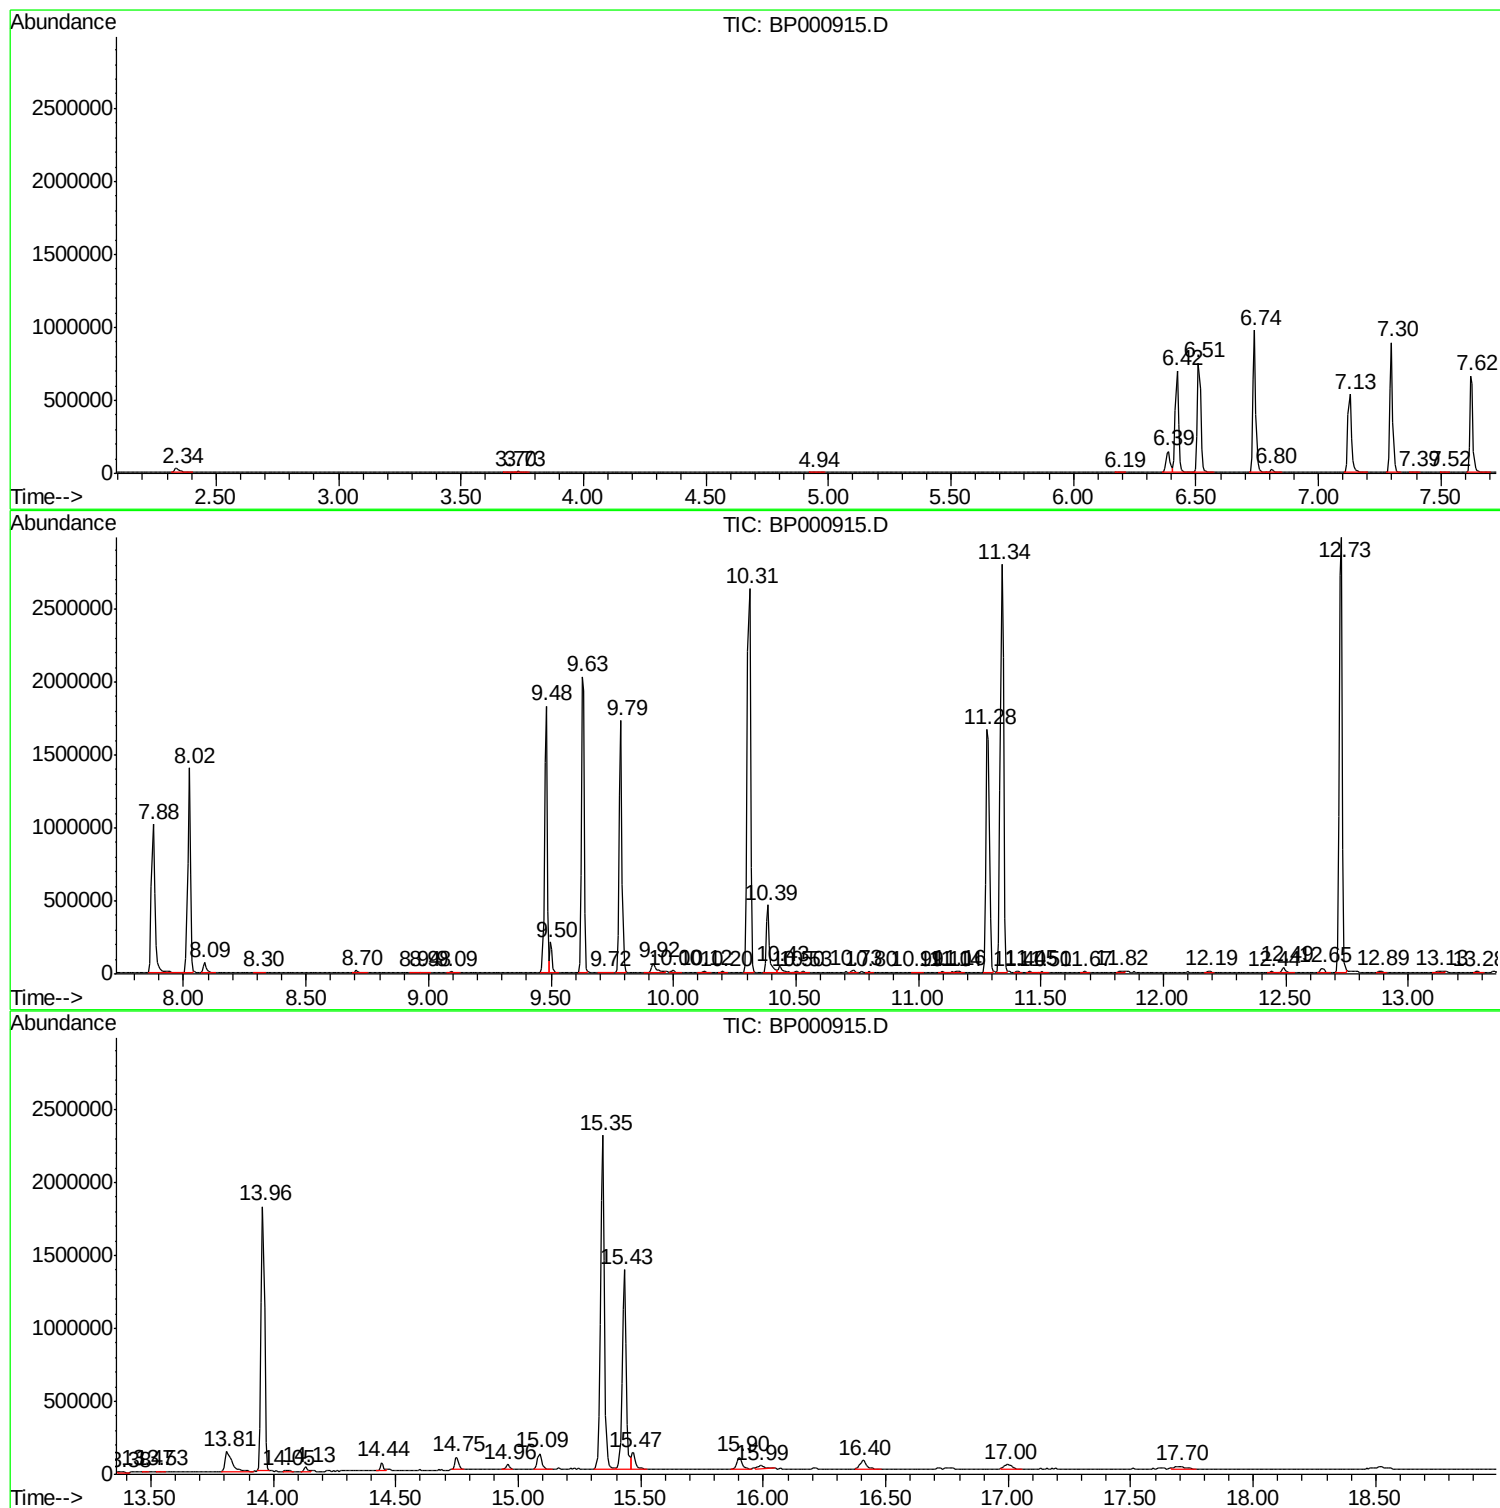

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000915.D
Acq On : 19 Oct 2019 15:27
Operator : JU
Sample : K5321-17
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
E0AA2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic13.81 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
13.81	3.26 ng/ul	266700	Chrysene-d12		13.96	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclopentadecane	210	C15H30	000295-48-7	94
2		Trifluoroacetic acid, n-octadecyl...	366	C20H37F3O2	079392-43-1	91
3		Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	90
4		1-Heneicosyl formate	340	C22H44O2	077899-03-7	90
5		Heptafluorobutanoic acid, heptad...	452	C21H35F7O2	1000282-97-3	87

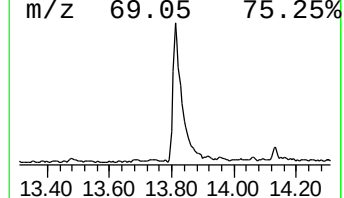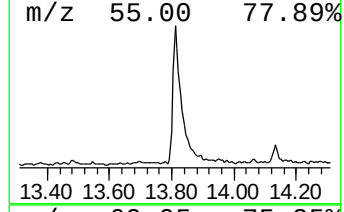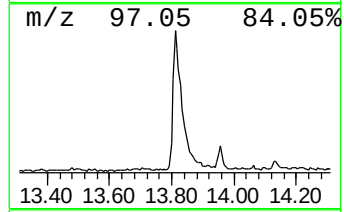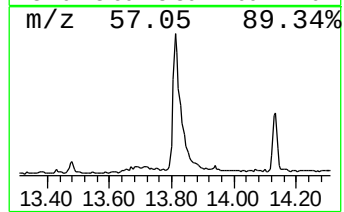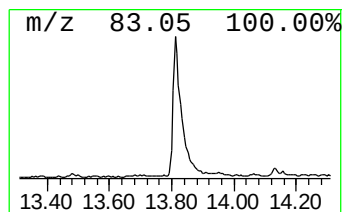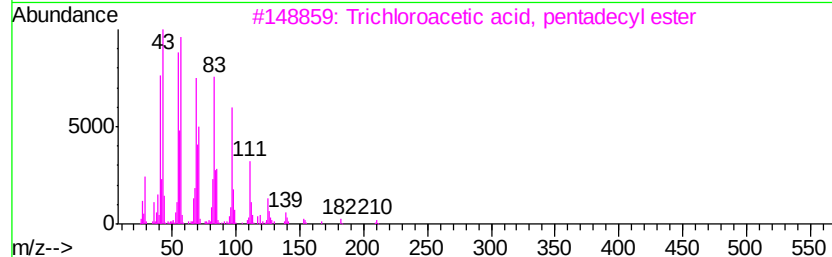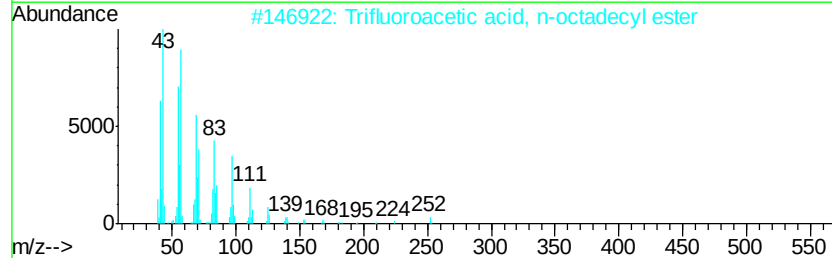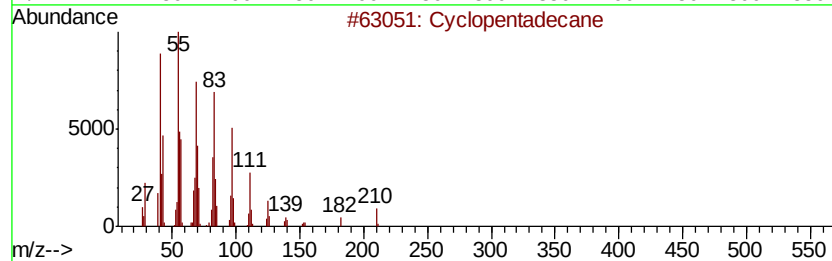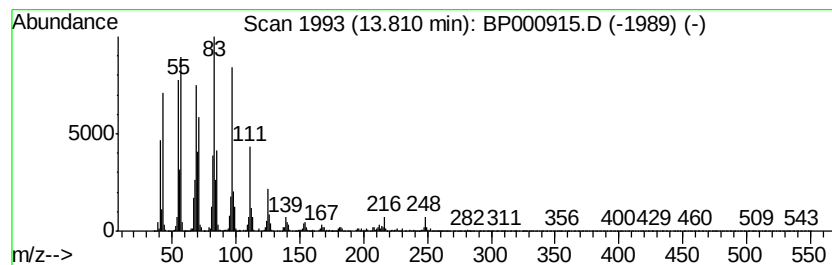

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000915.D
Acq On : 19 Oct 2019 15:27
Operator : JU
Sample : K5321-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AA2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Cyc...	13.81	3.3	ng/ul	266700	5	13.96	1634240	20.0