

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000918.D
 Acq On : 19 Oct 2019 16:39
 Operator : JU
 Sample : K5321-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.334	39	42	51	rBV	25802	37687	1.50%	0.162%
2	3.699	269	274	277	rBV	2742	4621	0.18%	0.020%
3	3.734	277	280	287	rVB	4965	7697	0.31%	0.033%
4	6.381	727	730	734	rBV	151285	162736	6.47%	0.700%
5	6.422	734	737	749	rVV	628805	532314	21.18%	2.289%
6	6.510	749	752	762	rVV	740248	617000	24.55%	2.653%
7	6.581	762	764	776	rVB8	2408	4263	0.17%	0.018%
8	6.740	787	791	800	rBV	827308	689342	27.43%	2.964%
9	6.804	800	802	809	rVB	12563	13618	0.54%	0.059%
10	7.128	854	857	872	rBV	523148	472520	18.80%	2.032%
11	7.299	882	886	898	rBV	808304	625914	24.90%	2.692%
12	7.622	938	941	952	rBV	583751	518866	20.64%	2.231%
13	7.875	981	984	1003	rBV	910189	824568	32.81%	3.546%
14	8.022	1005	1009	1012	rVV	1221278	916834	36.48%	3.943%
15	8.093	1016	1021	1026	rVB2	6287	9446	0.38%	0.041%
16	8.304	1053	1057	1064	rVB	3331	4569	0.18%	0.020%
17	8.604	1105	1108	1113	rBV2	1996	2557	0.10%	0.011%
18	8.710	1122	1126	1130	rBV	14592	14531	0.58%	0.062%
19	9.093	1188	1191	1194	rBV	4162	3709	0.15%	0.016%
20	9.269	1216	1221	1225	rBV5	1598	2612	0.10%	0.011%
21	9.475	1253	1256	1260	rBV	1295037	1149107	45.72%	4.942%
22	9.628	1279	1282	1286	rBV	1733696	1448564	57.63%	6.229%
23	9.787	1305	1309	1312	rBV	1362788	1150225	45.76%	4.946%
24	9.916	1328	1331	1339	rBV	62271	92929	3.70%	0.400%
25	9.993	1342	1344	1350	rVB6	3433	4339	0.17%	0.019%
26	10.122	1362	1366	1370	rBV2	8637	7445	0.30%	0.032%
27	10.169	1371	1374	1377	rVV	6138	5218	0.21%	0.022%
28	10.204	1377	1380	1384	rVB2	4327	4515	0.18%	0.019%
29	10.304	1394	1397	1401	rBV	2013564	1807116	71.90%	7.771%
30	10.387	1407	1411	1417	rBV	387364	374232	14.89%	1.609%
31	10.434	1417	1419	1428	rVB	31018	34195	1.36%	0.147%
32	10.528	1433	1435	1440	rVB2	5644	5495	0.22%	0.024%
33	10.734	1467	1470	1473	rVB	8639	7110	0.28%	0.031%
34	11.098	1529	1532	1536	rVB2	4669	4138	0.16%	0.018%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000918.D
 Acq On : 19 Oct 2019 16:39
 Operator : JU
 Sample : K5321-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0AB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	11.163	1539	1543	1548	rVV	4735	5660	0.23%	0.024%
36	11.281	1560	1563	1567	rBV	1441426	1259769	50.12%	5.417%
37	11.340	1569	1573	1577	rBV	2439161	2029023	80.73%	8.725%
38	11.451	1590	1592	1595	rVB	5869	4652	0.19%	0.020%
39	11.510	1599	1602	1611	rVB2	2440	3444	0.14%	0.015%
40	11.675	1627	1630	1634	rVB	13261	10707	0.43%	0.046%
41	12.104	1699	1703	1709	rVB8	2540	3735	0.15%	0.016%
42	12.187	1714	1717	1722	rVV	77694	61679	2.45%	0.265%
43	12.439	1757	1760	1765	rVB5	2493	2938	0.12%	0.013%
44	12.492	1765	1769	1774	rBV	27894	25619	1.02%	0.110%
45	12.651	1793	1796	1800	rVB	22015	19887	0.79%	0.086%
46	12.722	1804	1808	1812	rBV	2485534	2402632	95.59%	10.332%
47	13.745	1980	1982	1986	rVB3	2474	3294	0.13%	0.014%
48	13.822	1991	1995	1999	rVB3	8582	13555	0.54%	0.058%
49	13.957	2014	2018	2025	rBV	1659205	1433196	57.02%	6.163%
50	14.051	2032	2034	2039	rVB	4357	4833	0.19%	0.021%
51	14.128	2044	2047	2051	rBV	6320	7296	0.29%	0.031%
52	14.439	2097	2100	2103	rBV	15145	13921	0.55%	0.060%
53	14.745	2149	2152	2159	rVB	28480	31978	1.27%	0.138%
54	14.957	2184	2188	2192	rBV	31567	32836	1.31%	0.141%
55	15.086	2206	2210	2219	rBV2	42802	57109	2.27%	0.246%
56	15.345	2248	2254	2263	rBV	2198140	2513406	100.00%	10.808%
57	15.433	2263	2269	2273	rVV	1259158	1510466	60.10%	6.495%
58	15.469	2273	2275	2280	rVB	54533	58972	2.35%	0.254%
59	15.904	2344	2349	2355	rBV	41855	65313	2.60%	0.281%
60	15.986	2361	2363	2373	rVB4	13191	19668	0.78%	0.085%
61	16.404	2430	2434	2442	rVB	33145	57032	2.27%	0.245%
62	16.998	2530	2535	2543	rVB3	20755	41416	1.65%	0.178%


Sum of corrected areas: 23254068

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000918.D
Acq On : 19 Oct 2019 16:39
Operator : JU
Sample : K5321-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

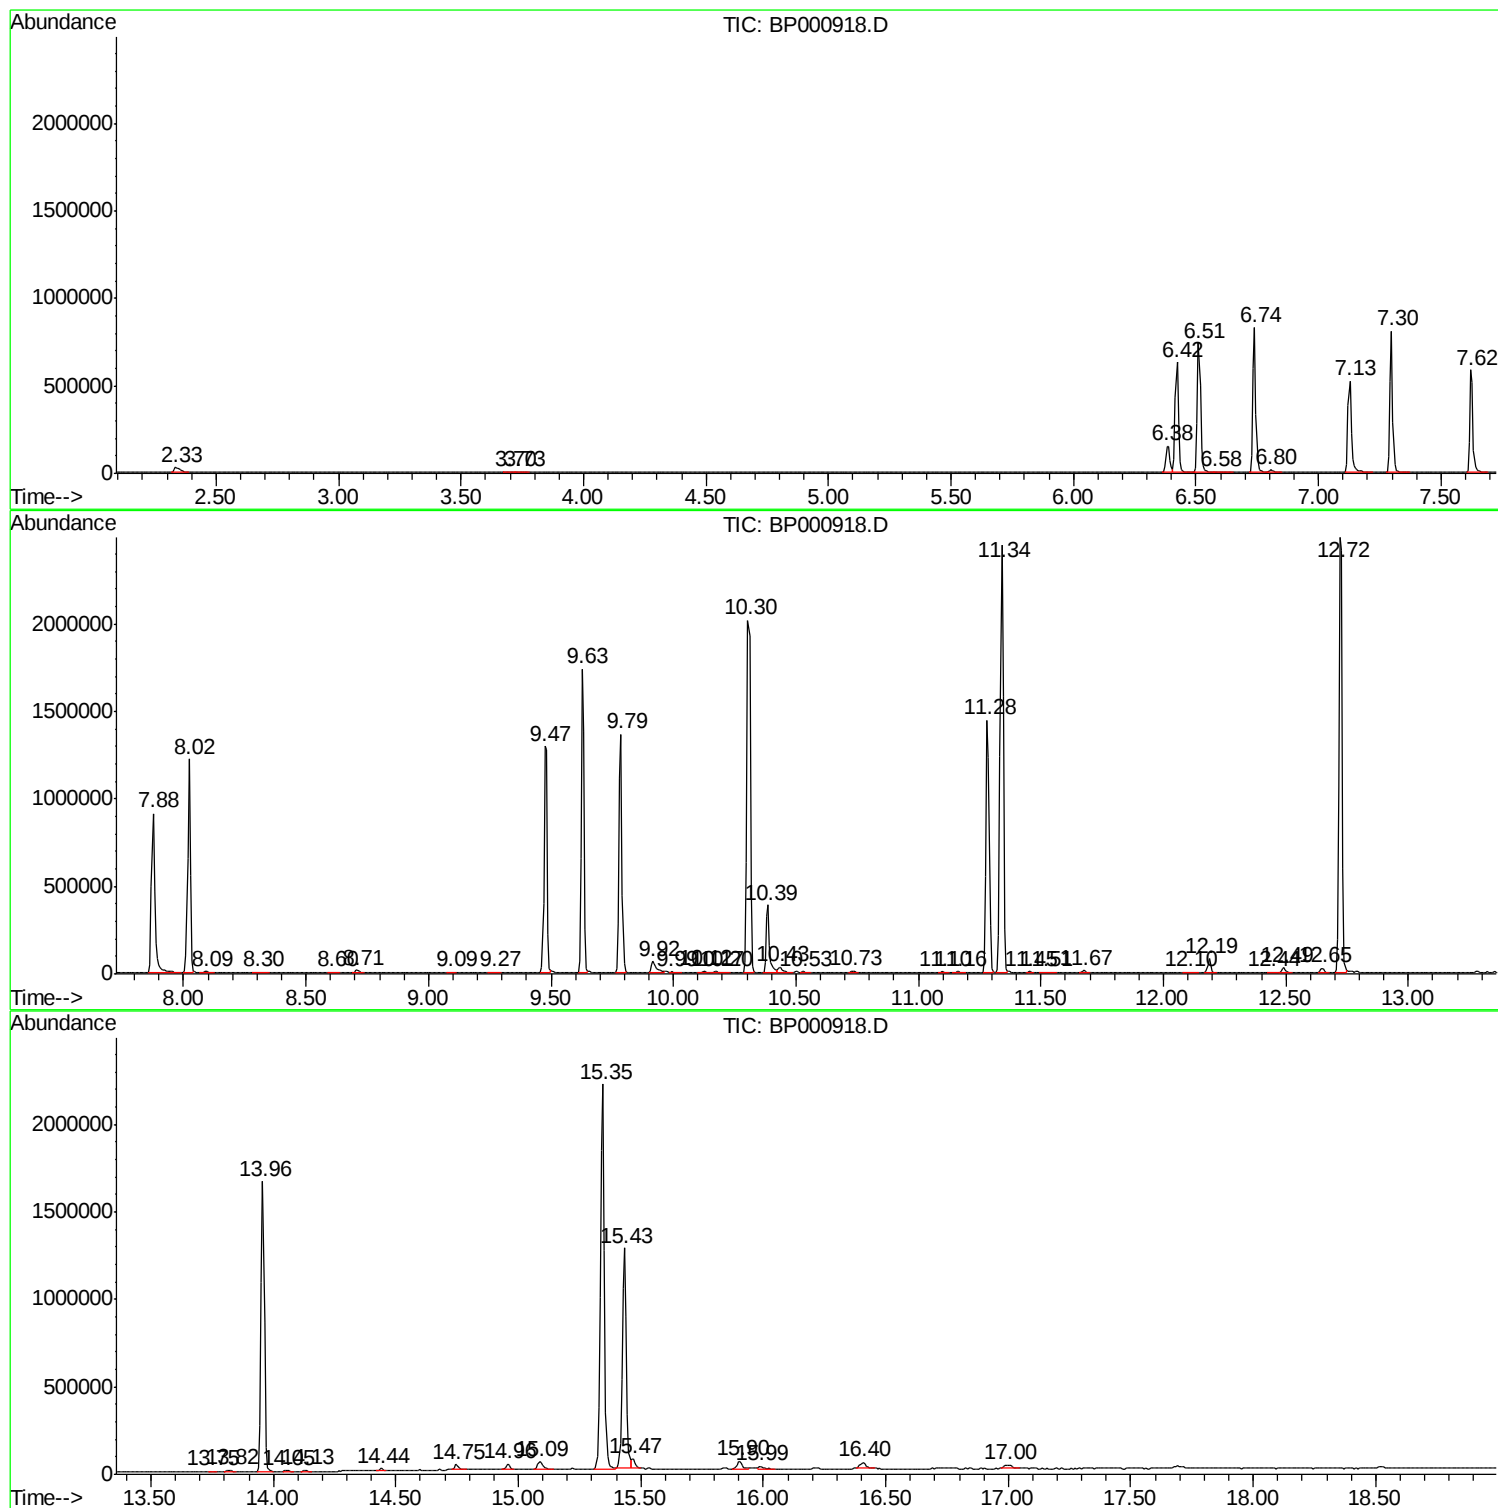

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000918.D
Acq On : 19 Oct 2019 16:39
Operator : JU
Sample : K5321-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000918.D
Acq On : 19 Oct 2019 16:39
Operator : JU
Sample : K5321-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0AB7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc