

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000922.D
 Acq On : 19 Oct 2019 18:15
 Operator : JU
 Sample : K5395-18
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0051

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	40	43	52	rBV	26807	38446	1.53%	0.158%
2	2.511	65	72	83	rVB	18828	29603	1.18%	0.122%
3	3.646	260	265	270	rBV3	2097	3607	0.14%	0.015%
4	3.699	270	274	277	rBV2	4815	7857	0.31%	0.032%
5	3.734	277	280	288	rVB	8056	13124	0.52%	0.054%
6	4.375	384	389	395	rBV	5940	7505	0.30%	0.031%
7	4.605	422	428	437	rVB9	1847	3525	0.14%	0.015%
8	5.322	544	550	558	rBV4	1874	3677	0.15%	0.015%
9	5.581	590	594	600	rBV2	2680	3918	0.16%	0.016%
10	6.381	727	730	734	rBV	173502	179787	7.16%	0.741%
11	6.422	734	737	749	rVV	716491	606945	24.17%	2.501%
12	6.511	749	752	767	rVB	840019	708491	28.22%	2.919%
13	6.740	787	791	806	rBV	854820	690773	27.51%	2.846%
14	7.128	853	857	873	rBV	584679	559908	22.30%	2.307%
15	7.299	882	886	889	rBV	923556	699968	27.88%	2.884%
16	7.622	938	941	955	rBV	708340	596040	23.74%	2.456%
17	7.875	981	984	1005	rBV	1050623	957727	38.14%	3.946%
18	8.022	1005	1009	1012	rBV	1204509	900991	35.88%	3.712%
19	8.087	1017	1020	1037	rVB	54252	58823	2.34%	0.242%
20	8.705	1122	1125	1130	rBV	16883	18446	0.73%	0.076%
21	9.258	1216	1219	1226	rVB3	10424	9257	0.37%	0.038%
22	9.481	1253	1257	1260	rBV	1556114	1282973	51.10%	5.286%
23	9.628	1279	1282	1286	rBV	1989053	1709739	68.09%	7.044%
24	9.710	1293	1296	1302	rVB4	1845	2607	0.10%	0.011%
25	9.787	1305	1309	1312	rBV	1379003	1131541	45.07%	4.662%
26	9.916	1328	1331	1342	rBV	65349	100898	4.02%	0.416%
27	9.993	1342	1344	1350	rVB6	4345	6468	0.26%	0.027%
28	10.199	1376	1379	1383	rBV2	2802	2603	0.10%	0.011%
29	10.310	1394	1398	1401	rBV	2244159	1991542	79.32%	8.206%
30	10.387	1407	1411	1417	rBV	374560	368325	14.67%	1.518%
31	10.434	1417	1419	1429	rVB	34822	37927	1.51%	0.156%
32	10.734	1467	1470	1474	rVB2	11009	9047	0.36%	0.037%
33	11.099	1529	1532	1536	rBV2	4706	3974	0.16%	0.016%
34	11.163	1539	1543	1552	rVV	4737	5541	0.22%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
 Data File : BP000922.D
 Acq On : 19 Oct 2019 18:15
 Operator : JU
 Sample : K5395-18
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0051

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	11.281	1560	1563	1567	rBV	1400069	1206515	48.05%	4.971%
36	11.340	1569	1573	1577	rBV	2504939	2077687	82.75%	8.560%
37	11.422	1585	1587	1590	rVB	4348	3710	0.15%	0.015%
38	11.675	1627	1630	1633	rBV3	4049	3365	0.13%	0.014%
39	11.751	1639	1643	1647	rBV3	2657	2692	0.11%	0.011%
40	11.851	1653	1660	1663	rBV3	1688	3027	0.12%	0.012%
41	12.446	1758	1761	1766	rBV6	1982	2557	0.10%	0.011%
42	12.493	1766	1769	1774	rBV	27765	24085	0.96%	0.099%
43	12.651	1792	1796	1801	rVB	22249	20053	0.80%	0.083%
44	12.722	1804	1808	1812	rBV	2462312	2364111	94.16%	9.741%
45	13.381	1916	1920	1925	rBV3	5850	7196	0.29%	0.030%
46	13.675	1966	1970	1972	rBV5	2304	3353	0.13%	0.014%
47	13.822	1991	1995	2000	rVB2	9652	13650	0.54%	0.056%
48	13.957	2014	2018	2031	rBV	1547835	1329061	52.93%	5.476%
49	14.051	2031	2034	2035	rBV	3635	3178	0.13%	0.013%
50	14.134	2045	2048	2051	rBV	6885	6542	0.26%	0.027%
51	14.440	2097	2100	2105	rBV2	15994	16371	0.65%	0.067%
52	14.728	2145	2149	2151	rBV	107641	124374	4.95%	0.512%
53	14.745	2151	2152	2159	rVB	47139	46872	1.87%	0.193%
54	14.957	2184	2188	2192	rBV	29390	31671	1.26%	0.130%
55	15.087	2206	2210	2218	rBV2	43441	58639	2.34%	0.242%
56	15.345	2248	2254	2263	rBV	2135308	2510835	100.00%	10.345%
57	15.434	2264	2269	2273	rBV	1212832	1417995	56.48%	5.842%
58	15.904	2344	2349	2355	rBV	43066	63348	2.52%	0.261%
59	15.992	2360	2364	2369	rVB6	11866	19127	0.76%	0.079%
60	16.404	2429	2434	2440	rBV	38266	70642	2.81%	0.291%
61	16.998	2530	2535	2542	rVB2	23828	45999	1.83%	0.190%
62	17.698	2649	2654	2665	rVB3	17041	42510	1.69%	0.175%


Sum of corrected areas: 24270768

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000922.D
Acq On : 19 Oct 2019 18:15
Operator : JU
Sample : K5395-18
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0051

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

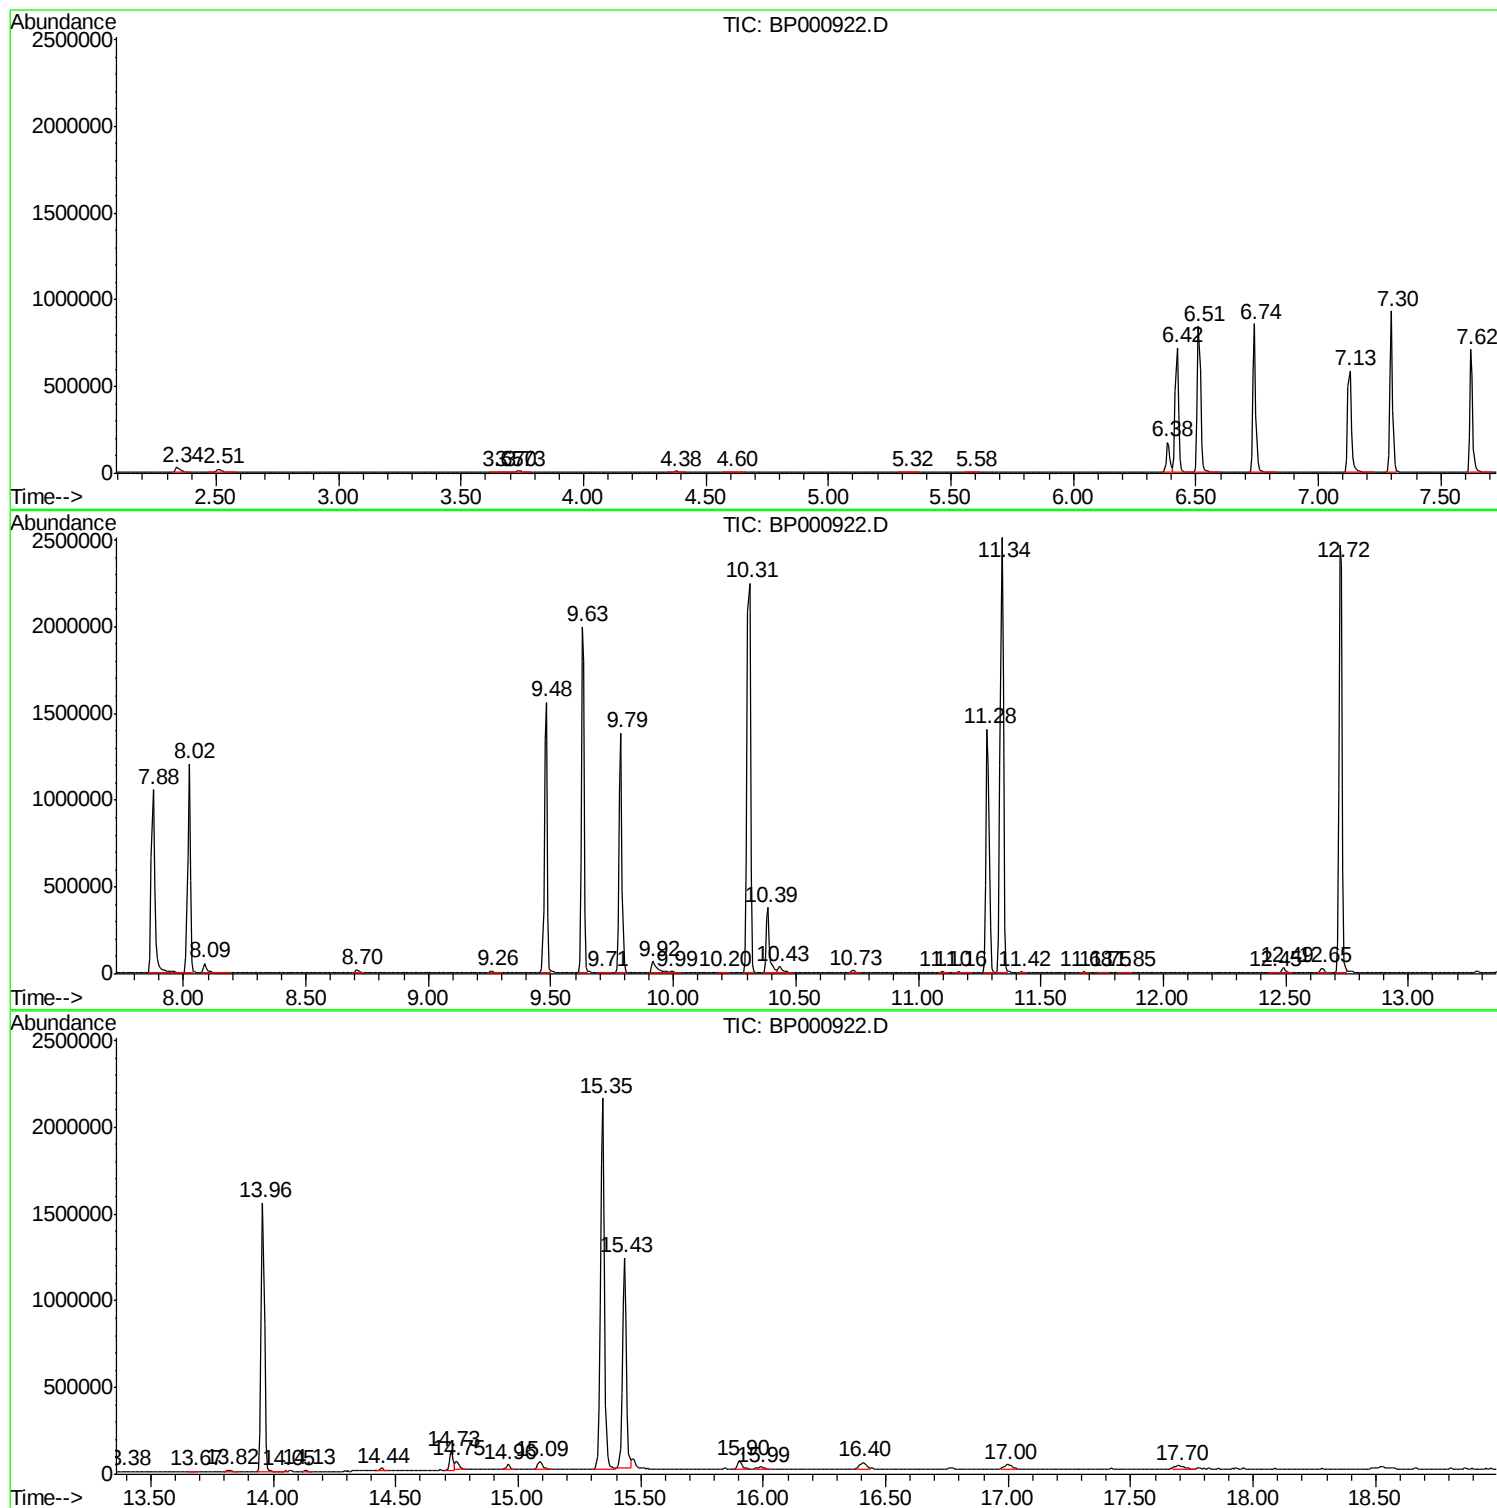

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000922.D
Acq On : 19 Oct 2019 18:15
Operator : JU
Sample : K5395-18
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0051

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000922.D
Acq On : 19 Oct 2019 18:15
Operator : JU
Sample : K5395-18
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0051

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc