

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000923.D
 Acq On : 19 Oct 2019 18:39
 Operator : JU
 Sample : K5395-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0052

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	40	43	57	rVB	24374	36663	1.50%	0.158%
2	2.505	66	71	81	rVB	14499	23201	0.95%	0.100%
3	3.699	268	274	276	rBV2	3340	5147	0.21%	0.022%
4	3.734	276	280	286	rVB	7157	11304	0.46%	0.049%
5	4.375	385	389	395	rBV	4953	5836	0.24%	0.025%
6	6.387	727	731	734	rBV	135273	148184	6.06%	0.637%
7	6.422	734	737	749	rVB	588790	507948	20.78%	2.184%
8	6.511	749	752	763	rBV	687434	584462	23.91%	2.513%
9	6.740	787	791	804	rVB	815628	661081	27.05%	2.842%
10	7.128	853	857	873	rBV	492671	466518	19.09%	2.006%
11	7.299	882	886	899	rVB	764170	599048	24.51%	2.575%
12	7.387	899	901	906	rVV4	2704	2607	0.11%	0.011%
13	7.469	910	915	920	rVV3	2904	3116	0.13%	0.013%
14	7.511	920	922	929	rVB6	1665	2521	0.10%	0.011%
15	7.622	938	941	958	rBV	570720	509013	20.83%	2.188%
16	7.875	981	984	1005	rBV	851826	813973	33.30%	3.499%
17	8.022	1005	1009	1012	rBV	1183146	881071	36.05%	3.788%
18	8.705	1122	1125	1138	rVB	14164	17333	0.71%	0.075%
19	9.269	1215	1221	1224	rBV5	2039	2939	0.12%	0.013%
20	9.481	1253	1257	1260	rBV	1369065	1198833	49.05%	5.154%
21	9.628	1279	1282	1286	rBV	1873973	1505547	61.60%	6.473%
22	9.705	1293	1295	1303	rVB6	1630	3026	0.12%	0.013%
23	9.787	1305	1309	1312	rBV	1323923	1132322	46.33%	4.868%
24	9.916	1328	1331	1343	rBV	61689	97511	3.99%	0.419%
25	9.993	1343	1344	1351	rVB6	3627	4240	0.17%	0.018%
26	10.199	1376	1379	1382	rBV2	2450	2495	0.10%	0.011%
27	10.305	1394	1397	1401	rBV	2077522	1851935	75.77%	7.962%
28	10.387	1407	1411	1417	rBV	355259	357933	14.64%	1.539%
29	10.434	1417	1419	1428	rVB	32713	34637	1.42%	0.149%
30	10.699	1459	1464	1467	rBV3	2991	4441	0.18%	0.019%
31	10.734	1467	1470	1474	rVB	8893	8145	0.33%	0.035%
32	11.099	1529	1532	1536	rBV2	4014	3651	0.15%	0.016%
33	11.163	1539	1543	1549	rVB	4497	5250	0.21%	0.023%
34	11.281	1560	1563	1567	rBV	1522493	1245019	50.94%	5.352%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000923.D
 Acq On : 19 Oct 2019 18:39
 Operator : JU
 Sample : K5395-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0052

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	11.340	1569	1573	1577	rBV	2446795	2004267	82.00%	8.617%
36	11.675	1627	1630	1634	rBV2	14096	11238	0.46%	0.048%
37	11.751	1640	1643	1648	rVB2	3510	3203	0.13%	0.014%
38	12.493	1765	1769	1773	rBV	26434	22789	0.93%	0.098%
39	12.651	1792	1796	1799	rVB	20696	18632	0.76%	0.080%
40	12.722	1804	1808	1812	rBV	2489750	2347937	96.07%	10.094%
41	13.375	1917	1919	1925	rVB7	2486	2540	0.10%	0.011%
42	13.428	1925	1928	1931	rBV5	2801	2793	0.11%	0.012%
43	13.669	1966	1969	1973	rBV4	3863	5869	0.24%	0.025%
44	13.751	1979	1983	1987	rBV	19426	21928	0.90%	0.094%
45	13.793	1987	1990	1992	rVV	29847	29041	1.19%	0.125%
46	13.822	1992	1995	2000	rVV	108642	94122	3.85%	0.405%
47	13.881	2002	2005	2009	rVB	4521	5266	0.22%	0.023%
48	13.957	2014	2018	2022	rBV	1591920	1394587	57.06%	5.996%
49	14.051	2031	2034	2035	rBV	3416	2783	0.11%	0.012%
50	14.134	2045	2048	2055	rVB	11594	11294	0.46%	0.049%
51	14.440	2097	2100	2105	rBV	21005	19961	0.82%	0.086%
52	14.728	2145	2149	2151	rBV	102940	123168	5.04%	0.530%
53	14.745	2151	2152	2164	rVB	54015	60886	2.49%	0.262%
54	14.957	2185	2188	2193	rVB	29142	28614	1.17%	0.123%
55	15.087	2206	2210	2218	rBV2	53781	68654	2.81%	0.295%
56	15.345	2248	2254	2263	rBV	2095212	2444103	100.00%	10.508%
57	15.434	2264	2269	2273	rVV	1218639	1473351	60.28%	6.334%
58	15.469	2273	2275	2285	rVB	65963	81787	3.35%	0.352%
59	15.904	2344	2349	2358	rBV	48816	75848	3.10%	0.326%
60	15.987	2361	2363	2370	rVB6	11138	16258	0.67%	0.070%
61	16.410	2430	2435	2442	rVB	36515	65863	2.69%	0.283%
62	17.004	2530	2536	2544	rVB3	23789	51919	2.12%	0.223%
63	17.692	2649	2653	2663	rVB3	14682	34873	1.43%	0.150%


Sum of corrected areas: 23260524

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000923.D
Acq On : 19 Oct 2019 18:39
Operator : JU
Sample : K5395-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
C0052

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

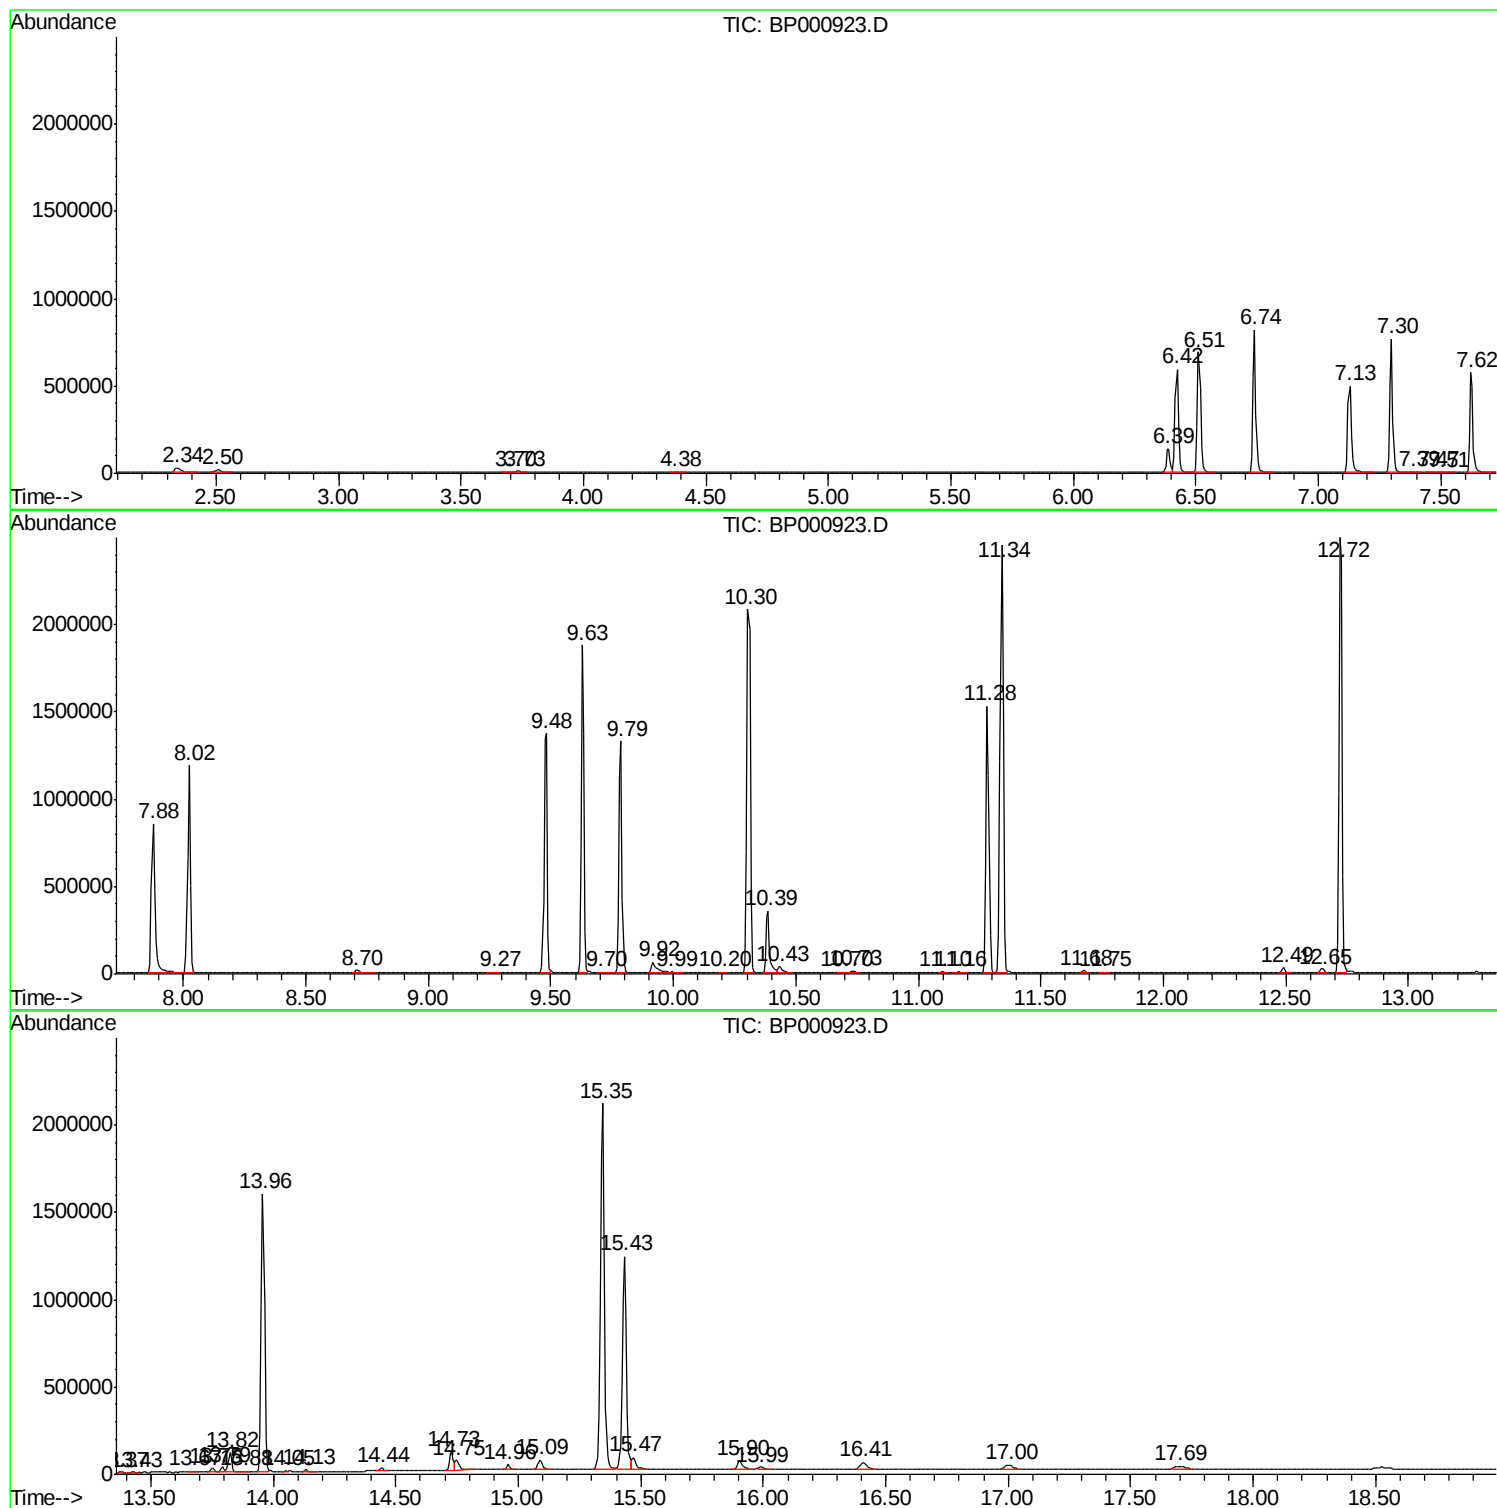

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000923.D
Acq On : 19 Oct 2019 18:39
Operator : JU
Sample : K5395-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0052

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000923.D
Acq On : 19 Oct 2019 18:39
Operator : JU
Sample : K5395-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0052

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc