

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
 Data File : BP000925.D
 Acq On : 19 Oct 2019 19:27
 Operator : JU
 Sample : PB123974BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.334	39	42	53	rBV	31135	46704	1.78%	0.167%
2	3.734	274	280	288	rBV2	3948	6936	0.26%	0.025%
3	6.381	726	730	734	rBV	901124	788306	29.99%	2.821%
4	6.422	734	737	749	rVV	785464	665775	25.33%	2.383%
5	6.510	749	752	767	rVB	1107987	906462	34.48%	3.244%
6	6.740	787	791	804	rBV	901028	722179	27.47%	2.585%
7	7.128	853	857	873	rBV	1188916	1051240	39.99%	3.762%
8	7.299	882	886	889	rBV	989747	748538	28.48%	2.679%
9	7.628	938	942	960	rBV	688435	633422	24.10%	2.267%
10	7.875	980	984	1006	rBV	1235906	1070031	40.70%	3.830%
11	8.022	1006	1009	1012	rVV	1292534	958557	36.46%	3.431%
12	8.087	1016	1020	1038	rVB	1116297	1011699	38.49%	3.621%
13	8.310	1055	1058	1068	rVB3	1836	3904	0.15%	0.014%
14	8.704	1122	1125	1137	rBV	17389	19360	0.74%	0.069%
15	9.375	1235	1239	1244	rBV4	3309	6982	0.27%	0.025%
16	9.481	1253	1257	1260	rBV	1680972	1360630	51.76%	4.870%
17	9.628	1279	1282	1286	rBV	1973110	1771008	67.37%	6.339%
18	9.787	1305	1309	1312	rBV	1479340	1205851	45.87%	4.316%
19	9.904	1326	1329	1343	rBV	401055	488015	18.56%	1.747%
20	9.998	1343	1345	1355	rVB5	8929	14369	0.55%	0.051%
21	10.310	1394	1398	1401	rBV	2385371	2060528	78.38%	7.375%
22	10.387	1407	1411	1417	rBV	414498	392512	14.93%	1.405%
23	10.434	1417	1419	1433	rVB	38300	43257	1.65%	0.155%
24	10.734	1467	1470	1476	rVB2	10989	9930	0.38%	0.036%
25	11.098	1524	1532	1536	rBV2	5007	5494	0.21%	0.020%
26	11.163	1539	1543	1547	rBV	4489	4939	0.19%	0.018%
27	11.281	1560	1563	1567	rBV	1539474	1319192	50.18%	4.721%
28	11.340	1569	1573	1577	rBV	2603046	2160046	82.17%	7.731%
29	11.504	1598	1601	1608	rVB2	2421	2775	0.11%	0.010%
30	12.440	1757	1760	1766	rBV6	2231	2838	0.11%	0.010%
31	12.492	1766	1769	1773	rBV	29059	25588	0.97%	0.092%
32	12.651	1792	1796	1801	rVB	24104	21998	0.84%	0.079%
33	12.722	1804	1808	1812	rBV	2575313	2507021	95.37%	8.973%
34	13.281	1900	1903	1909	rBV3	2544	3102	0.12%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000925.D
Acq On : 19 Oct 2019 19:27
Operator : JU
Sample : PB123974BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

35	13.816	1991	1994	2001	rVB2	6750	11037	0.42%	0.040%
36	13.957	2014	2018	2031	rBV	1760554	1492785	56.79%	5.343%
37	14.051	2031	2034	2039	rVB	2996	3950	0.15%	0.014%
38	14.134	2045	2048	2052	rVB2	4418	4165	0.16%	0.015%
39	14.439	2098	2100	2103	rBV	8312	7786	0.30%	0.028%
40	14.751	2150	2153	2157	rVB	17600	17549	0.67%	0.063%
41	14.957	2185	2188	2192	rBV	30600	29594	1.13%	0.106%
42	15.086	2207	2210	2218	rBV2	21718	33716	1.28%	0.121%
43	15.345	2248	2254	2263	rBV	2208041	2628749	100.00%	9.408%
44	15.434	2264	2269	2274	rBV	1304398	1569361	59.70%	5.617%
45	15.904	2344	2349	2356	rBV	21180	35477	1.35%	0.127%
46	15.992	2360	2364	2370	rVB4	13455	20458	0.78%	0.073%
47	16.410	2430	2435	2445	rVB2	17427	31109	1.18%	0.111%
48	16.998	2532	2535	2541	rVB2	9102	15312	0.58%	0.055%


Sum of corrected areas: 27940236

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101919\
Data File : BP000925.D
Acq On : 19 Oct 2019 19:27
Operator : JU
Sample : PB123974BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK74

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

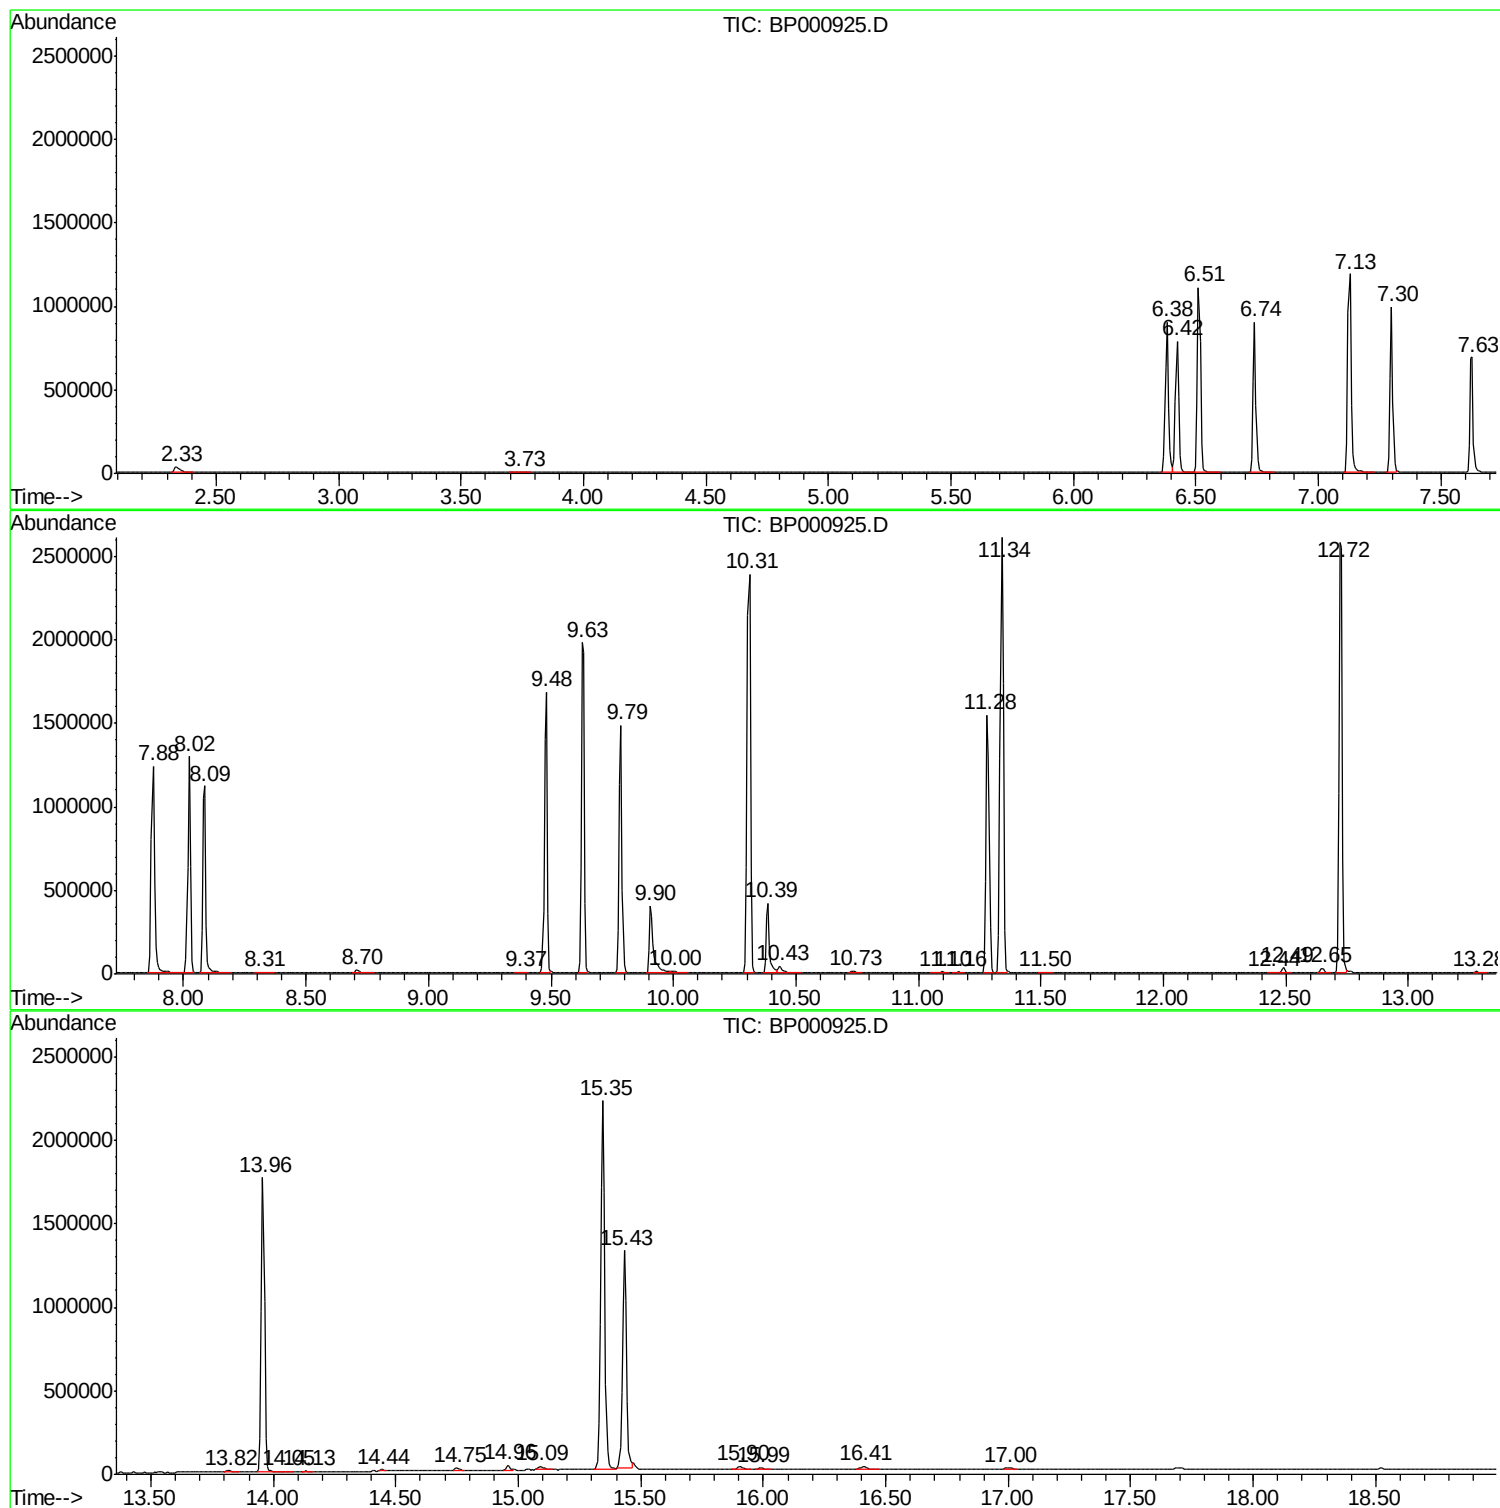

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000925.D
Acq On : 19 Oct 2019 19:27
Operator : JU
Sample : PB123974BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK74

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101919\
Data File : BP000925.D
Acq On : 19 Oct 2019 19:27
Operator : JU
Sample : PB123974BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK74

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc