
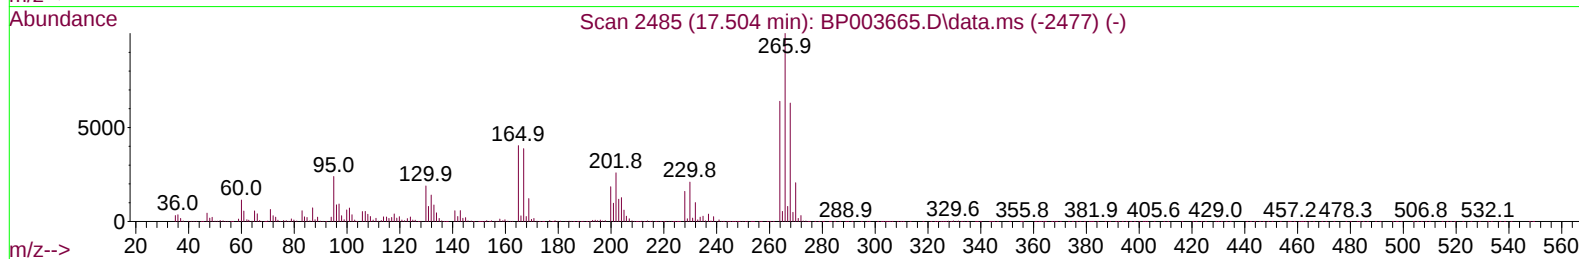
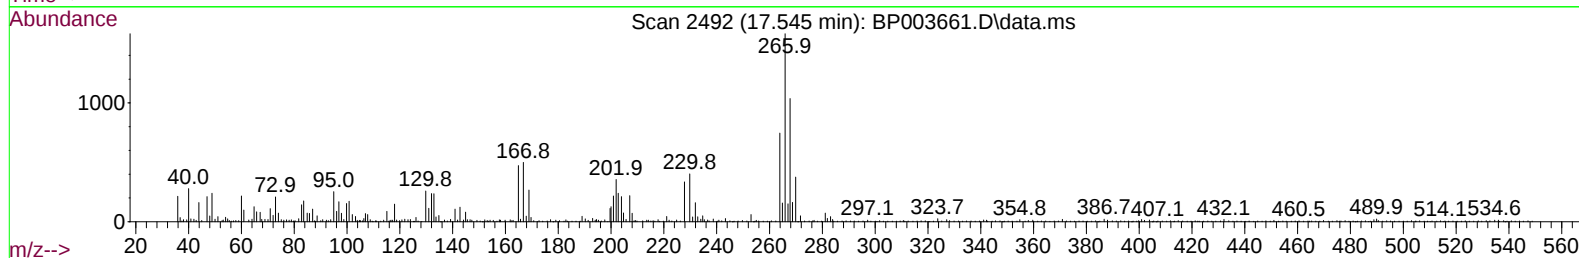


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101920\
Data File : BP003661.D
Acq On : 19 Oct 2020 09:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 17:45:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 14:54:24 2020
Response via : Initial Calibration

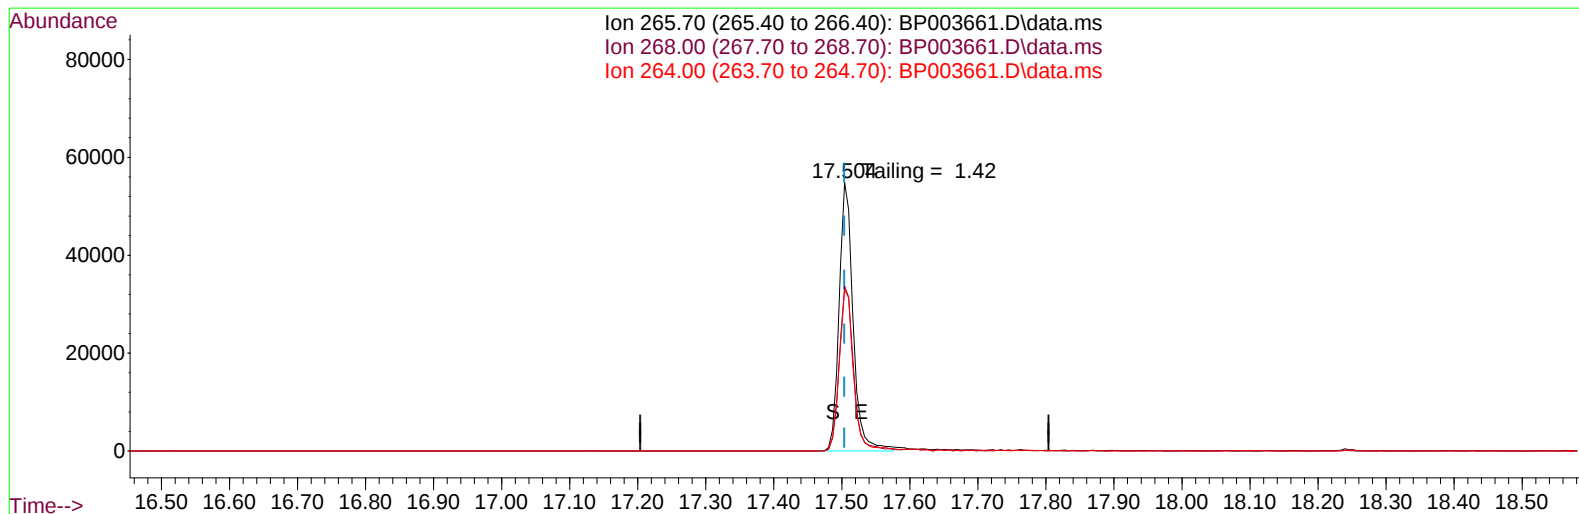

TIC: BP003661.D\data.ms

(70) Pentachlorophenol (C)




17.545min (+ 0.042) 7210.17 ng m

response 2030

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.55
264.00	63.30	47.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101920\
 Data File : BP003661.D
 Acq On : 19 Oct 2020 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 17:45:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 19 14:54:24 2020
 Response via : Initial Calibration

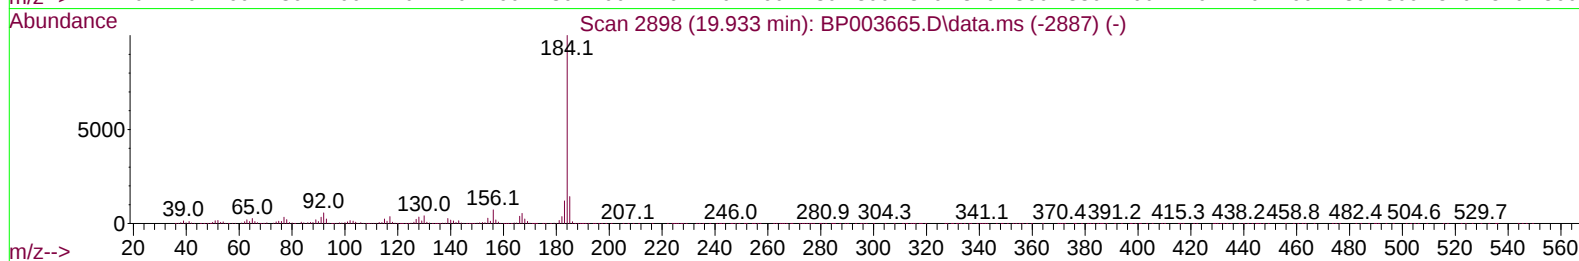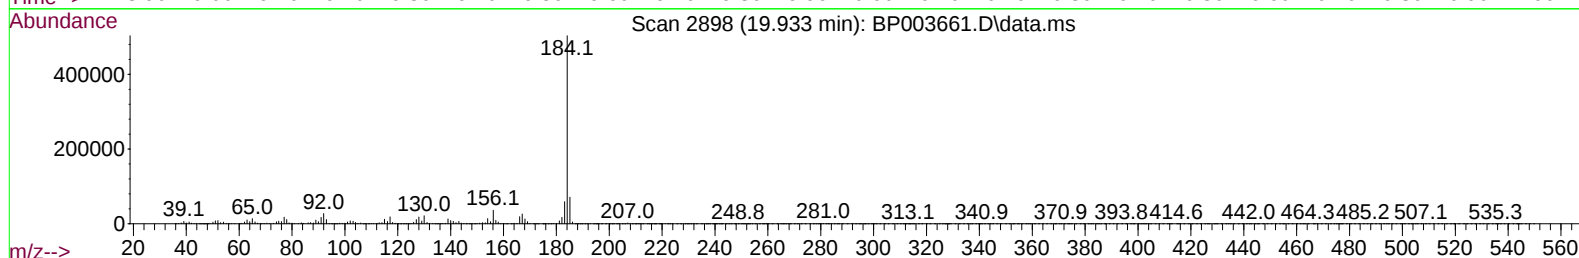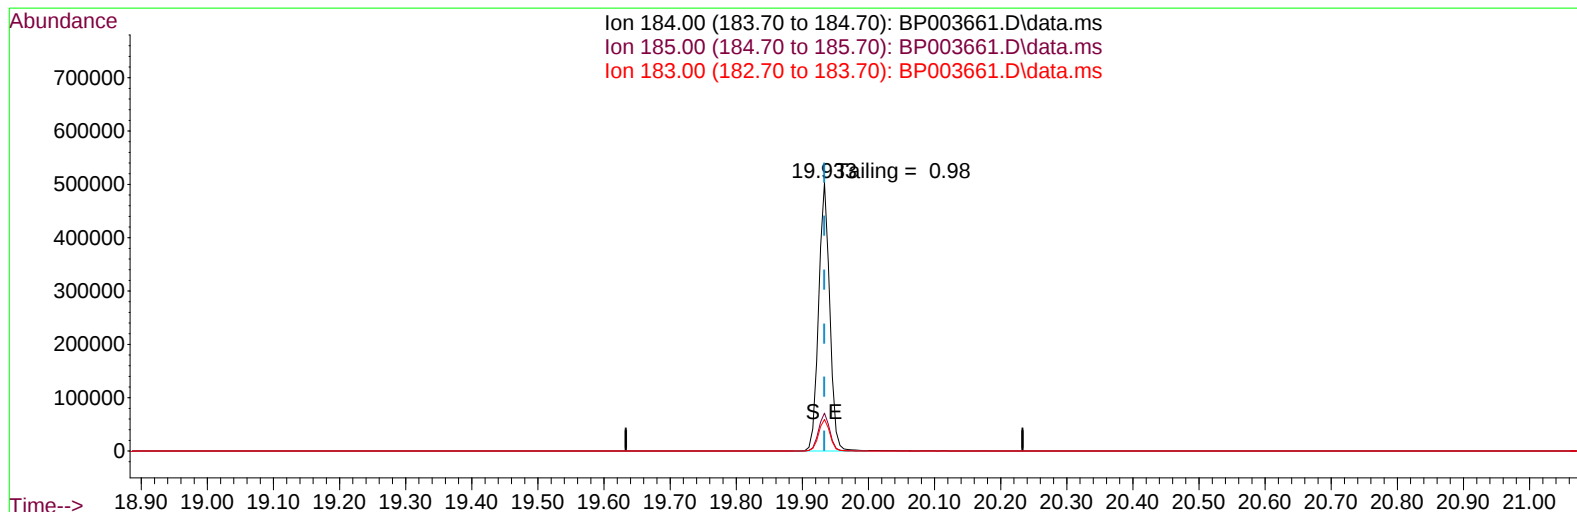

TIC: BP003661.D\data.ms

(77) Benzidine**19.933min (+ 0.000) 1115413.66 ng****response 587961**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	12.00	11.74
0.00	0.00	0.00