


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101920\
 Data File : BP003661.D
 Acq On : 19 Oct 2020 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 19 14:54:24 2020

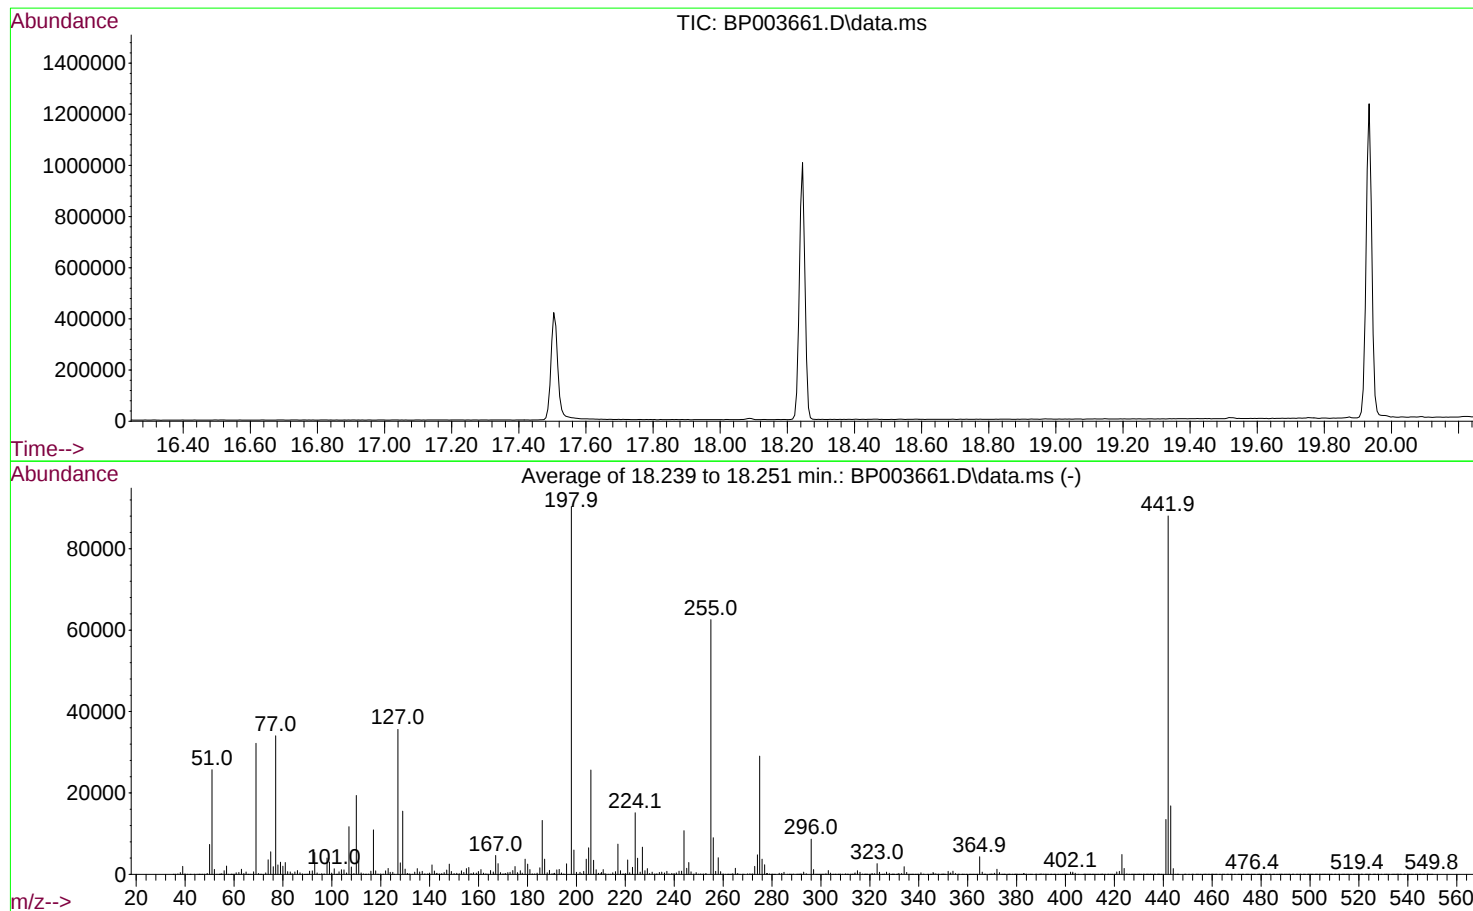

AutoFind: Scans 2610, 2611, 2612; Background Corrected with Scan 2603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	25701	PASS
68	69	0.00	2	2.0	644	PASS
69	198	0.00	100	35.6	32215	PASS
70	69	0.00	2	0.6	188	PASS
127	198	10	80	39.4	35635	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90378	PASS
199	198	5	9	6.6	5980	PASS
275	198	10	60	32.2	29065	PASS
365	198	1	100	4.8	4330	PASS
441	198	0.01	100	14.9	13503	PASS
442	198	50	100	97.4	88042	PASS
443	442	15	24	19.1	16824	PASS