

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101922\
 Data File : BP012205.D
 Acq On : 19 Oct 2022 15:15
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV602

Quant Time: Oct 20 00:55:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	359191	20.000	ng/u1	0.00
20) Naphthalene-d8	10.640	136	1592703	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.487	164	1036724	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	2182666	20.000	ng/u1	0.00
79) Chrysene-d12	21.339	240	2029712	20.000	ng/u1	0.00
88) Perylene-d12	23.751	264	1758864	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	66406	7.482	ng/uL	0.00
4) Pyridine-d5	3.681	84	457774	17.899	ng/u1	0.00
7) Phenol-d5	6.999	99	543588	17.530	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.164	67	380293	20.222	ng/u1	0.00
11) 2-Chlorophenol-d4	7.364	132	462843	19.609	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	468693	19.447	ng/u1	0.00
21) Nitrobenzene-d5	8.999	128	235242	19.954	ng/u1	0.00
24) 2-Nitrophenol-d4	9.722	143	254216	19.986	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.258	165	464181	19.455	ng/u1	0.00
31) 4-Chloroaniline-d4	10.781	131	676012	19.942	ng/u1	0.00
46) Dimethylphthalate-d6	13.899	166	1484841	20.590	ng/u1	0.00
49) Acenaphthylene-d8	14.175	160	1719260	20.886	ng/u1	0.00
54) 4-Nitrophenol-d4	14.698	143	264337	19.565	ng/u1	0.00
60) Fluorene-d10	15.481	176	1235671	19.917	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.610	200	233601	18.813	ng/u1	0.00
73) Anthracene-d10	17.345	188	1851941	19.357	ng/u1	0.00
81) Pyrene-d10	19.581	212	2183477	18.894	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.592	264	1689434	19.154	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.299	88	68602	7.182	ng/uL	99
5) Pyridine	3.705	79	416060	16.551	ng/u1	98
6) Benzaldehyde	6.975	77	377124	25.874	ng/u1	96
8) Phenol	7.028	94	592536	18.264	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.258	93	487080	18.602	ng/u1	99
12) 2-Chlorophenol	7.393	128	478178	18.776	ng/u1	99
13) 2-Methylphenol	8.281	108	454047	18.590	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.363	45	630872	18.118	ng/u1	99
16) Acetophenone	8.663	105	751188	20.178	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.646	70	368816	19.571	ng/u1	98
18) 4-Methylphenol	8.611	108	496653	18.672	ng/u1	96
19) Hexachloroethane	8.911	117	188825	18.770	ng/u1	95
22) Nitrobenzene	9.040	77	540521	18.818	ng/u1	98
23) Isophorone	9.569	82	1040935	18.881	ng/u1	99
25) 2-Nitrophenol	9.752	139	282770	19.567	ng/u1	99
26) 2,4-Dimethylphenol	9.816	107	539885	18.953	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.052	93	682838	18.920	ng/u1	99
29) 2,4-Dichlorophenol	10.287	162	474573	19.221	ng/u1	99
30) Naphthalene	10.687	128	1582144	18.574	ng/u1	100
32) 4-Chloroaniline	10.805	127	688206	19.669	ng/u1	99
33) Hexachlorobutadiene	10.969	225	300447	19.347	ng/u1	99
34) Caprolactam	11.605	113	149714	19.534	ng/u1	98
35) 4-Chloro-3-methylphenol	11.934	107	516491	19.376	ng/u1	99
36) 2-Methylnaphthalene	12.299	142	1126631	19.439	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101922\
 Data File : BP012205.D
 Acq On : 19 Oct 2022 15:15
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV602

Quant Time: Oct 20 00:55:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.522	142	1081002	18.680	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.669	216	606234	19.245	ng/ul	99
40) Hexachlorocyclopentadiene	12.646	237	289397	17.280	ng/ul	99
41) 2,4,6-Trichlorophenol	12.916	196	387835	19.077	ng/ul	98
42) 2,4,5-Trichlorophenol	12.987	196	421091	18.987	ng/ul	99
43) 1,1'-Biphenyl	13.316	154	1504298	19.509	ng/ul	99
44) 2-Chloronaphthalene	13.357	162	1141615	18.675	ng/ul	100
45) 2-Nitroaniline	13.569	65	313885	19.314	ng/ul	98
47) Dimethylphthalate	13.946	163	1444480	19.115	ng/ul	99
48) 2,6-Dinitrotoluene	14.069	165	310621	21.482	ng/ul	98
50) Acenaphthylene	14.204	152	1809920	19.733	ng/ul	100
51) 3-Nitroaniline	14.404	138	326351	21.382	ng/ul	94
52) Acenaphthene	14.551	153	1214530	18.724	ng/ul	99
53) 2,4-Dinitrophenol	14.610	184	152404	17.553	ng/ul	96
55) 4-Nitrophenol	14.710	109	193778	19.305	ng/ul	94
56) Dibenzofuran	14.887	168	1732625	19.512	ng/ul	98
57) 2,4-Dinitrotoluene	14.857	165	410669	19.900	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.116	232	370697	19.771	ng/ul	98
59) Diethylphthalate	15.310	149	1419107	19.107	ng/ul	99
61) Fluorene	15.540	166	1360998	19.346	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.534	204	685090	19.541	ng/ul	98
63) 4-Nitroaniline	15.569	138	327480	22.856	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.622	198	238371	18.287	ng/ul	94
67) N-Nitrosodiphenylamine	15.751	169	1203607	18.999	ng/ul	98
68) 4-Bromophenyl-phenylether	16.434	248	438802	18.988	ng/ul	100
69) Hexachlorobenzene	16.545	284	524708	19.262	ng/ul	98
70) Atrazine	16.710	200	435354	19.686	ng/ul	99
71) Pentachlorophenol	16.892	266	300571	18.279	ng/ul	100
72) Phenanthrene	17.287	178	2187173	18.644	ng/ul	99
74) Anthracene	17.381	178	2206158	19.007	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.281	216	595152	18.273	ng/ul	99
76) Pentachlorobenzene	14.804	250	603209	17.583	ng/ul	99
77) Carbazole	17.657	167	2036957	19.885	ng/ul	100
78) Di-n-butylphthalate	18.204	149	2427472	19.754	ng/ul	100
80) Fluoranthene	19.257	202	2527970	17.703	ng/ul	98
82) Pyrene	19.610	202	2617454	17.916	ng/ul	97
83) Butylbenzylphthalate	20.486	149	1049437	18.468	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.257	252	956912	21.646	ng/ul	99
85) Benzo(a)anthracene	21.322	228	2434357	18.402	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.245	149	1503463	18.885	ng/ul	99
87) Chrysene	21.375	228	2269215	18.382	ng/ul	100
89) Di-n-octyl phthalate	22.169	149	2373894	19.514	ng/ul	100
90) Benzo(b)fluoranthene	23.010	252	2209273	18.848	ng/ul	100
91) Benzo(k)fluoranthene	23.057	252	2181014	18.876	ng/ul	99
93) Benzo(a)pyrene	23.645	252	1870121	18.657	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.257	276	2144869	18.485	ng/ul	98
95) Dibenzo(a,h)anthracene	26.268	278	1902202	18.183	ng/ul	99
96) Benzo(g,h,i)perylene	27.027	276	1833272	16.827	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA P

ClientSampleId :

SICV602


Quant Time: Oct 20 00:55:51 2022


Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Oct 20 00:51:41 2022

Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 7.182 ng/uL
RT: 3.299 min Scan# 51
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion: 88 Resp: 68602
Ion Ratio Lower Upper
88 100
43 25.6 20.6 30.8
58 71.2 56.1 84.1

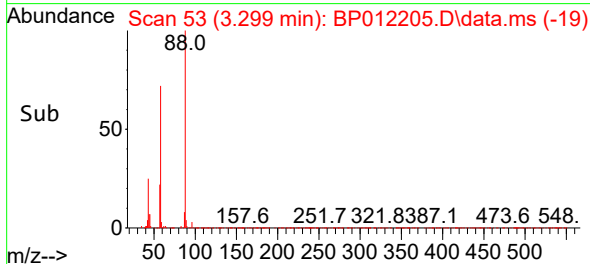

#5
Pyridine
Concen: 16.551 ng/uL
RT: 3.705 min Scan# 122
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion: 79 Resp: 416060
Ion Ratio Lower Upper
79 100
52 72.0 59.4 89.2
51 33.0 26.5 39.7


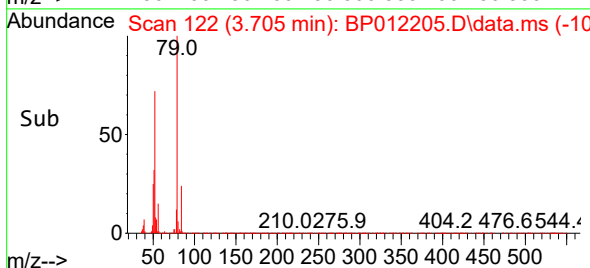
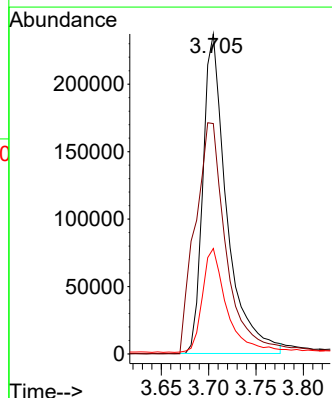
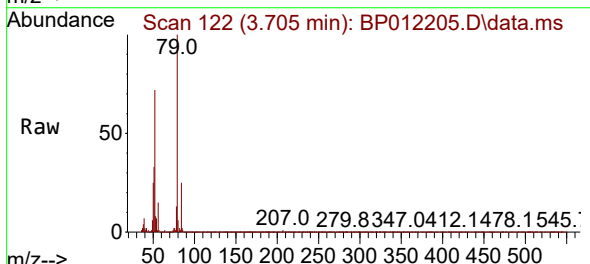




#6
Benzaldehyde
Concen: 25.874 ng/ul
RT: 6.975 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion: 77 Resp: 377124
Ion Ratio Lower Upper
77 100
105 103.3 79.0 118.6
106 98.5 76.4 114.6



#8
Phenol
Concen: 18.264 ng/ul
RT: 7.028 min Scan# 687
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion: 94 Resp: 592536
Ion Ratio Lower Upper
94 100
65 26.0 20.6 31.0
66 34.3 26.2 39.4

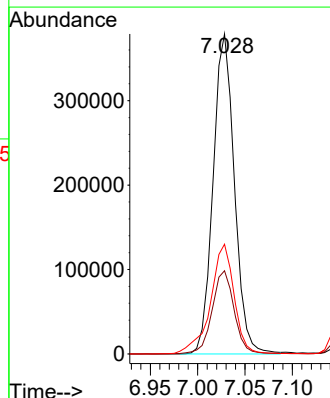







#10
 Bis(2-Chloroethyl)ether
 Concen: 18.602 ng/ul
 RT: 7.258 min Scan# 726
 Delta R.T. 0.000 min
 Lab File: BP012205.D
 Acq: 19 Oct 2022 15:15

Instrument :
 BNA_P
 ClientSampleId :
 SICV602

Tgt Ion: 93 Resp: 487080




Ion	Ratio	Lower	Upper
93	100		
63	75.9	60.2	90.2
95	32.6	26.1	39.1




#12
 2-Chlorophenol
 Concen: 18.776 ng/ul
 RT: 7.393 min Scan# 749
 Delta R.T. 0.000 min
 Lab File: BP012205.D
 Acq: 19 Oct 2022 15:15

Tgt Ion:128 Resp: 478178

Ion	Ratio	Lower	Upper
128	100		
64	44.8	35.4	53.2
130	32.4	26.1	39.1









#13
2-Methylphenol
Concen: 18.590 ng/ul
RT: 8.281 min Scan# 900
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:108 Resp: 454047
Ion Ratio Lower Upper
108 100
107 90.3 71.1 106.7



#14
2,2'-oxybis(1-Chloropropane)
Concen: 18.118 ng/ul
RT: 8.363 min Scan# 914
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion: 45 Resp: 630872
Ion Ratio Lower Upper
45 100
77 15.7 12.1 18.1
79 11.8 9.3 13.9




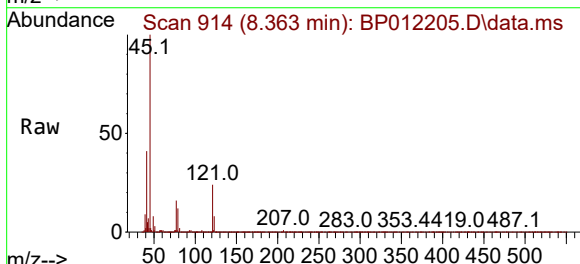




#16
Acetophenone
Concen: 20.178 ng/ul
RT: 8.663 min Scan# 965
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:105 Resp: 751188
Ion Ratio Lower Upper
105 100
77 74.1 60.0 90.0
51 23.4 20.1 30.1



#17
N-Nitroso-di-n-propylamine
Concen: 19.571 ng/ul
RT: 8.646 min Scan# 962
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion: 70 Resp: 368816
Ion Ratio Lower Upper
70 100
42 50.8 42.4 63.6
101 9.9 7.6 11.4
130 21.7 17.3 25.9









#18
4-Methylphenol
Concen: 18.672 ng/ul
RT: 8.611 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:108 Resp: 496653
Ion Ratio Lower Upper
108 100
107 112.2 86.6 130.0



#19
Hexachloroethane
Concen: 18.770 ng/ul
RT: 8.911 min Scan# 1007
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:117 Resp: 188825
Ion Ratio Lower Upper
117 100
201 105.1 79.7 119.5
199 66.8 50.7 76.1



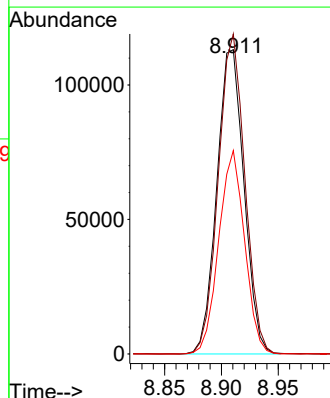





#22
Nitrobenzene
Concen: 18.818 ng/ul
RT: 9.040 min Scan# 1029
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion: 77 Resp: 540521
Ion Ratio Lower Upper
77 100
123 47.9 37.1 55.7
65 13.0 10.0 15.0



#23
Isophorone
Concen: 18.881 ng/ul
RT: 9.569 min Scan# 1119
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion: 82 Resp: 1040935
Ion Ratio Lower Upper
82 100
95 7.0 5.4 8.0
138 17.6 14.5 21.7









#25
2-Nitrophenol
Concen: 19.567 ng/ul
RT: 9.752 min Scan# 1150
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:139 Resp: 282770
Ion Ratio Lower Upper
139 100
65 47.2 38.0 57.0
109 28.3 21.6 32.4



#26
2,4-Dimethylphenol
Concen: 18.953 ng/ul
RT: 9.816 min Scan# 1161
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:107 Resp: 539885
Ion Ratio Lower Upper
107 100
121 52.2 40.6 60.8
122 86.2 71.0 106.6









#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.920 ng/ul
 RT: 10.052 min Scan# 1201
 Delta R.T. 0.000 min
 Lab File: BP012205.D
 Acq: 19 Oct 2022 15:15




Instrument :
 BNA_P
 ClientSampleId :
 SICV602


Tgt Ion: 93 Resp: 682838
 Ion Ratio Lower Upper
 93 100
 95 33.0 26.2 39.4
 123 11.6 9.0 13.6



#29
 2,4-Dichlorophenol
 Concen: 19.221 ng/ul
 RT: 10.287 min Scan# 1241
 Delta R.T. 0.006 min
 Lab File: BP012205.D
 Acq: 19 Oct 2022 15:15

Tgt Ion:162 Resp: 474573
 Ion Ratio Lower Upper
 162 100
 164 64.7 51.2 76.8
 98 36.3 28.3 42.5




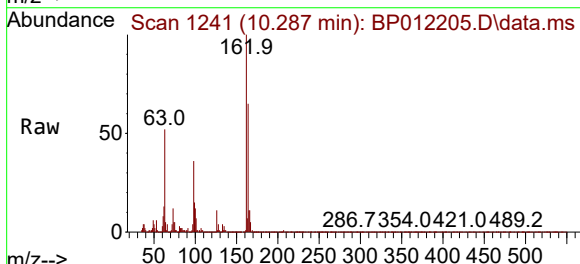




#30
Naphthalene
Concen: 18.574 ng/ul
RT: 10.687 min Scan# 1308
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:128 Resp: 1582144
Ion Ratio Lower Upper
128 100
129 10.9 8.8 13.2
127 12.9 10.2 15.4



#32
4-Chloroaniline
Concen: 19.669 ng/ul
RT: 10.805 min Scan# 1329
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:127 Resp: 688206
Ion Ratio Lower Upper
127 100
129 32.3 25.6 38.4

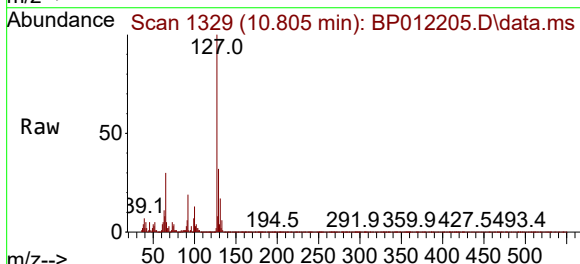



#33

Hexachlorobutadiene

Concen: 19.347 ng/ul

RT: 10.969 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:225 Resp: 300447

Ion Ratio Lower Upper

225 100

223 62.1 50.2 75.4

227 63.5 51.9 77.9



#34

Caprolactam

Concen: 19.534 ng/ul

RT: 11.605 min Scan# 1465

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:113 Resp: 149714


Ion Ratio Lower Upper

113 100

55 163.3 133.7 200.5

56 117.5 95.4 143.2


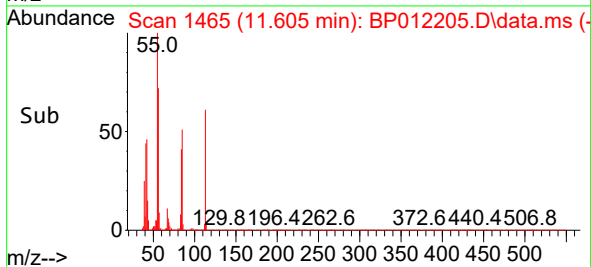

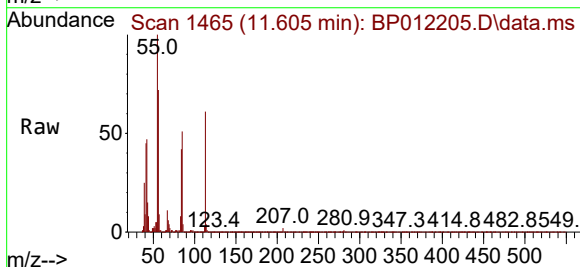




#35
4-Chloro-3-methylphenol
Concen: 19.376 ng/ul
RT: 11.934 min Scan# 1521
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:107 Resp: 516491
Ion Ratio Lower Upper
107 100
144 26.8 21.2 31.8
142 83.0 65.5 98.3

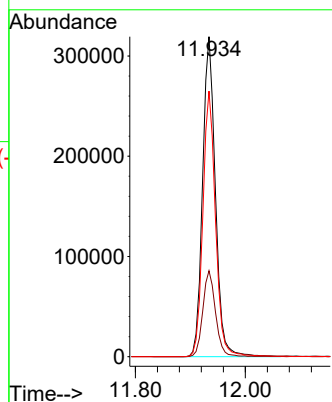

#36
2-Methylnaphthalene
Concen: 19.439 ng/ul
RT: 12.299 min Scan# 1583
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:142 Resp: 1126631
Ion Ratio Lower Upper
142 100
141 88.1 70.3 105.5





#37

1-Methylnaphthalene

Concen: 18.680 ng/ul

RT: 12.522 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:142 Resp: 1081002

Ion Ratio Lower Upper

142 100

141 91.1 73.4 110.0

116 3.8 3.0 4.4



#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.245 ng/ul

RT: 12.669 min Scan# 1646

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Tgt Ion:216 Resp: 606234




Ion Ratio Lower Upper


216 100

214 77.1 62.5 93.7

179 20.0 16.5 24.7

108 16.3 13.4 20.0

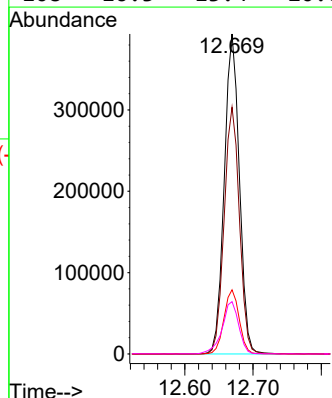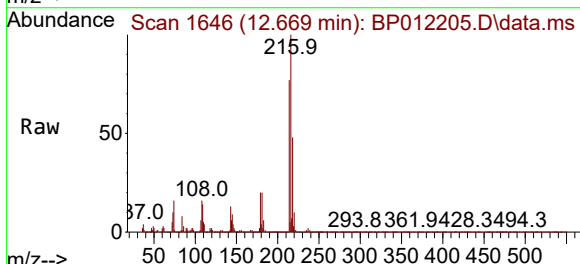



#40

Hexachlorocyclopentadiene

Concen: 17.280 ng/ul

RT: 12.646 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:237 Resp: 289397

Ion Ratio Lower Upper

237 100

235 62.0 49.4 74.0

272 12.5 10.5 15.7

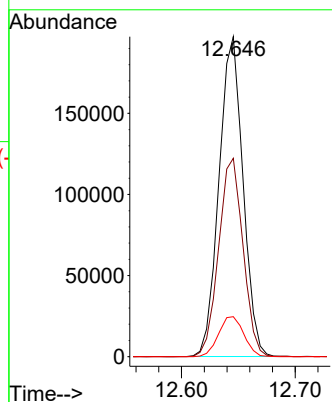

#41

2,4,6-Trichlorophenol

Concen: 19.077 ng/ul

RT: 12.916 min Scan# 1688

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:196 Resp: 387835


Ion Ratio Lower Upper

196 100

198 95.0 77.4 116.2

200 31.4 24.6 36.8









#42
2,4,5-Trichlorophenol
Concen: 18.987 ng/ul
RT: 12.987 min Scan# 1699
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:196 Resp: 421091
Ion Ratio Lower Upper
196 100
198 95.1 76.2 114.2
200 32.0 24.7 37.1



#43
1,1'-Biphenyl
Concen: 19.509 ng/ul
RT: 13.316 min Scan# 1756
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:154 Resp: 1504298
Ion Ratio Lower Upper
154 100
153 39.7 31.5 47.3
76 12.9 11.0 16.4


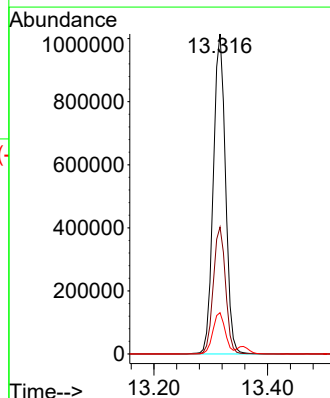

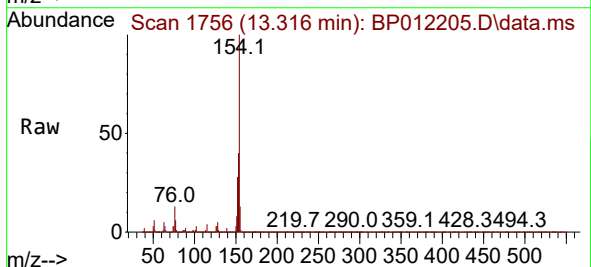




#44
2-Chloronaphthalene
Concen: 18.675 ng/ul
RT: 13.357 min Scan# 1762
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:162 Resp: 1141615
Ion Ratio Lower Upper
162 100
164 32.8 26.1 39.1
127 38.4 30.8 46.2

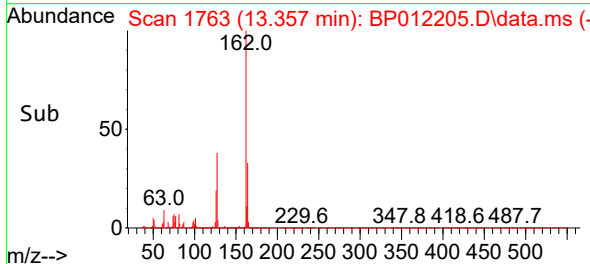

#45
2-Nitroaniline
Concen: 19.314 ng/ul
RT: 13.569 min Scan# 1799
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion: 65 Resp: 313885
Ion Ratio Lower Upper
65 100
92 73.6 57.5 86.3
138 112.7 92.5 138.7


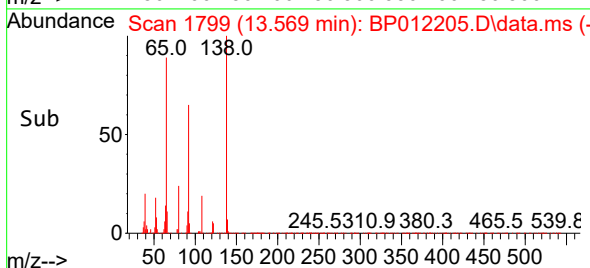
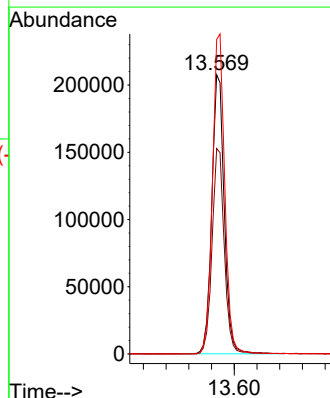
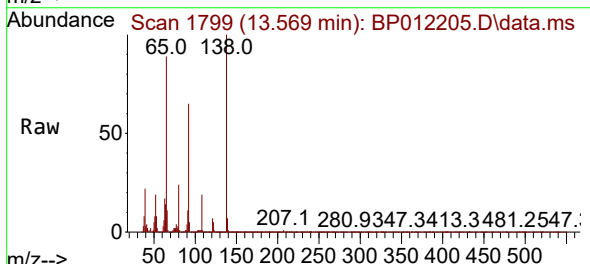




#47
Dimethylphthalate
Concen: 19.115 ng/ul
RT: 13.946 min Scan# 1863
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:163 Resp: 1444480
Ion Ratio Lower Upper
163 100
194 4.0 3.0 4.6
164 10.3 8.1 12.1



#48
2,6-Dinitrotoluene
Concen: 21.482 ng/ul
RT: 14.069 min Scan# 1884
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:165 Resp: 310621
Ion Ratio Lower Upper
165 100
89 56.8 43.9 65.9
121 21.3 17.1 25.7




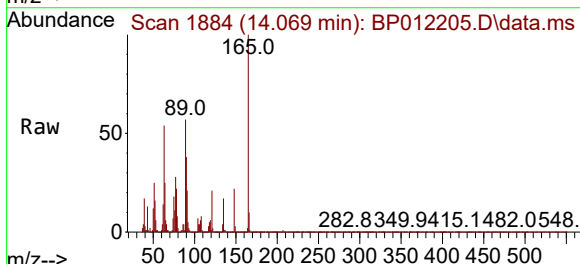




#50
Acenaphthylene
Concen: 19.733 ng/ul
RT: 14.204 min Scan# 1907
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:152 Resp: 1809920
Ion Ratio Lower Upper
152 100
151 19.8 15.8 23.8
153 13.1 10.6 16.0

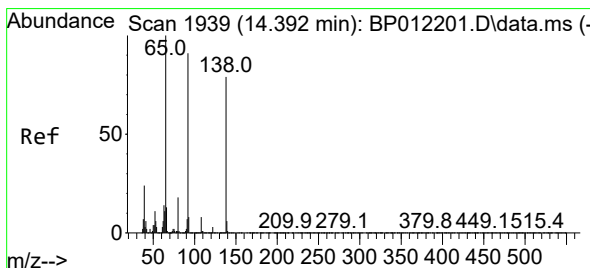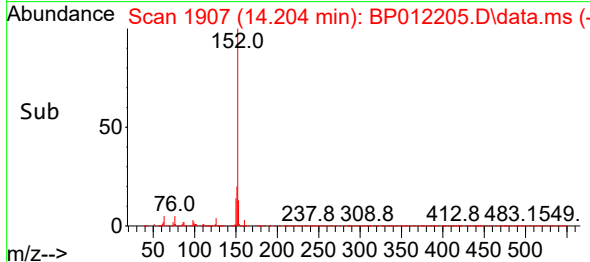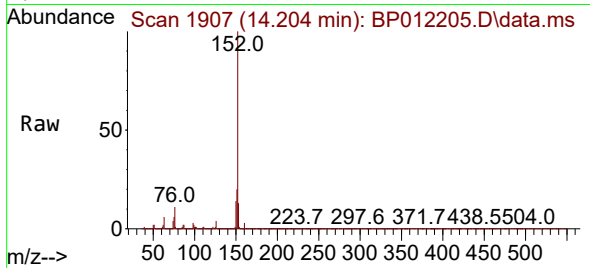

#51
3-Nitroaniline
Concen: 21.382 ng/ul
RT: 14.404 min Scan# 1941
Delta R.T. 0.012 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:138 Resp: 326351
Ion Ratio Lower Upper
138 100
108 10.3 8.2 12.2
92 109.1 93.1 139.7

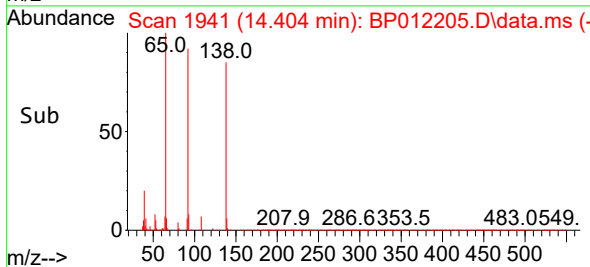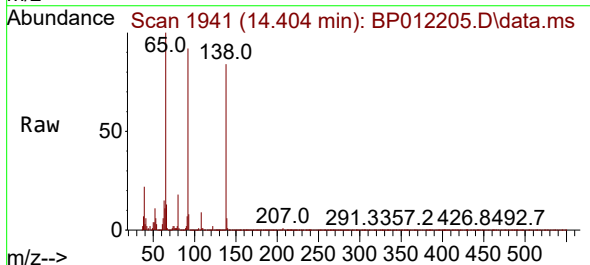



#52

Acenaphthene

Concen: 18.724 ng/ul

RT: 14.551 min Scan# 1966

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:153 Resp: 1214530

Ion Ratio Lower Upper

153 100

152 48.4 38.1 57.1

154 88.8 71.4 107.2

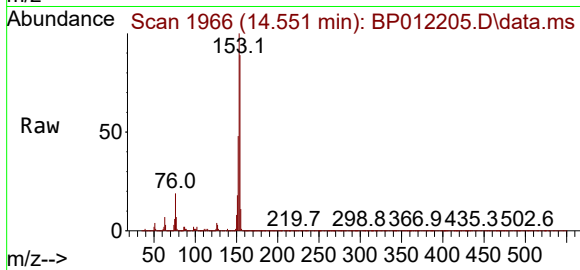

#53

2,4-Dinitrophenol

Concen: 17.553 ng/ul

RT: 14.610 min Scan# 1976

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:184 Resp: 152404


Ion Ratio Lower Upper

184 100

63 60.4 51.1 76.7

154 61.5 47.2 70.8



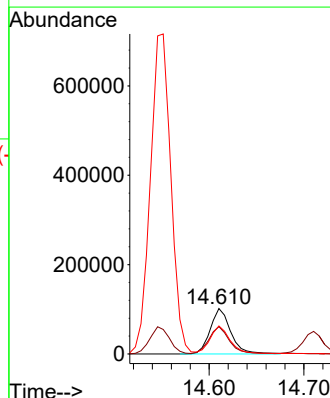
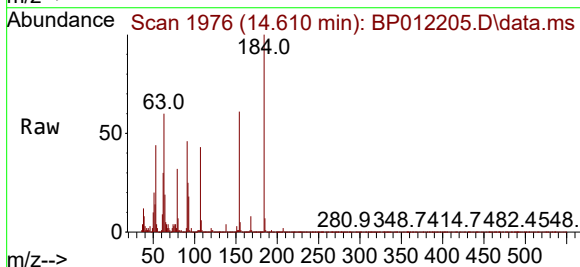




#55
4-Nitrophenol
Concen: 19.305 ng/ul
RT: 14.710 min Scan# 1993
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:109 Resp: 193778
Ion Ratio Lower Upper
109 100
139 140.4 118.5 177.7
65 131.7 110.5 165.7



#56
Dibenzofuran
Concen: 19.512 ng/ul
RT: 14.887 min Scan# 2023
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:168 Resp: 1732625
Ion Ratio Lower Upper
168 100
139 37.2 29.0 43.4

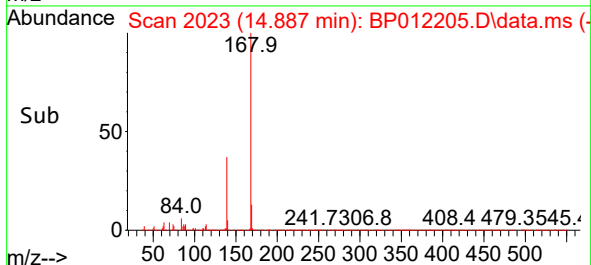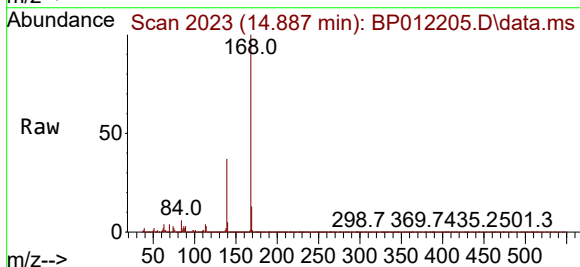



#57

2,4-Dinitrotoluene

Concen: 19.900 ng/ul

RT: 14.857 min Scan# 2017

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:165 Resp: 410669

Ion Ratio Lower Upper

165 100

63 42.2 34.1 51.1

182 2.9 2.1 3.1



#58

2,3,4,6-Tetrachlorophenol

Concen: 19.771 ng/ul

RT: 15.116 min Scan# 2062

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Tgt Ion:232 Resp: 370697




Ion Ratio Lower Upper


232 100

131 42.3 35.0 52.4

130 2.4 1.8 2.8

166 28.5 23.5 35.3

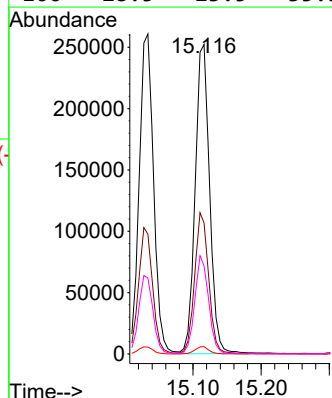



#59

Diethylphthalate

Concen: 19.107 ng/ul

RT: 15.310 min Scan# 2095

Delta R.T. 0.000 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:149 Resp: 1419107

Ion Ratio Lower Upper

149 100

177 22.1 17.9 26.9

150 12.7 10.1 15.1

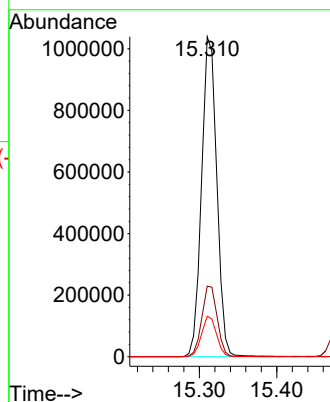

#61

Fluorene

Concen: 19.346 ng/ul

RT: 15.540 min Scan# 2134

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:166 Resp: 1360998


Ion Ratio Lower Upper

166 100

165 97.7 78.0 117.0

167 13.0 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 19.541 ng/ul
RT: 15.534 min Scan# 2132
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:204 Resp: 685090
Ion Ratio Lower Upper
204 100
206 32.3 26.6 39.8
141 58.3 45.3 67.9



#63
4-Nitroaniline
Concen: 22.856 ng/ul
RT: 15.569 min Scan# 2139
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:138 Resp: 327480
Ion Ratio Lower Upper
138 100
92 49.7 41.6 62.4
108 71.6 57.0 85.6



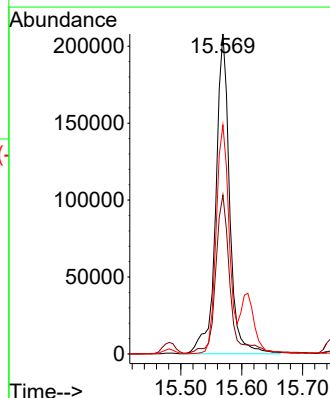
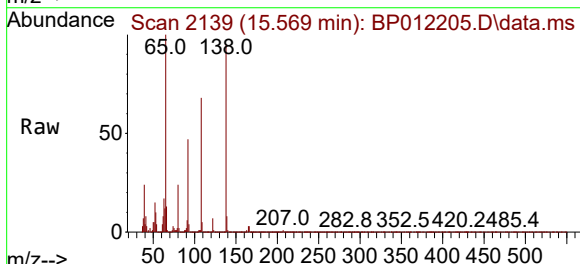




#66
4,6-Dinitro-2-methylphenol
Concen: 18.287 ng/ul
RT: 15.622 min Scan# 2148
Delta R.T. 0.000 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:198 Resp: 238371
Ion Ratio Lower Upper
198 100
182 5.2 3.8 5.6
77 25.3 17.8 26.6

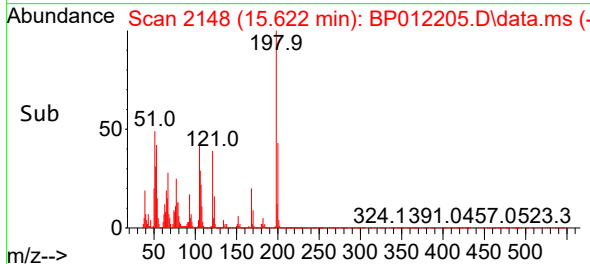

#67
N-Nitrosodiphenylamine
Concen: 18.999 ng/ul
RT: 15.751 min Scan# 2170
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:169 Resp: 1203607
Ion Ratio Lower Upper
169 100
168 64.8 53.4 80.0
167 36.0 29.2 43.8


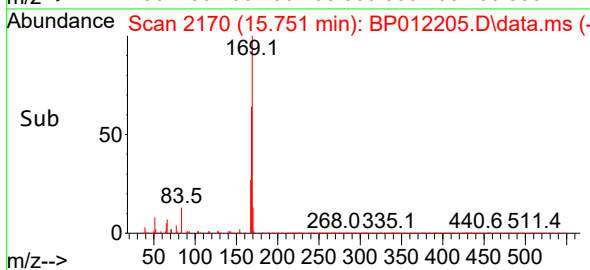

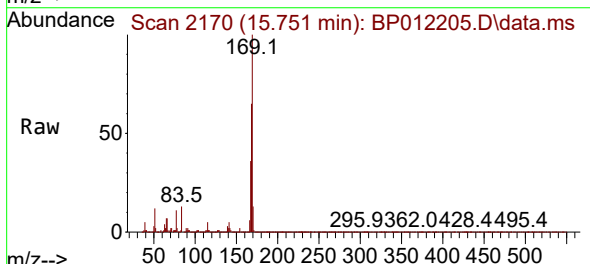




#68
4-Bromophenyl-phenylether
Concen: 18.988 ng/ul
RT: 16.434 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:248 Resp: 438802
Ion Ratio Lower Upper
248 100
250 98.6 79.0 118.4
141 69.3 55.1 82.7

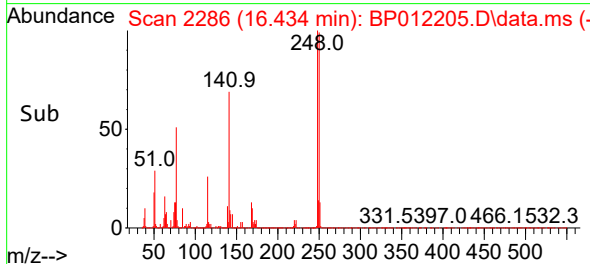

#69
Hexachlorobenzene
Concen: 19.262 ng/ul
RT: 16.545 min Scan# 2305
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:284 Resp: 524708
Ion Ratio Lower Upper
284 100
142 30.3 25.5 38.3
249 28.7 23.6 35.4

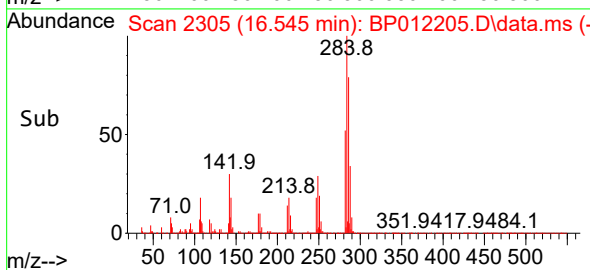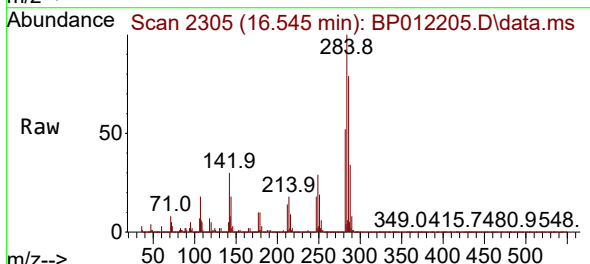



#70

Atrazine

Concen: 19.686 ng/ul

RT: 16.710 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:200 Resp: 435354

Ion Ratio Lower Upper

200 100

173 25.9 21.4 32.0

215 47.0 38.2 57.2



#71

Pentachlorophenol

Concen: 18.279 ng/ul

RT: 16.892 min Scan# 2364

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:266 Resp: 300571


Ion Ratio Lower Upper

266 100

264 62.6 50.1 75.1

268 62.8 50.6 76.0

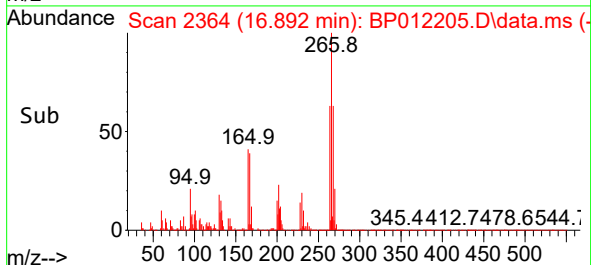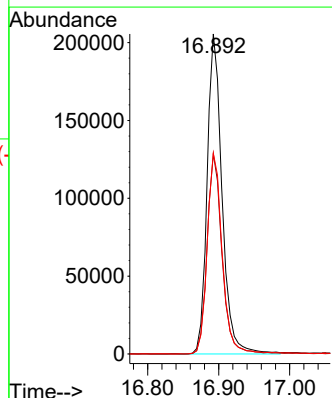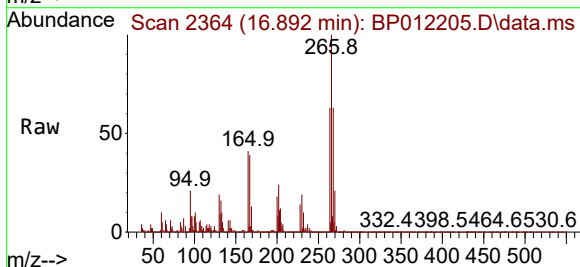

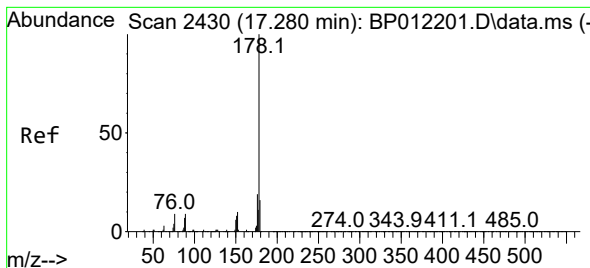

#72

Phenanthrene

Concen: 18.644 ng/ul

RT: 17.287 min Scan# 2430

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:178 Resp: 2187173

Ion Ratio Lower Upper

178 100

179 15.5 12.6 18.8

176 19.1 15.6 23.4

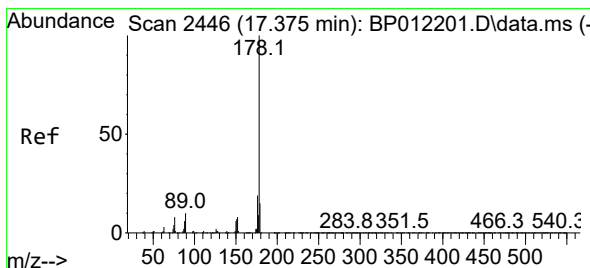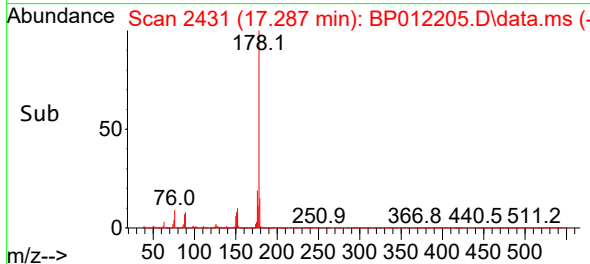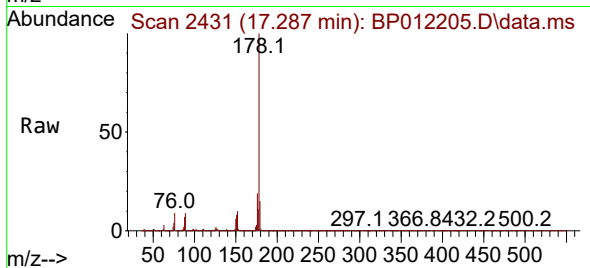

#74

Anthracene

Concen: 19.007 ng/ul

RT: 17.381 min Scan# 2447

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:178 Resp: 2206158


Ion Ratio Lower Upper

178 100

179 15.2 12.3 18.5

176 18.6 15.0 22.4

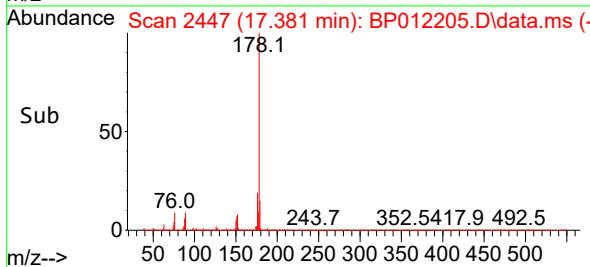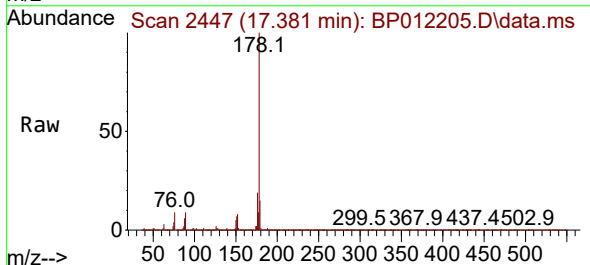



#75

1,2,3,4-Tetrachlorobenzene

Concen: 18.273 ng/uL

RT: 13.281 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:216 Resp: 595152

Ion Ratio Lower Upper

216 100

214 77.4 62.9 94.3

218 49.2 38.6 57.8

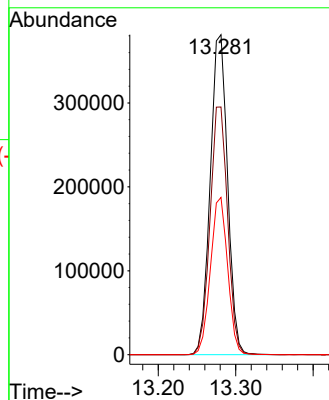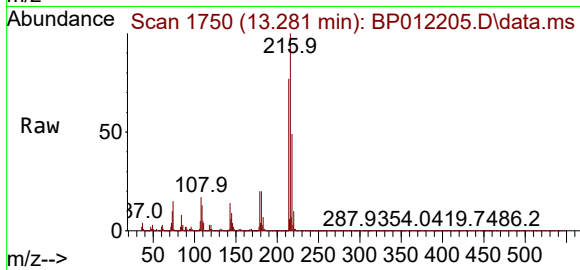

#76

Pentachlorobenzene

Concen: 17.583 ng/uL

RT: 14.804 min Scan# 2009

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:250 Resp: 603209


Ion Ratio Lower Upper

250 100

248 62.4 50.3 75.5

252 64.1 52.0 78.0



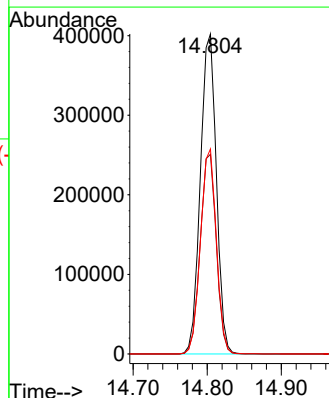
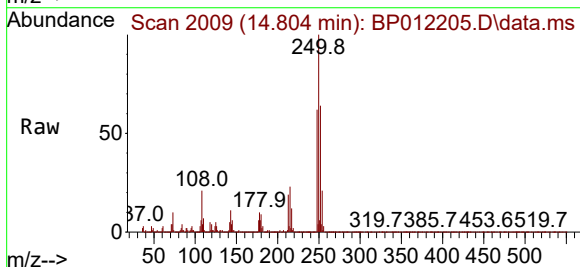




#77
Carbazole
Concen: 19.885 ng/ul
RT: 17.657 min Scan# 2494
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:167 Resp: 2036957
Ion Ratio Lower Upper
167 100
166 21.7 17.3 25.9
139 12.8 10.2 15.4



#78
Di-n-butylphthalate
Concen: 19.754 ng/ul
RT: 18.204 min Scan# 2587
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:149 Resp: 2427472
Ion Ratio Lower Upper
149 100
150 9.2 7.3 10.9
104 4.8 3.8 5.6

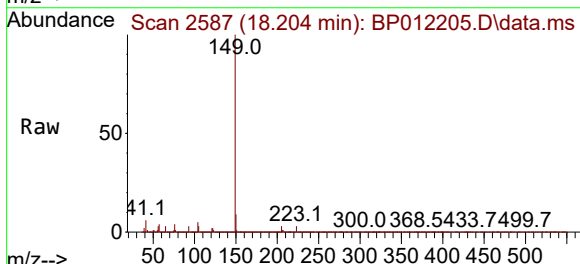



#80

Fluoranthene

Concen: 17.703 ng/ul

RT: 19.257 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:202 Resp: 2527970

Ion Ratio Lower Upper

202 100

101 11.9 10.4 15.6

100 9.2 7.7 11.5



#82

Pyrene

Concen: 17.916 ng/ul

RT: 19.610 min Scan# 2826

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:202 Resp: 2617454


Ion Ratio Lower Upper

202 100

101 14.2 12.3 18.5

100 11.1 10.0 15.0

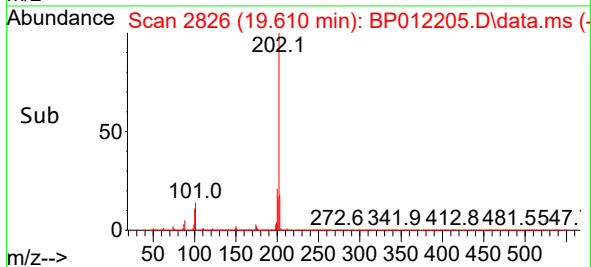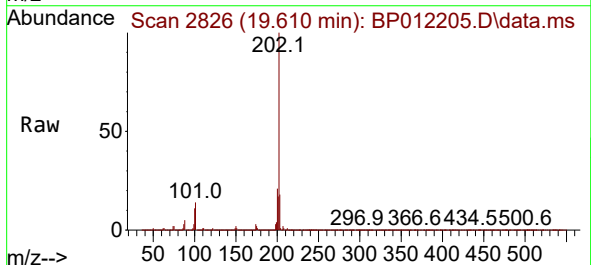



#83

Butylbenzylphthalate

Concen: 18.468 ng/ul

RT: 20.486 min Scan# 2974

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:149 Resp: 1049437

Ion Ratio Lower Upper

149 100

91 68.8 56.1 84.1

206 20.7 16.1 24.1



#84

3,3'-Dichlorobenzidine

Concen: 21.646 ng/ul

RT: 21.257 min Scan# 3106

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:252 Resp: 956912


Ion Ratio Lower Upper

252 100

254 65.1 52.2 78.4

126 11.3 9.8 14.6





#85

Benzo(a)anthracene

Concen: 18.402 ng/ul

RT: 21.322 min Scan# 3117

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:228 Resp: 2434357

Ion Ratio Lower Upper

228 100

229 20.0 16.1 24.1

226 27.2 21.9 32.9

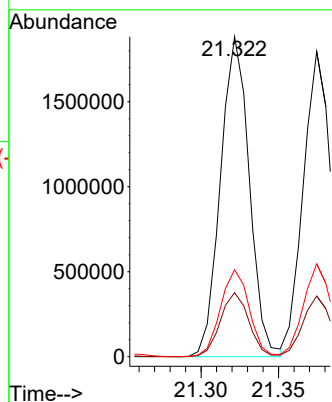

#86

Bis(2-ethylhexyl)phthalate

Concen: 18.885 ng/ul

RT: 21.245 min Scan# 3104

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:149 Resp: 1503463


Ion Ratio Lower Upper

149 100

167 27.6 21.6 32.4

279 4.5 3.4 5.0





#87

Chrysene

Concen: 18.382 ng/ul

RT: 21.375 min Scan# 3125

Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:228 Resp: 2269215

Ion Ratio Lower Upper

228 100

226 30.4 24.2 36.4

229 19.9 15.8 23.8

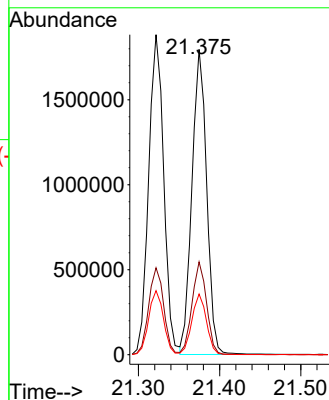

#89

Di-n-octyl phthalate

Concen: 19.514 ng/ul




RT: 22.169 min Scan# 3261


Delta R.T. 0.006 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Tgt Ion:149 Resp: 2373894



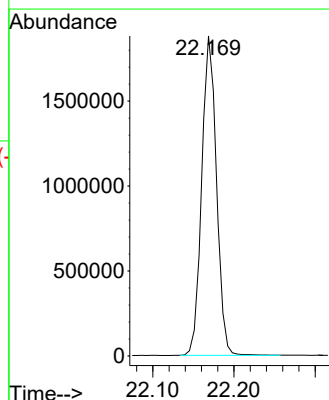





#90
Benzo(b)fluoranthene
Concen: 18.848 ng/ul
RT: 23.010 min Scan# 3404
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:252 Resp: 2209273
Ion Ratio Lower Upper
252 100
253 21.8 17.5 26.3
125 10.3 8.5 12.7



#91
Benzo(k)fluoranthene
Concen: 18.876 ng/ul
RT: 23.057 min Scan# 3412
Delta R.T. 0.006 min
Lab File: BP012205.D
Acq: 19 Oct 2022 15:15

Tgt Ion:252 Resp: 2181014
Ion Ratio Lower Upper
252 100
253 22.0 17.9 26.9
125 10.3 8.6 13.0





#93

Benzo(a)pyrene

Concen: 18.657 ng/ul

RT: 23.645 min Scan# 3

Delta R.T. 0.012 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:252 Resp: 1870121

Ion Ratio Lower Upper

252 100

253 21.6 17.8 26.6

125 11.0 9.7 14.5

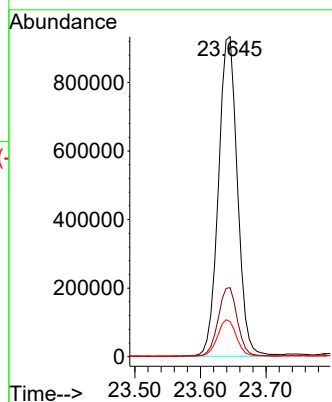

#94

Indeno(1,2,3-cd)pyrene

Concen: 18.485 ng/ul

RT: 26.257 min Scan# 3956

Delta R.T. 0.012 min

Lab File: BP012205.D

Acq: 19 Oct 2022 15:15




Tgt Ion:276 Resp: 2144869


Ion Ratio Lower Upper

276 100

138 23.9 20.3 30.5

277 25.3 20.2 30.4









#95
 Dibenzo(a,h)anthracene
 Concen: 18.183 ng/ul
 RT: 26.268 min Scan# 3957
 Delta R.T. 0.006 min
 Lab File: BP012205.D
 Acq: 19 Oct 2022 15:15

Instrument :
 BNA_P
 ClientSampleId :
 SICV602

Tgt Ion:278 Resp: 1902202
 Ion Ratio Lower Upper
 278 100
 139 15.9 12.9 19.3
 279 22.9 19.0 28.4



#96
 Benzo(g,h,i)perylene
 Concen: 16.827 ng/ul
 RT: 27.027 min Scan# 4087
 Delta R.T. 0.018 min
 Lab File: BP012205.D
 Acq: 19 Oct 2022 15:15

Tgt Ion:276 Resp: 1833272
 Ion Ratio Lower Upper
 276 100
 138 20.6 17.9 26.9
 277 23.6 18.9 28.3

