
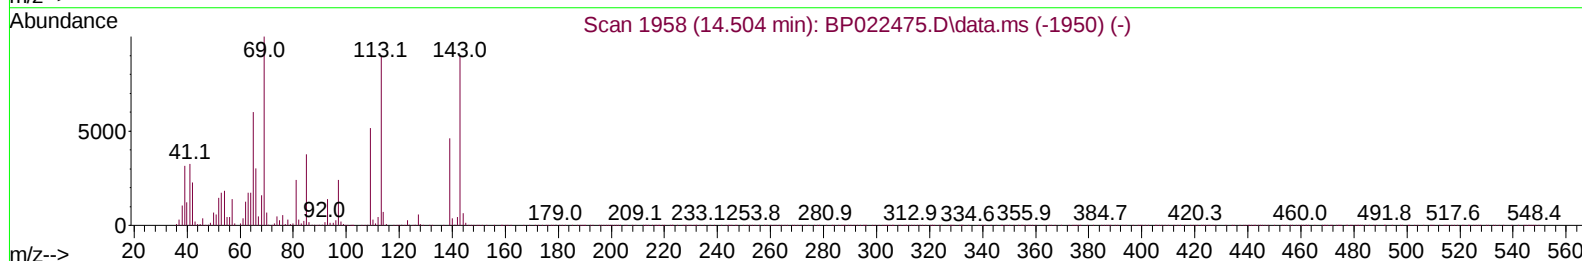
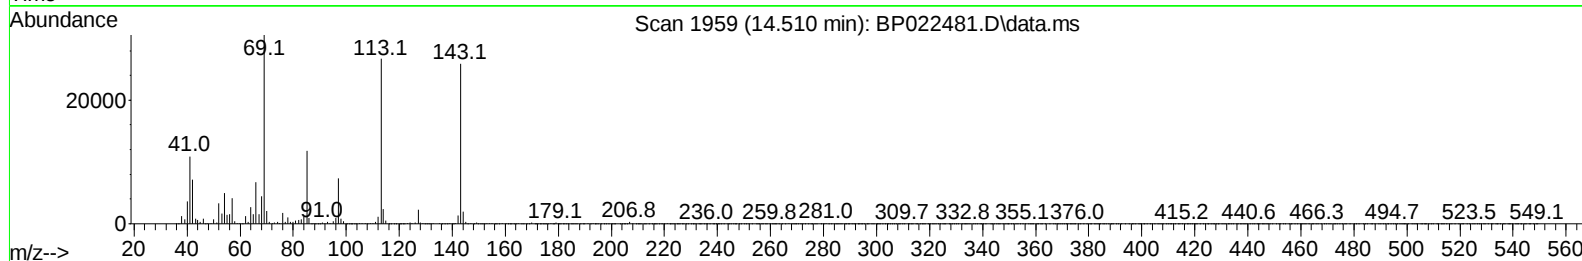


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022481.D
Acq On : 19 Oct 2024 18:19
Operator : RC/JU
Sample : P4361-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Oct 21 02:00:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

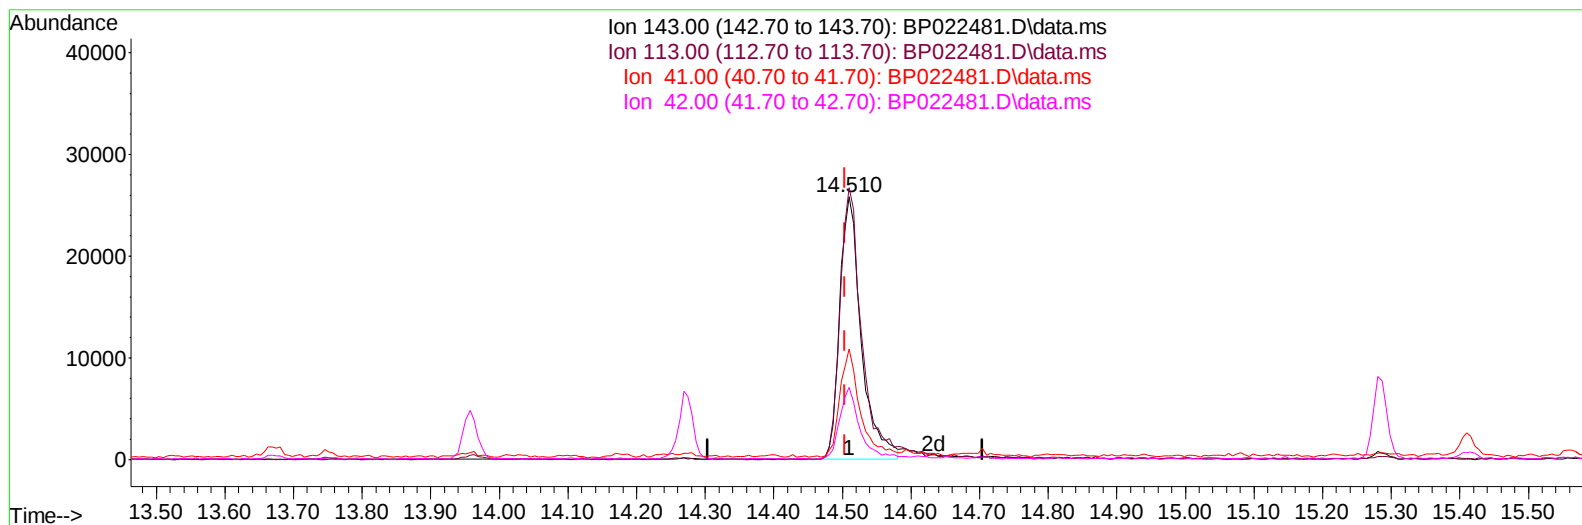




TIC: BP022481.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.510min (+ 0.006) 12.13 ng/u1****response 56529**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	103.37
41.00	35.90	42.16
42.00	23.70	27.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022481.D
Acq On : 19 Oct 2024 18:19
Operator : RC/JU
Sample : P4361-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Oct 21 02:00:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

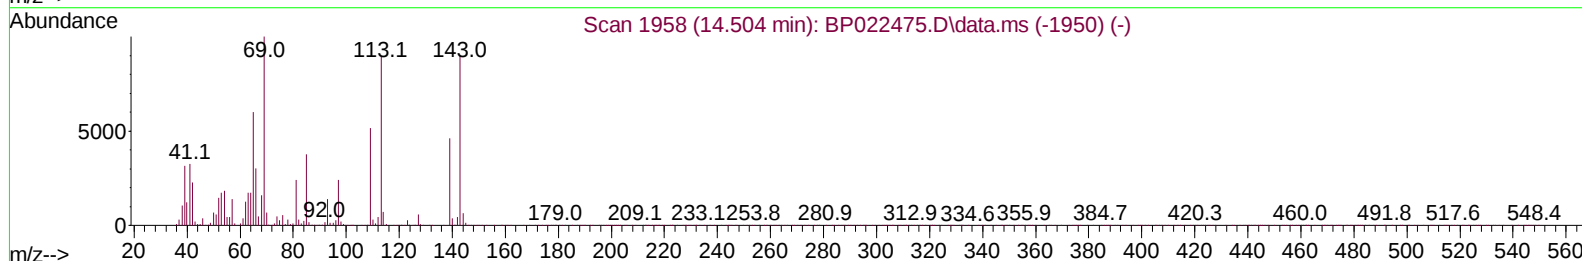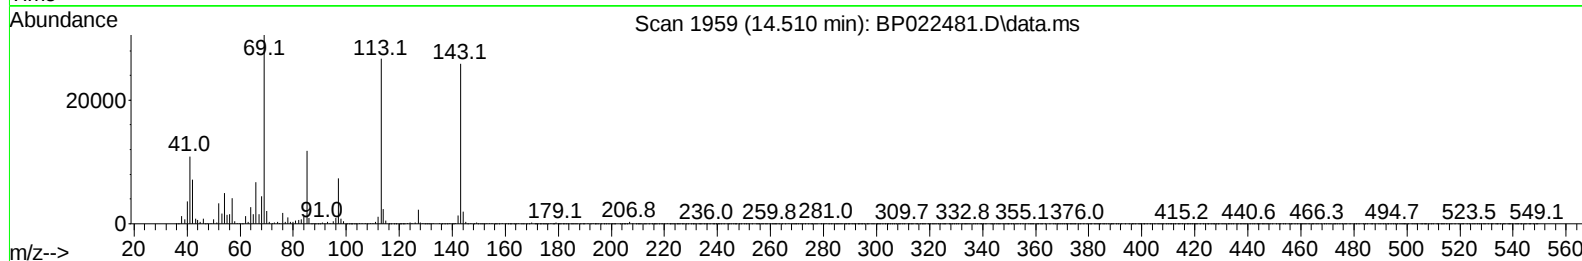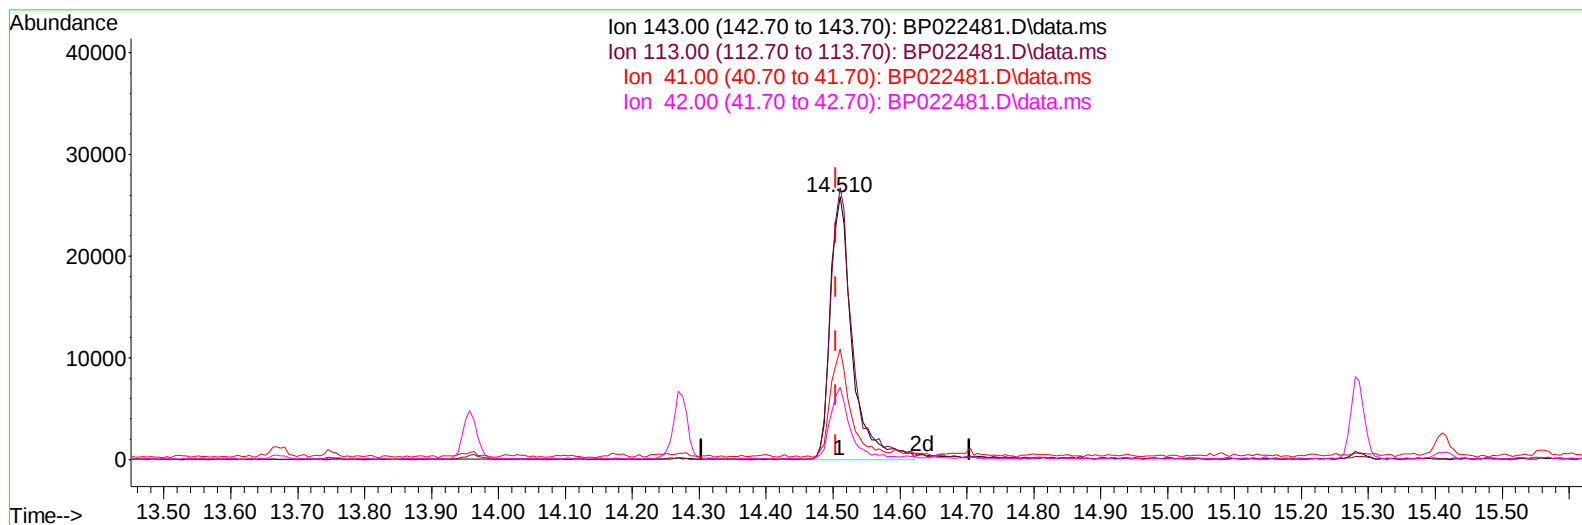

TIC: BP022481.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.510min (+ 0.006) 12.61 ng/ul m

response 58741

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	103.37
41.00	35.90	42.16
42.00	23.70	27.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022481.D
Acq On : 19 Oct 2024 18:19
Operator : RC/JU
Sample : P4361-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Oct 21 02:02:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

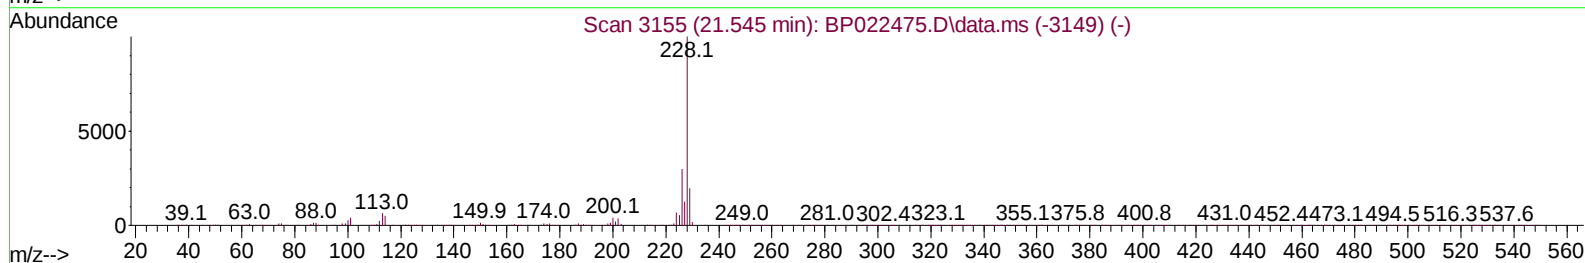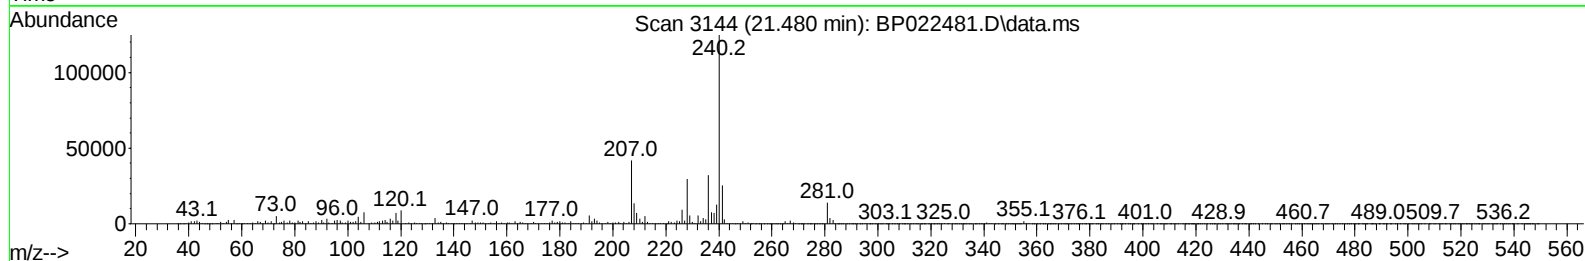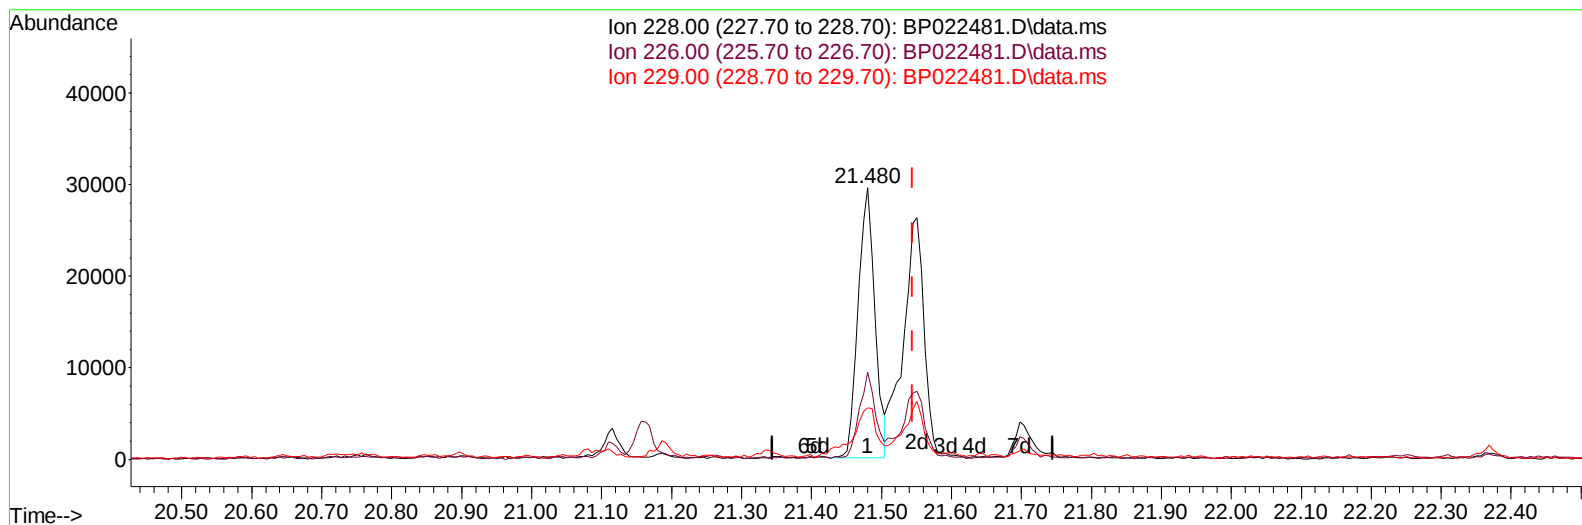




TIC: BP022481.D\data.ms

(87) Chrysene**21.480min (-0.064) 1.02 ng/u1****response 48907**

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.80	32.12
229.00	19.40	18.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022481.D
Acq On : 19 Oct 2024 18:19
Operator : RC/JU
Sample : P4361-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Oct 21 02:02:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

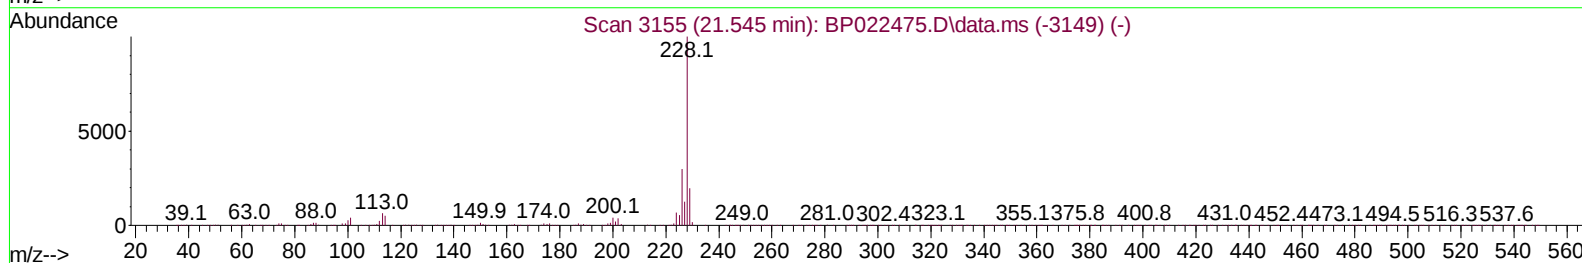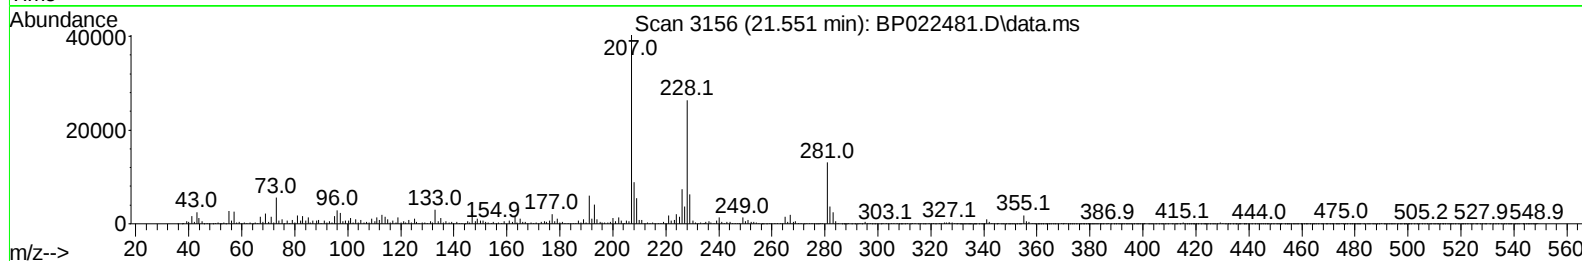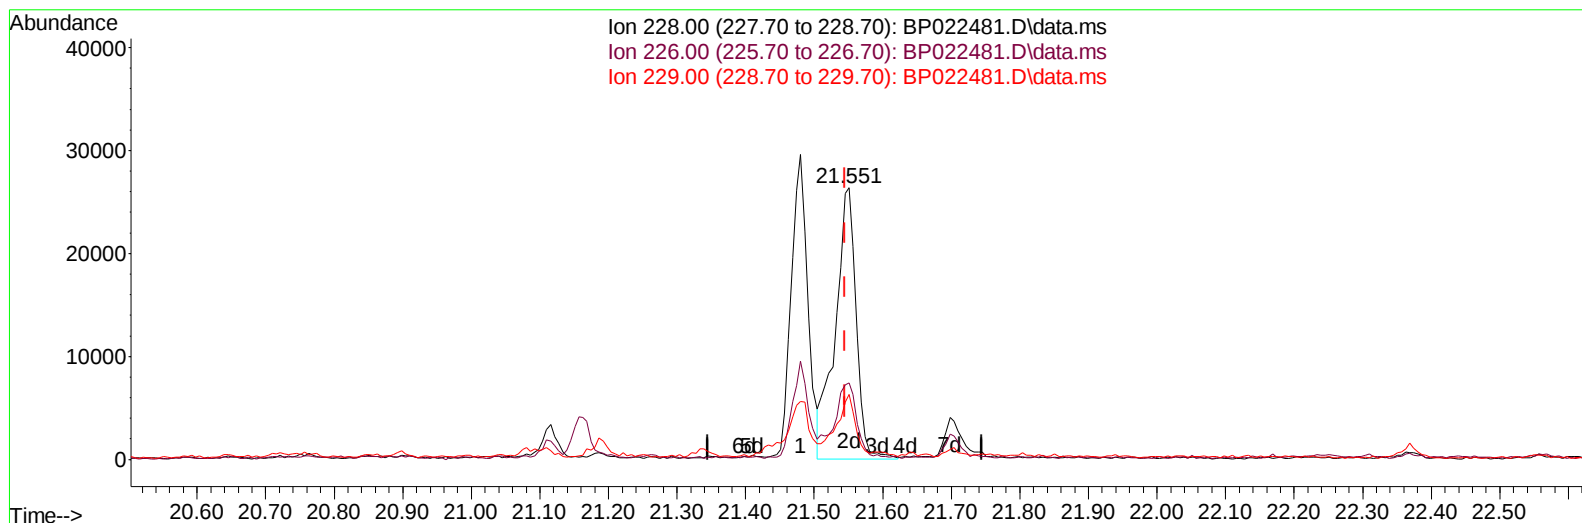

TIC: BP022481.D\data.ms

(87) Chrysene

21.551min (+ 0.006) 1.17 ng/ul m

response 56121

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.80	28.16
229.00	19.40	23.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022481.D
 Acq On : 19 Oct 2024 18:19
 Operator : RC/JU
 Sample : P4361-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Oct 21 02:06:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 18 11:08:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	106293	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	431478	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	349514	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	853768	20.000	ng/ul	-0.01
79) Chrysene-d12	21.498	240	739705	20.000	ng/ul	0.00
88) Perylene-d12	24.751	264	769102	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	6977	2.551	ng/uL	0.00
4) Pyridine-d5	3.611	84	104674	13.940	ng/ul	0.00
7) Phenol-d5	6.852	99	155412	17.369	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	93424	17.765	ng/ul	0.00
11) 2-Chlorophenol-d4	7.205	132	115171	18.140	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	138523	19.400	ng/ul	0.00
21) Nitrobenzene-d5	8.805	128	61392	18.505	ng/ul	0.00
24) 2-Nitrophenol-d4	9.516	143	75291	19.602	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.052	165	159886	19.585	ng/ul	0.00
31) 4-Chloroaniline-d4	10.552	131	182262	18.895	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	584461	21.047	ng/ul	-0.01
49) Acenaphthylene-d8	13.957	160	613508	20.801	ng/ul	0.00
54) 4-Nitrophenol-d4	14.510	143	58741m	12.609	ng/ul	0.00
60) Fluorene-d10	15.287	176	518944	21.545	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	55203	9.831	ng/ul	0.00
73) Anthracene-d10	17.163	188	872838	21.732	ng/ul	0.00
81) Pyrene-d10	19.551	212	1039213	26.567	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.545	264	931503	22.679	ng/ul	0.02
Target Compounds						
					Qvalue	
80) Fluoranthene	19.204	202	98733	2.196	ng/ul	98
82) Pyrene	19.580	202	88955	1.846	ng/ul	99
87) Chrysene	21.551	228	56121m	1.167	ng/ul	
90) Benzo(b)fluoranthene	23.733	252	73559	1.519	ng/ul	94
93) Benzo(a)pyrene	24.598	252	46491	1.043	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022481.D
Acq On : 19 Oct 2024 18:19
Operator : RC/JU
Sample : P4361-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Oct 21 02:06:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

