
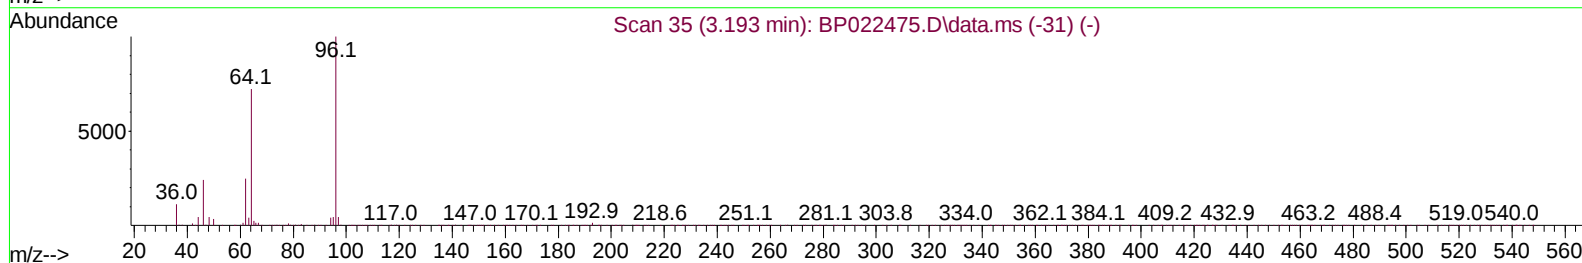
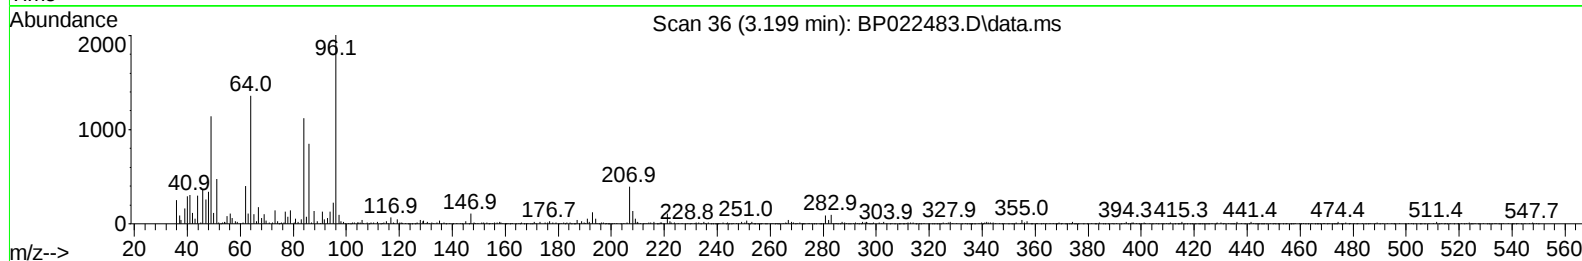


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 20 08:45:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

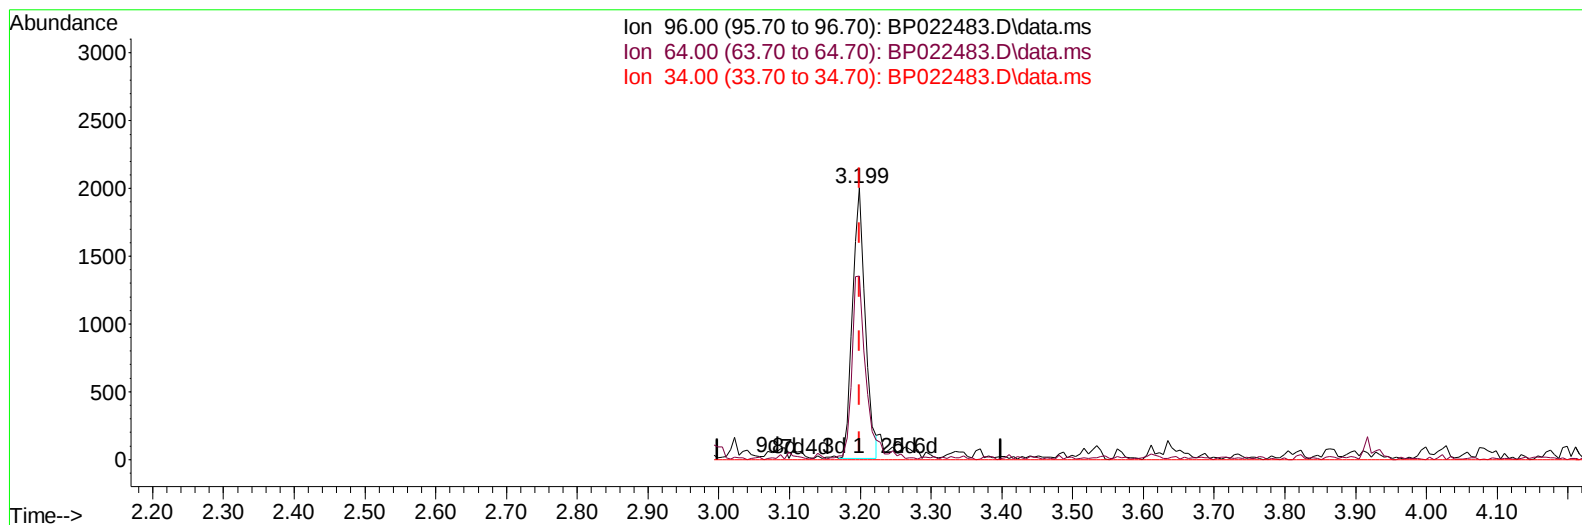




TIC: BP022483.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.199min (+ 0.000) 0.82 ng/uL****response 2497**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	67.66
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 20 08:45:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

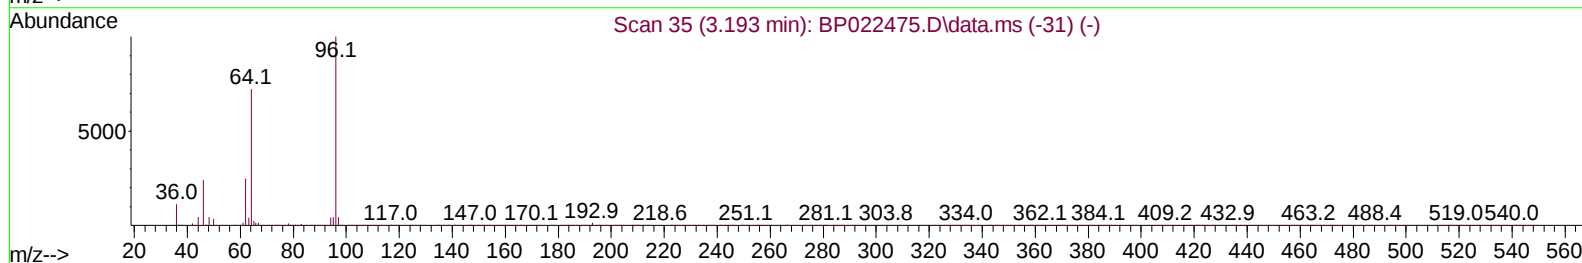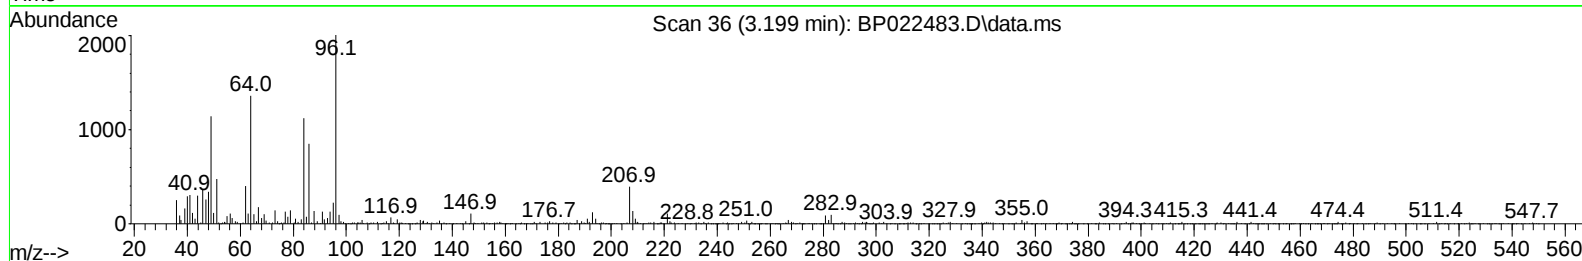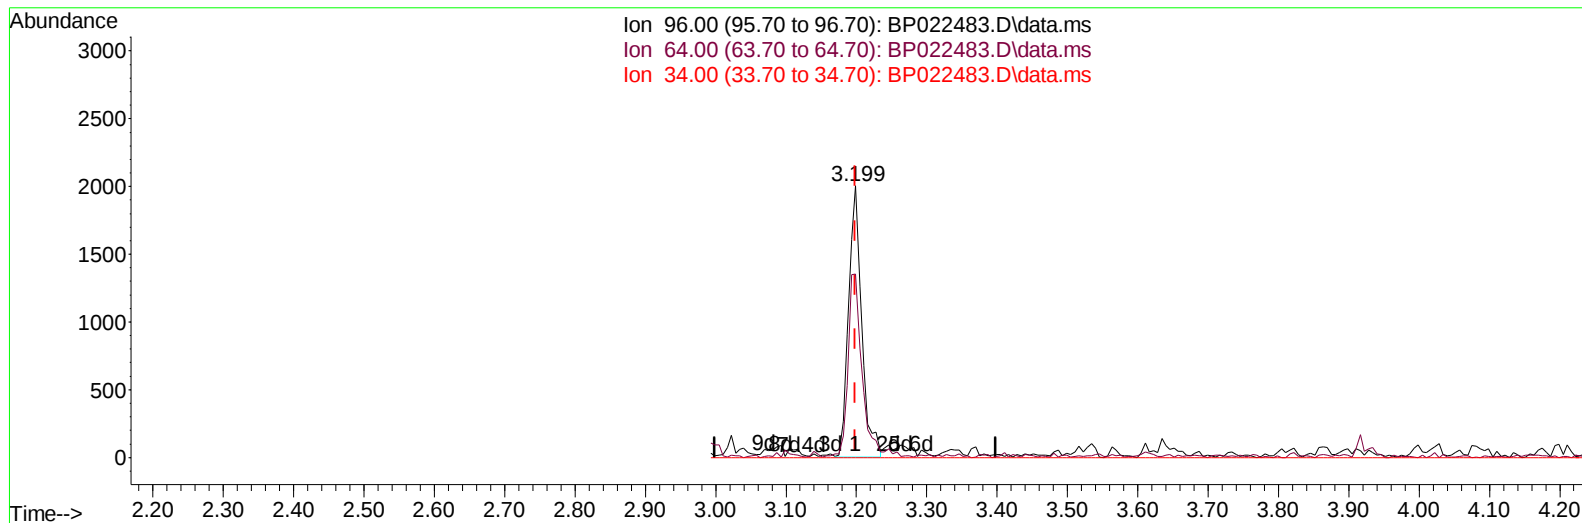

TIC: BP022483.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.199min (+ 0.000) 0.85 ng/uL m

response 2601

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	67.66
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 20 08:45:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

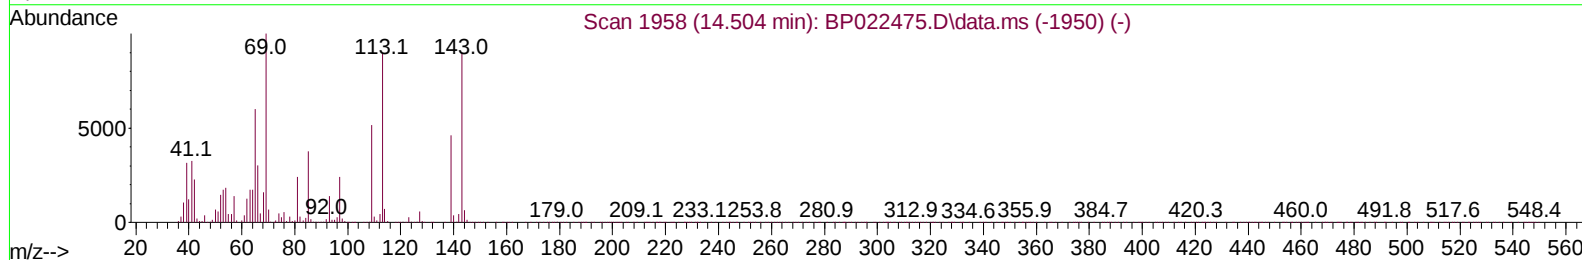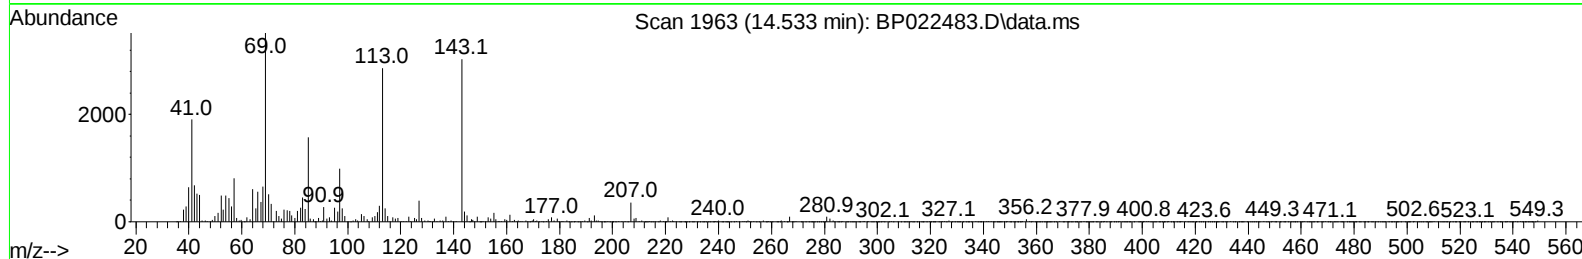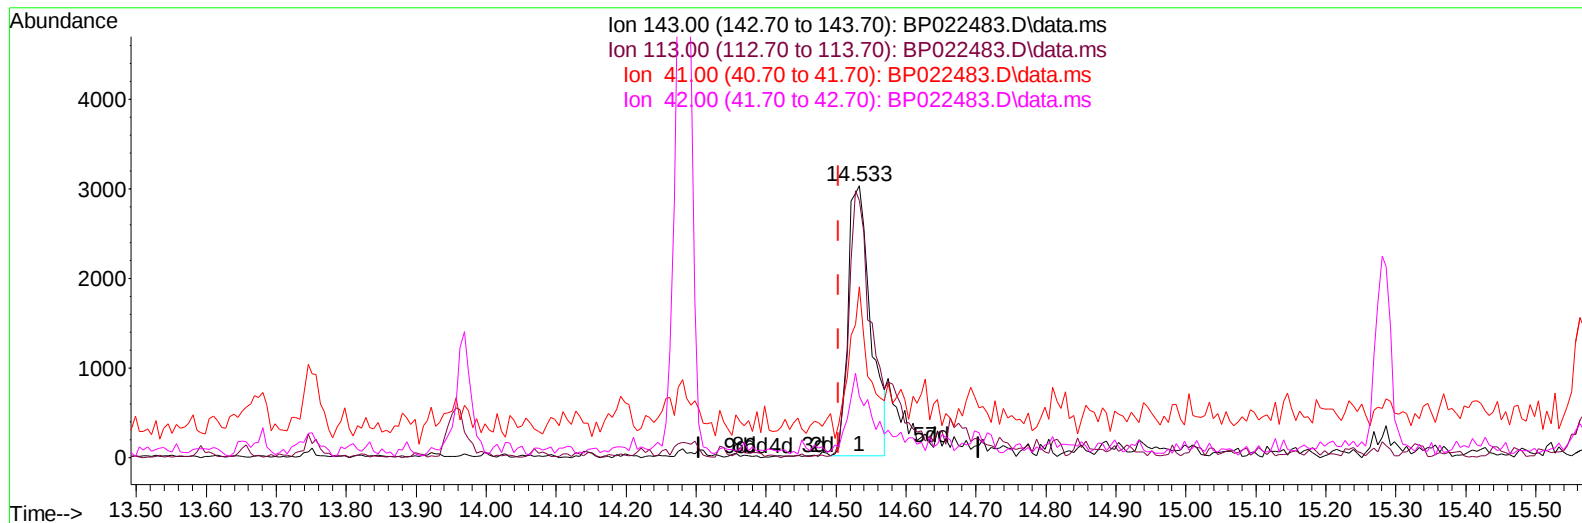

TIC: BP022483.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.533min (+ 0.030) 1.26 ng/ul

response 6691

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	94.62
41.00	35.90	62.90#
42.00	23.70	22.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 20 08:45:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

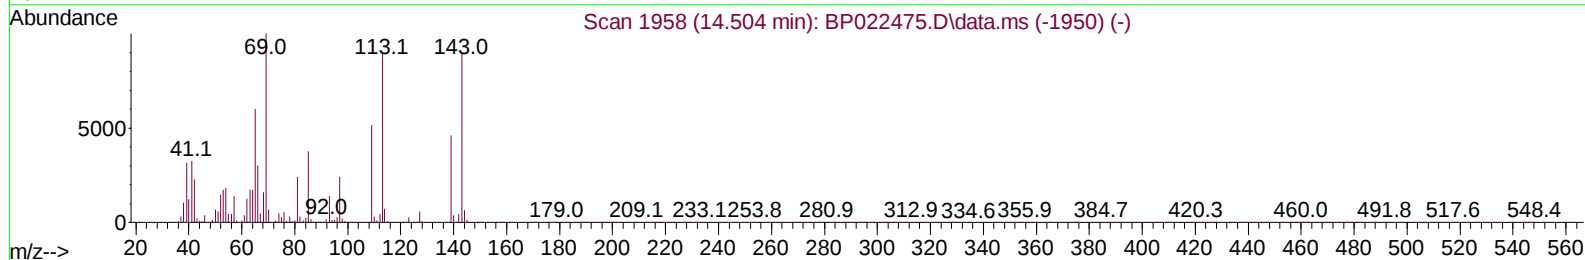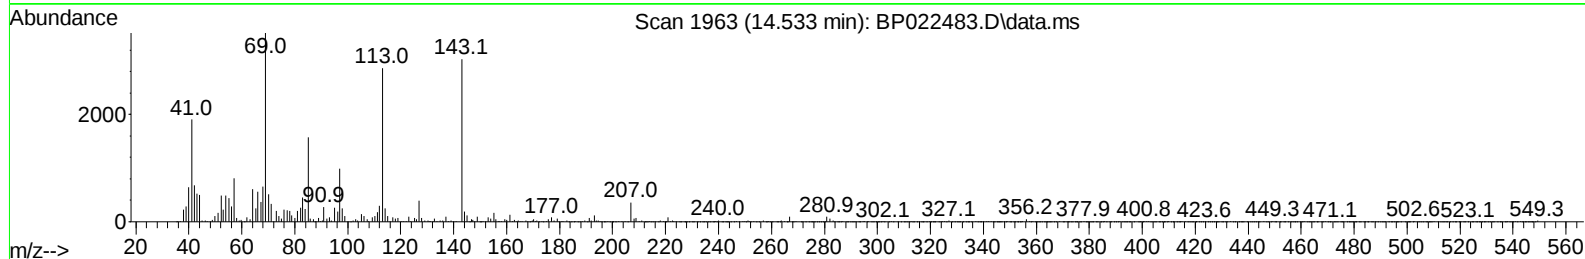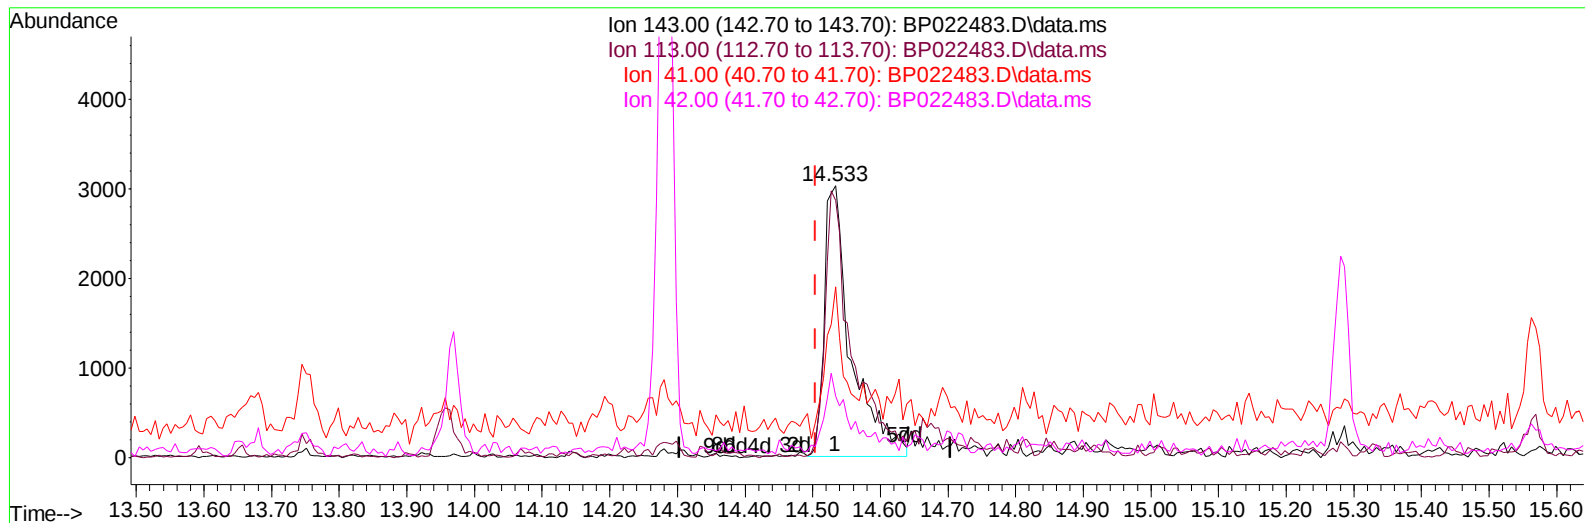

TIC: BP022483.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.533min (+ 0.030) 1.57 ng/ul m

response 8308

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	94.62
41.00	35.90	62.90#
42.00	23.70	22.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 20 08:45:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

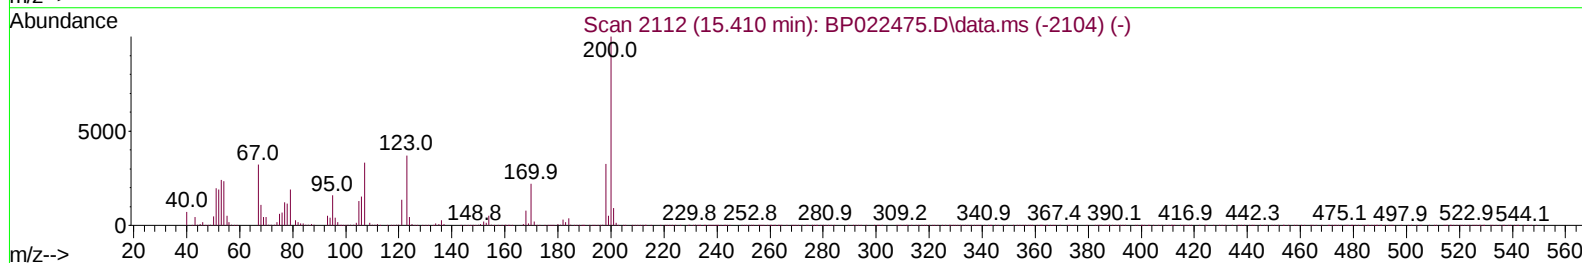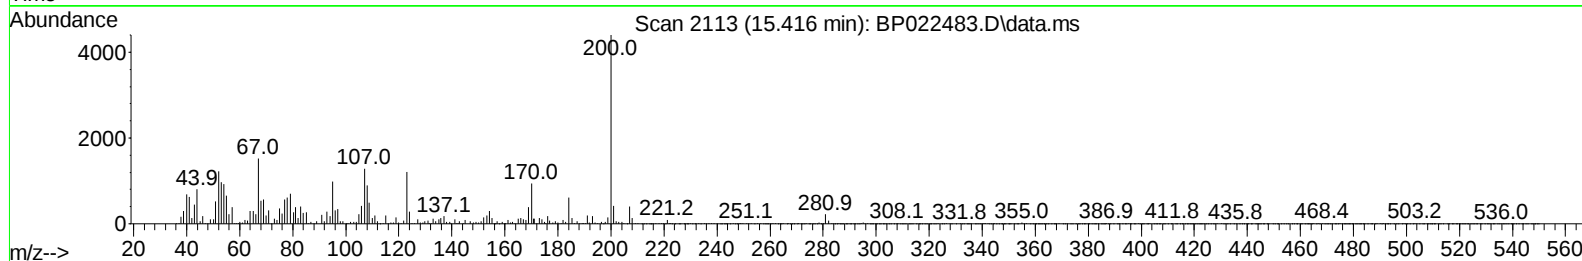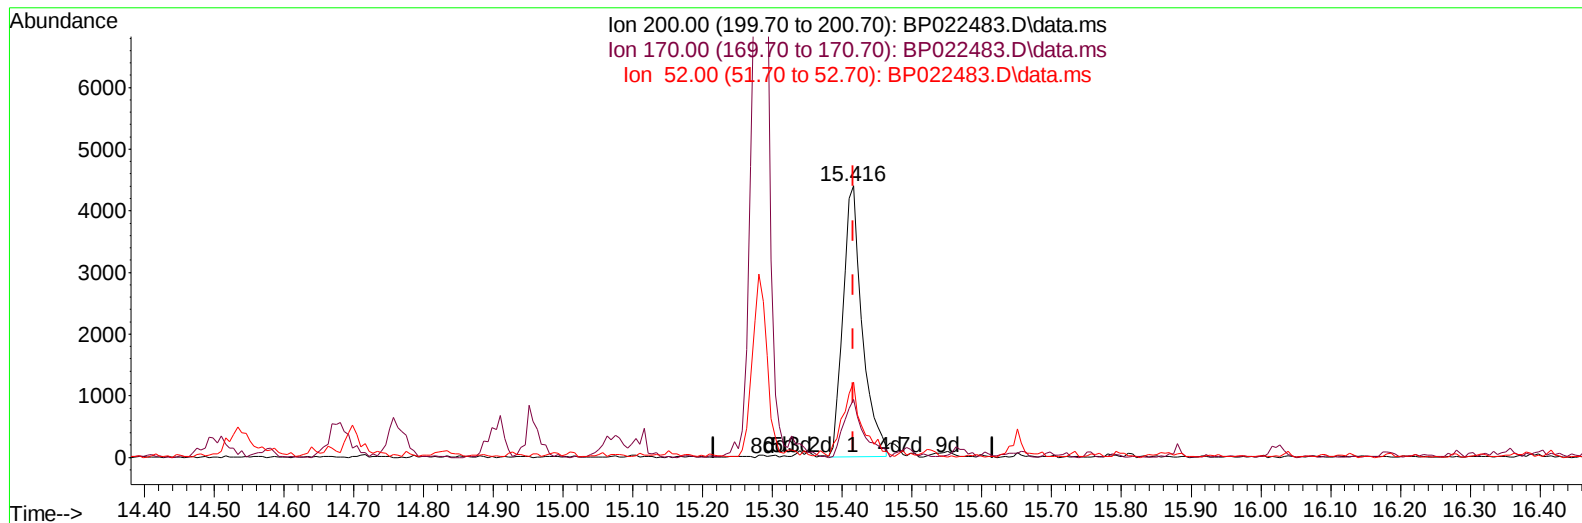




TIC: BP022483.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)**15.416min (+ 0.000) 1.36 ng/ul****response 8440**

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.00	21.34
52.00	36.60	27.70#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 20 08:45:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

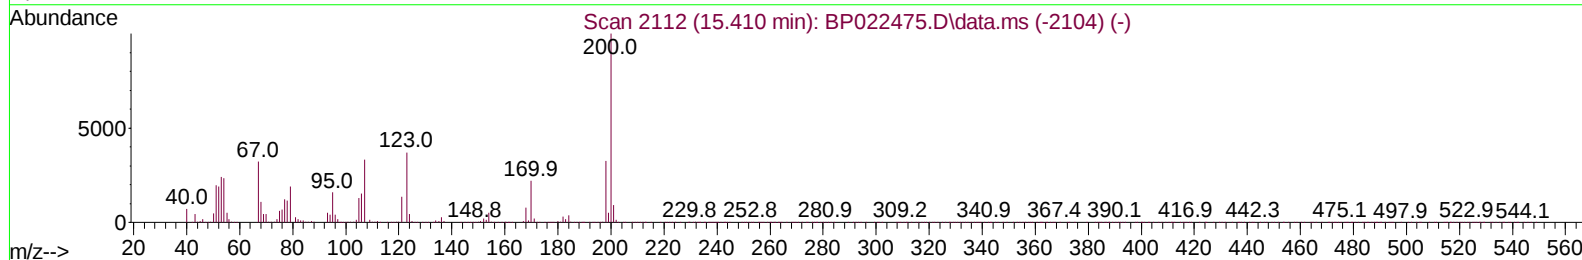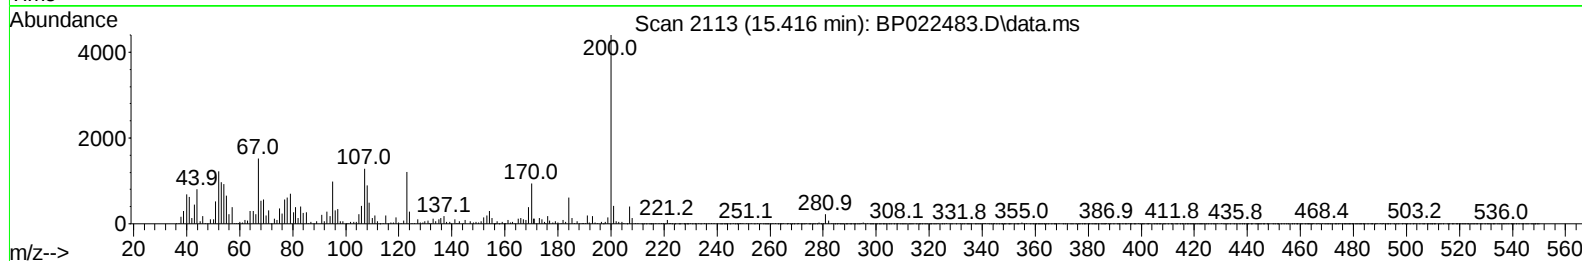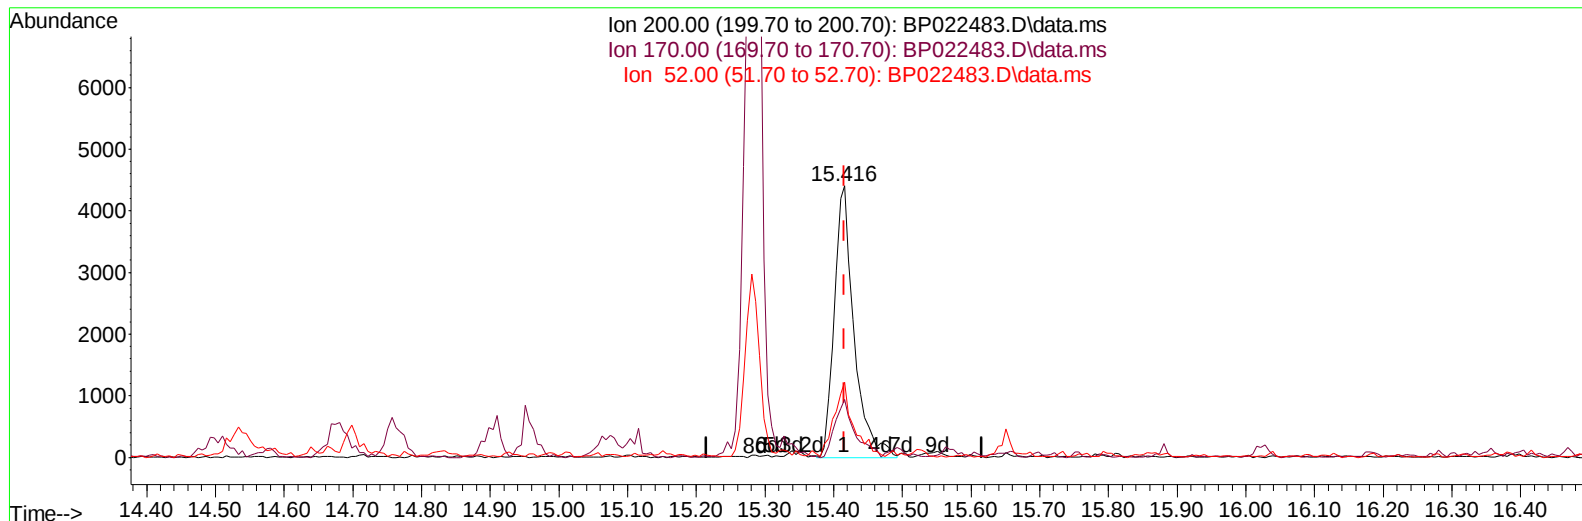

TIC: BP022483.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)




15.416min (+ 0.000) 1.41 ng/ul m

response 8737

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.00	21.34
52.00	36.60	27.70#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 21 02:18:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

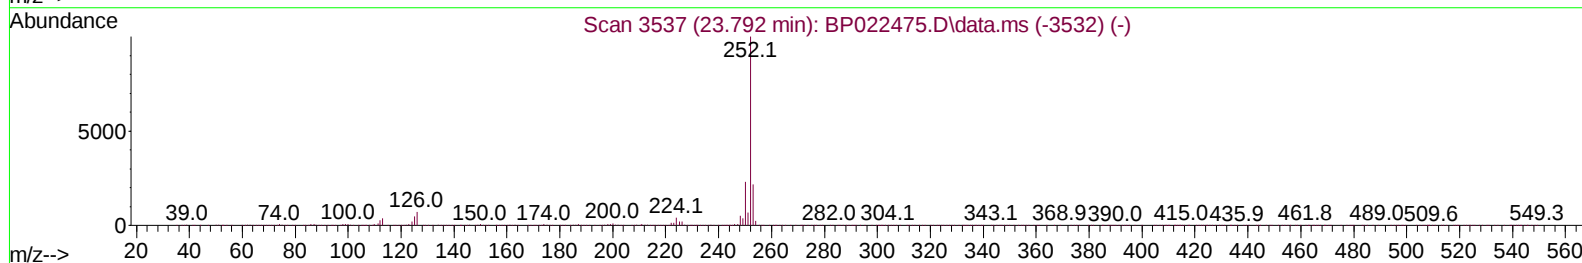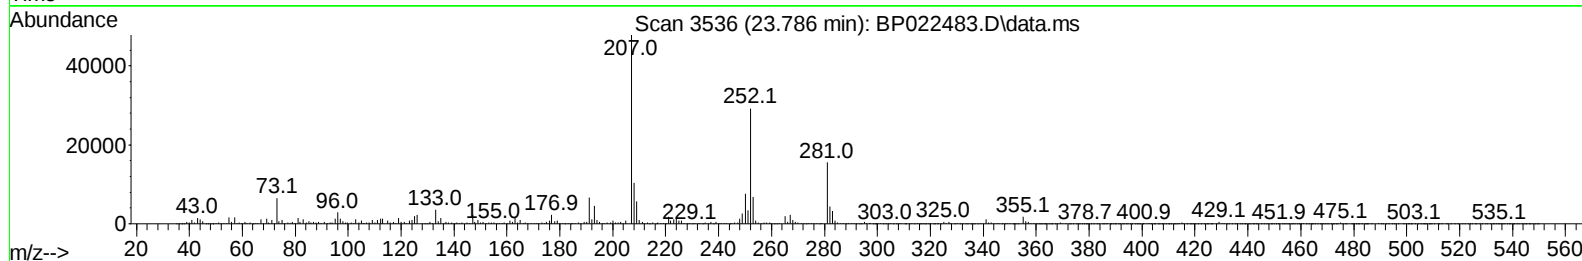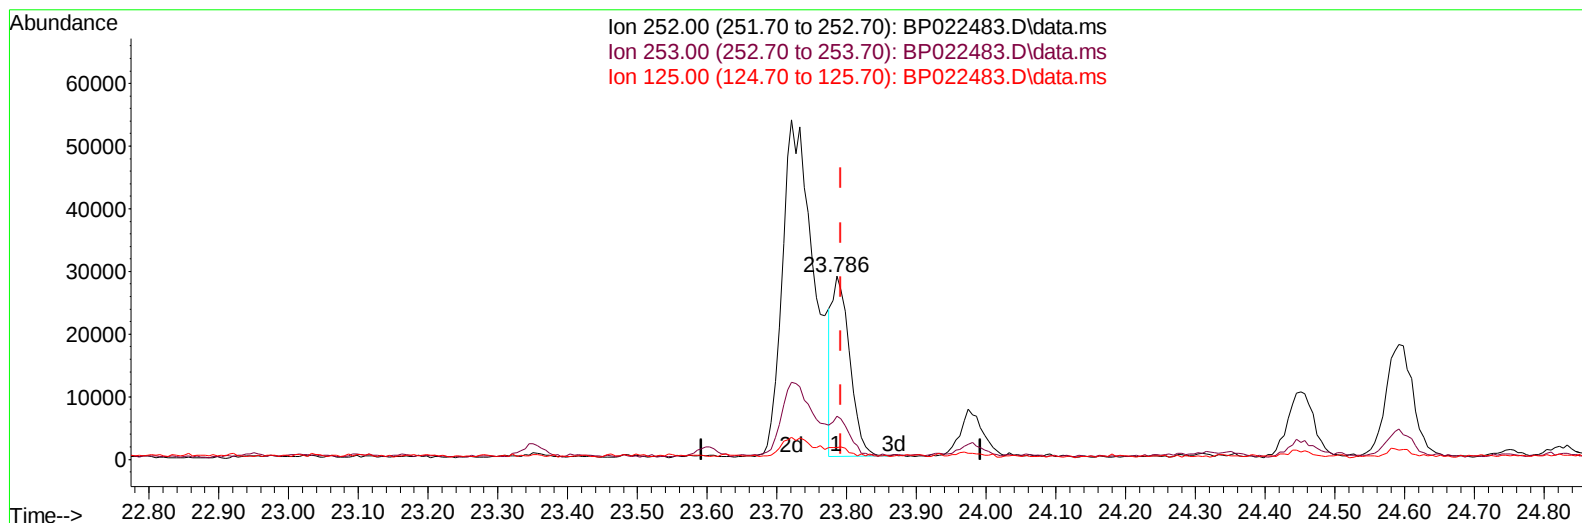

TIC: BP022483.D\data.ms

(91) Benzo(k)fluoranthene




23.786min (-0.006) 0.92 ng/u1

response 50313

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	23.56
125.00	5.70	6.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 21 02:18:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

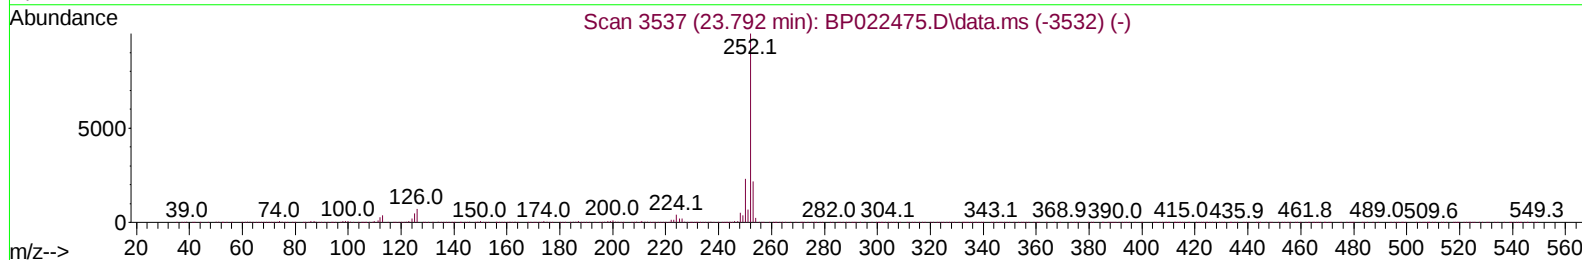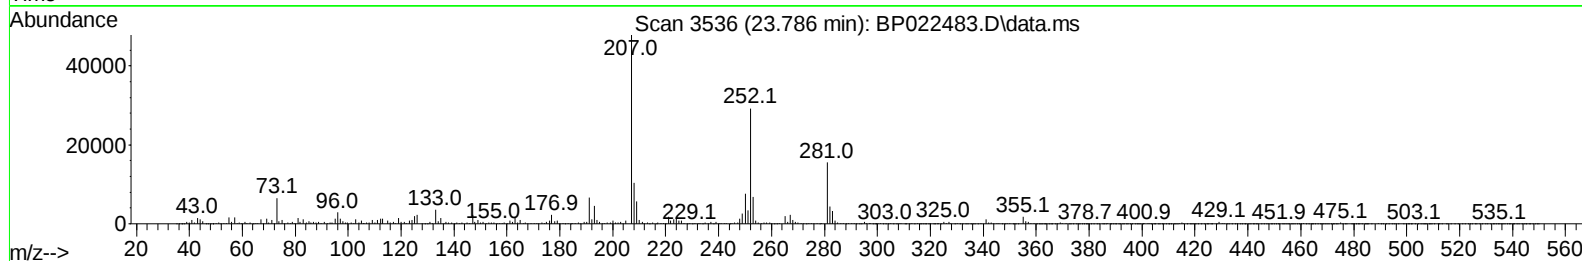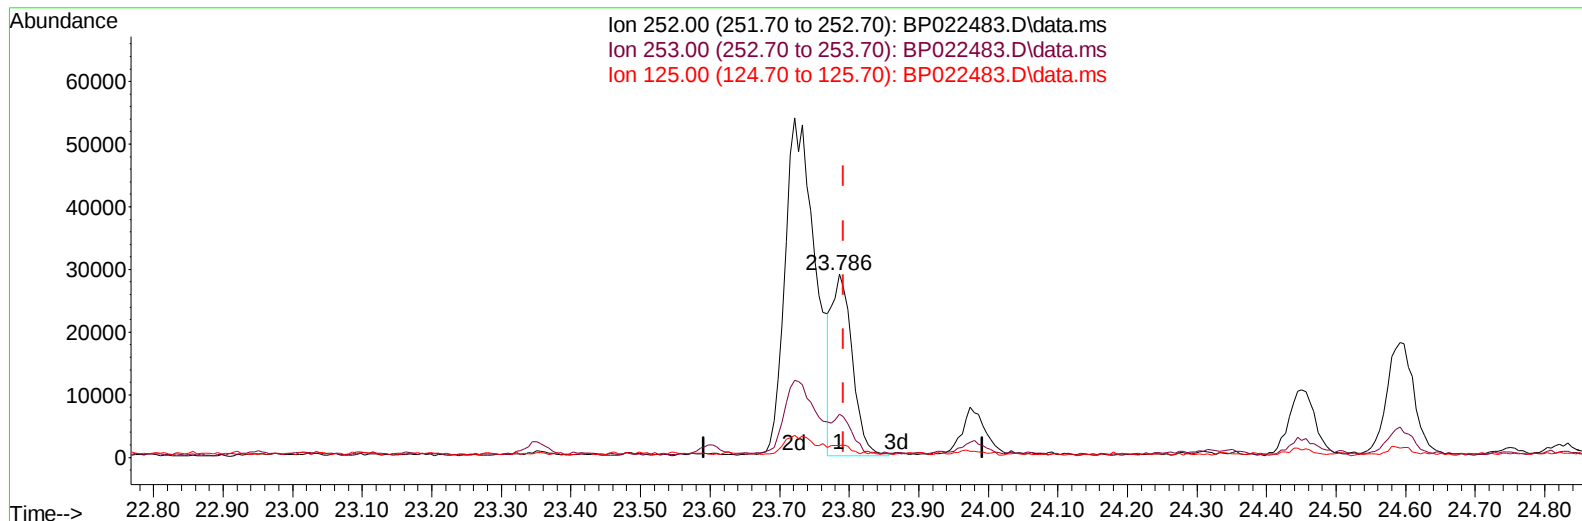

TIC: BP022483.D\data.ms

(91) Benzo(k)fluoranthene

23.786min (-0.006) 1.10 ng/ul m

response 60074

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.70	23.56
125.00	5.70	6.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022483.D
 Acq On : 19 Oct 2024 19:40
 Operator : RC/JU
 Sample : P4361-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 21 02:21:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 18 11:08:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	118988	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136	470929	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	397718	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.063	188	943944	20.000	ng/ul	-0.02
79) Chrysene-d12	21.498	240	866683	20.000	ng/ul	0.00
88) Perylene-d12	24.751	264	888313	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	2601m	0.849	ng/uL	0.00
4) Pyridine-d5	3.622	84	8087	0.962	ng/ul	0.01
7) Phenol-d5	6.857	99	43939	4.387	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.004	67	28877	4.905	ng/ul	0.00
11) 2-Chlorophenol-d4	7.210	132	33690	4.740	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	24457	3.060	ng/ul	0.00
21) Nitrobenzene-d5	8.804	128	18121	5.004	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	21604	5.153	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.057	165	41719	4.682	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	30015	2.851	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	173598	5.494	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	170160	5.070	ng/ul	0.00
54) 4-Nitrophenol-d4	14.533	143	8308m	1.567	ng/ul	0.03
60) Fluorene-d10	15.286	176	153096	5.586	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	8737m	1.407	ng/ul	0.00
73) Anthracene-d10	17.180	188	248835	5.604	ng/ul	0.01
81) Pyrene-d10	19.545	212	248741	5.427	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.521	264	161740	3.409	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.475	105	42966	3.256	ng/ul	95
72) Phenanthrene	17.110	178	100981	2.000	ng/ul	100
80) Fluoranthene	19.198	202	220147	4.178	ng/ul	99
82) Pyrene	19.574	202	137716	2.439	ng/ul	99
85) Benzo(a)anthracene	21.474	228	128244	2.111	ng/ul	97
87) Chrysene	21.545	228	175951	3.123	ng/ul	97
90) Benzo(b)fluoranthene	23.721	252	162683	2.909	ng/ul	99
91) Benzo(k)fluoranthene	23.786	252	60074m	1.097	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 21 02:21:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration

