

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022497.D
 Acq On : 20 Oct 2024 05:50
 Operator : RC/JU
 Sample : P4361-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ0

Quant Time: Oct 21 04:24:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 18 11:08:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	151506	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136	594820	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	436190	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.075	188	866505	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	735356	20.000	ng/ul	0.00
88) Perylene-d12	24.751	264	888402	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	13005	3.336	ng/uL	0.00
4) Pyridine-d5	3.605	84	188043	17.569	ng/ul	0.00
7) Phenol-d5	6.852	99	273691	21.460	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	161210	21.507	ng/ul	0.00
11) 2-Chlorophenol-d4	7.205	132	206874	22.861	ng/ul	0.00
15) 4-Methylphenol-d8	8.363	113	236727	23.259	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	107887	23.589	ng/ul	0.00
24) 2-Nitrophenol-d4	9.516	143	132597	25.042	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.052	165	265290	23.573	ng/ul	0.00
31) 4-Chloroaniline-d4	10.552	131	298956	22.481	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	924937	26.689	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	947933	25.753	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	59708	10.270	ng/ul	0.00
60) Fluorene-d10	15.275	176	764020	25.417	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.422	200	60789	10.667	ng/ul	0.00
73) Anthracene-d10	17.175	188	1116059	27.380	ng/ul	0.00
81) Pyrene-d10	19.545	212	1140566	29.330	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.527	264	1362206	28.711	ng/ul	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.198	202	58372	1.306	ng/ul	98
82) Pyrene	19.575	202	52009	1.085	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022497.D
Acq On : 20 Oct 2024 05:50
Operator : RC/JU
Sample : P4361-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ0

Quant Time: Oct 21 04:24:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 18 11:08:24 2024
Response via : Initial Calibration




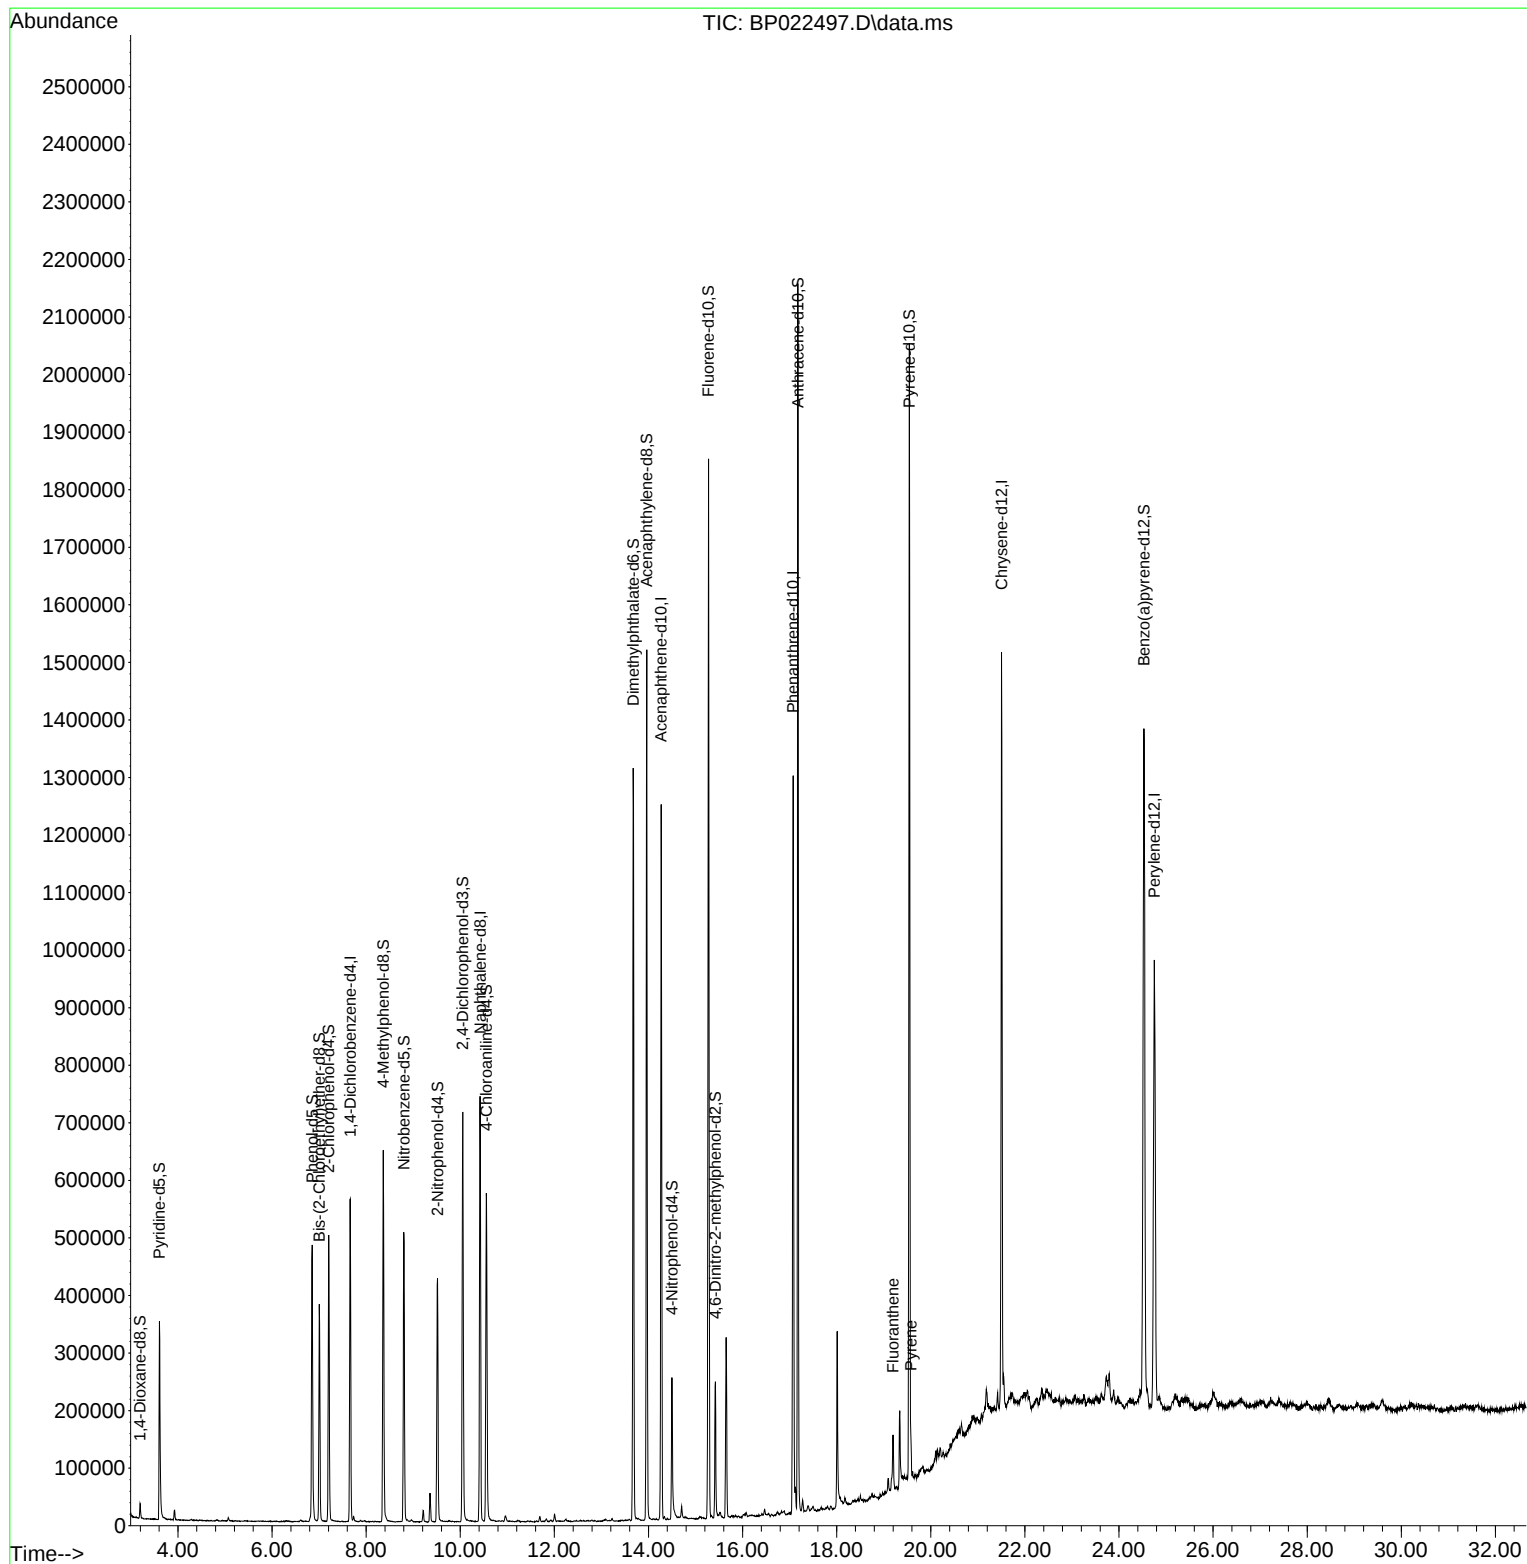


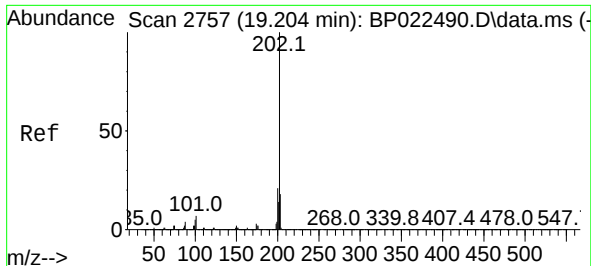

#80
Fluoranthene
Concen: 1.306 ng/ul
RT: 19.198 min Scan# 21
Delta R.T. -0.011 min
Lab File: BP022497.D
Acq: 20 Oct 2024 05:50

Instrument :
BNA_P
ClientSampleId :
EOAZ0

Tgt Ion:202 Resp: 58372
Ion Ratio Lower Upper
202 100
101 6.6 5.8 8.8
100 6.1 4.5 6.7

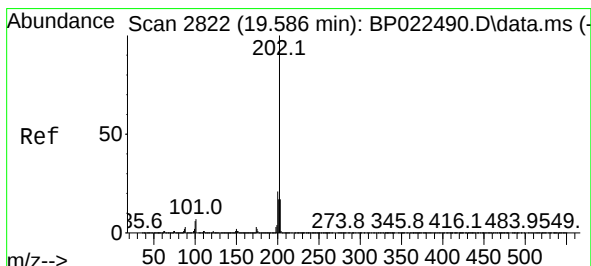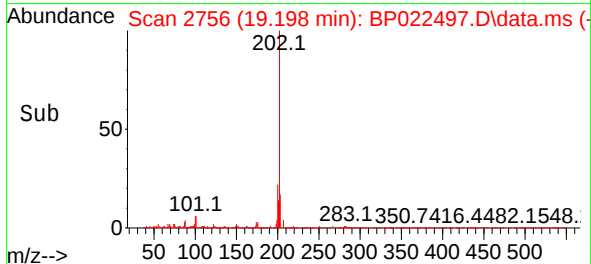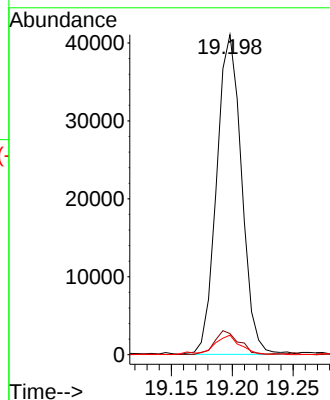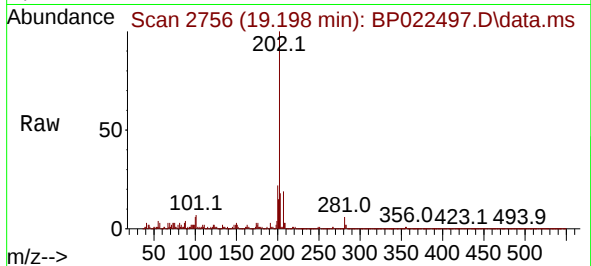

#82
Pyrene
Concen: 1.085 ng/ul
RT: 19.575 min Scan# 2820
Delta R.T. -0.011 min
Lab File: BP022497.D
Acq: 20 Oct 2024 05:50

Tgt Ion:202 Resp: 52009
Ion Ratio Lower Upper
202 100
101 8.9 6.7 10.1
100 6.0 5.8 8.6

