

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022476.D
 Acq On : 19 Oct 2024 14:57
 Operator : RC/JU
 Sample : PB164170BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	31	36	43	rVB	28354	39834	1.47%	0.126%
2	3.605	101	105	129	rBV	372172	580968	21.50%	1.838%
3	3.928	156	160	164	rVB	5782	8168	0.30%	0.026%
4	6.852	644	657	669	rBV	476081	790001	29.24%	2.499%
5	7.005	676	683	694	rVB	365885	578204	21.40%	1.829%
6	7.205	708	717	729	rBV	466512	785881	29.08%	2.486%
7	7.664	787	795	804	rBV	433537	712489	26.37%	2.254%
8	8.363	906	914	929	rBV2	600567	1015180	37.57%	3.211%
9	8.805	980	989	1001	rBV	503131	822576	30.44%	2.602%
10	9.210	1051	1058	1064	rVV2	7162	12136	0.45%	0.038%
11	9.516	1102	1110	1124	rBV	447172	736261	27.25%	2.329%
12	10.052	1193	1201	1224	rBV	616998	1130083	41.82%	3.574%
13	10.416	1255	1263	1273	rBV	602540	998332	36.94%	3.158%
14	10.557	1278	1287	1300	rBV	644225	1042183	38.57%	3.296%
15	11.693	1475	1480	1484	rVB3	6171	9546	0.35%	0.030%
16	12.004	1528	1533	1541	rBV3	9079	19453	0.72%	0.062%
17	13.063	1704	1713	1716	rBV9	1493	2799	0.10%	0.009%
18	13.234	1739	1742	1747	rBV7	1972	2830	0.10%	0.009%
19	13.681	1810	1818	1832	rBV	1153177	1782306	65.96%	5.637%
20	13.793	1832	1837	1843	rVB8	2488	6238	0.23%	0.020%
21	13.963	1856	1866	1879	rBV	1234197	1965067	72.72%	6.215%
22	14.269	1911	1918	1927	rBV	1025267	1495476	55.34%	4.730%
23	14.498	1951	1957	1971	rBV	395909	675806	25.01%	2.138%
24	15.275	2082	2089	2103	rBV	1681203	2508284	92.82%	7.934%
25	15.416	2106	2113	2128	rVV	392714	666474	24.66%	2.108%
26	15.528	2128	2132	2138	rVB4	9446	16500	0.61%	0.052%
27	15.928	2196	2200	2203	rVB5	2144	3048	0.11%	0.010%
28	15.998	2207	2212	2215	rBV5	2549	4428	0.16%	0.014%
29	16.334	2265	2269	2275	rBV8	2330	4255	0.16%	0.013%
30	16.398	2275	2280	2285	rVV2	4043	5591	0.21%	0.018%
31	16.457	2285	2290	2295	rVV6	3866	5731	0.21%	0.018%
32	16.557	2303	2307	2310	rVB5	2558	3609	0.13%	0.011%
33	16.739	2334	2338	2343	rVB7	2524	4812	0.18%	0.015%
34	16.857	2355	2358	2364	rBV3	2839	4262	0.16%	0.013%
35	17.063	2386	2393	2405	rBV	1086130	1801337	66.66%	5.698%
36	17.175	2405	2412	2423	rBV	1792317	2649193	98.04%	8.379%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022476.D
Acq On : 19 Oct 2024 14:57
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	17.545	2471	2475	2476	rBV4	2795	3447	0.13%	0.011%
38	18.004	2550	2553	2558	rVB7	3845	6122	0.23%	0.019%
39	19.098	2734	2739	2746	rBV2	21454	33794	1.25%	0.107%
40	19.175	2748	2752	2759	rVV2	19505	29958	1.11%	0.095%
41	19.557	2810	2817	2824	rBV	1857029	2702240	100.00%	8.547%
42	21.504	3142	3148	3155	rVB	962829	1588195	58.77%	5.023%
43	24.545	3656	3665	3680	rVB	1055587	2662353	98.52%	8.421%
44	24.763	3694	3702	3715	rVB	671144	1700341	62.92%	5.378%


Sum of corrected areas: 31615791

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022476.D
Acq On : 19 Oct 2024 14:57
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

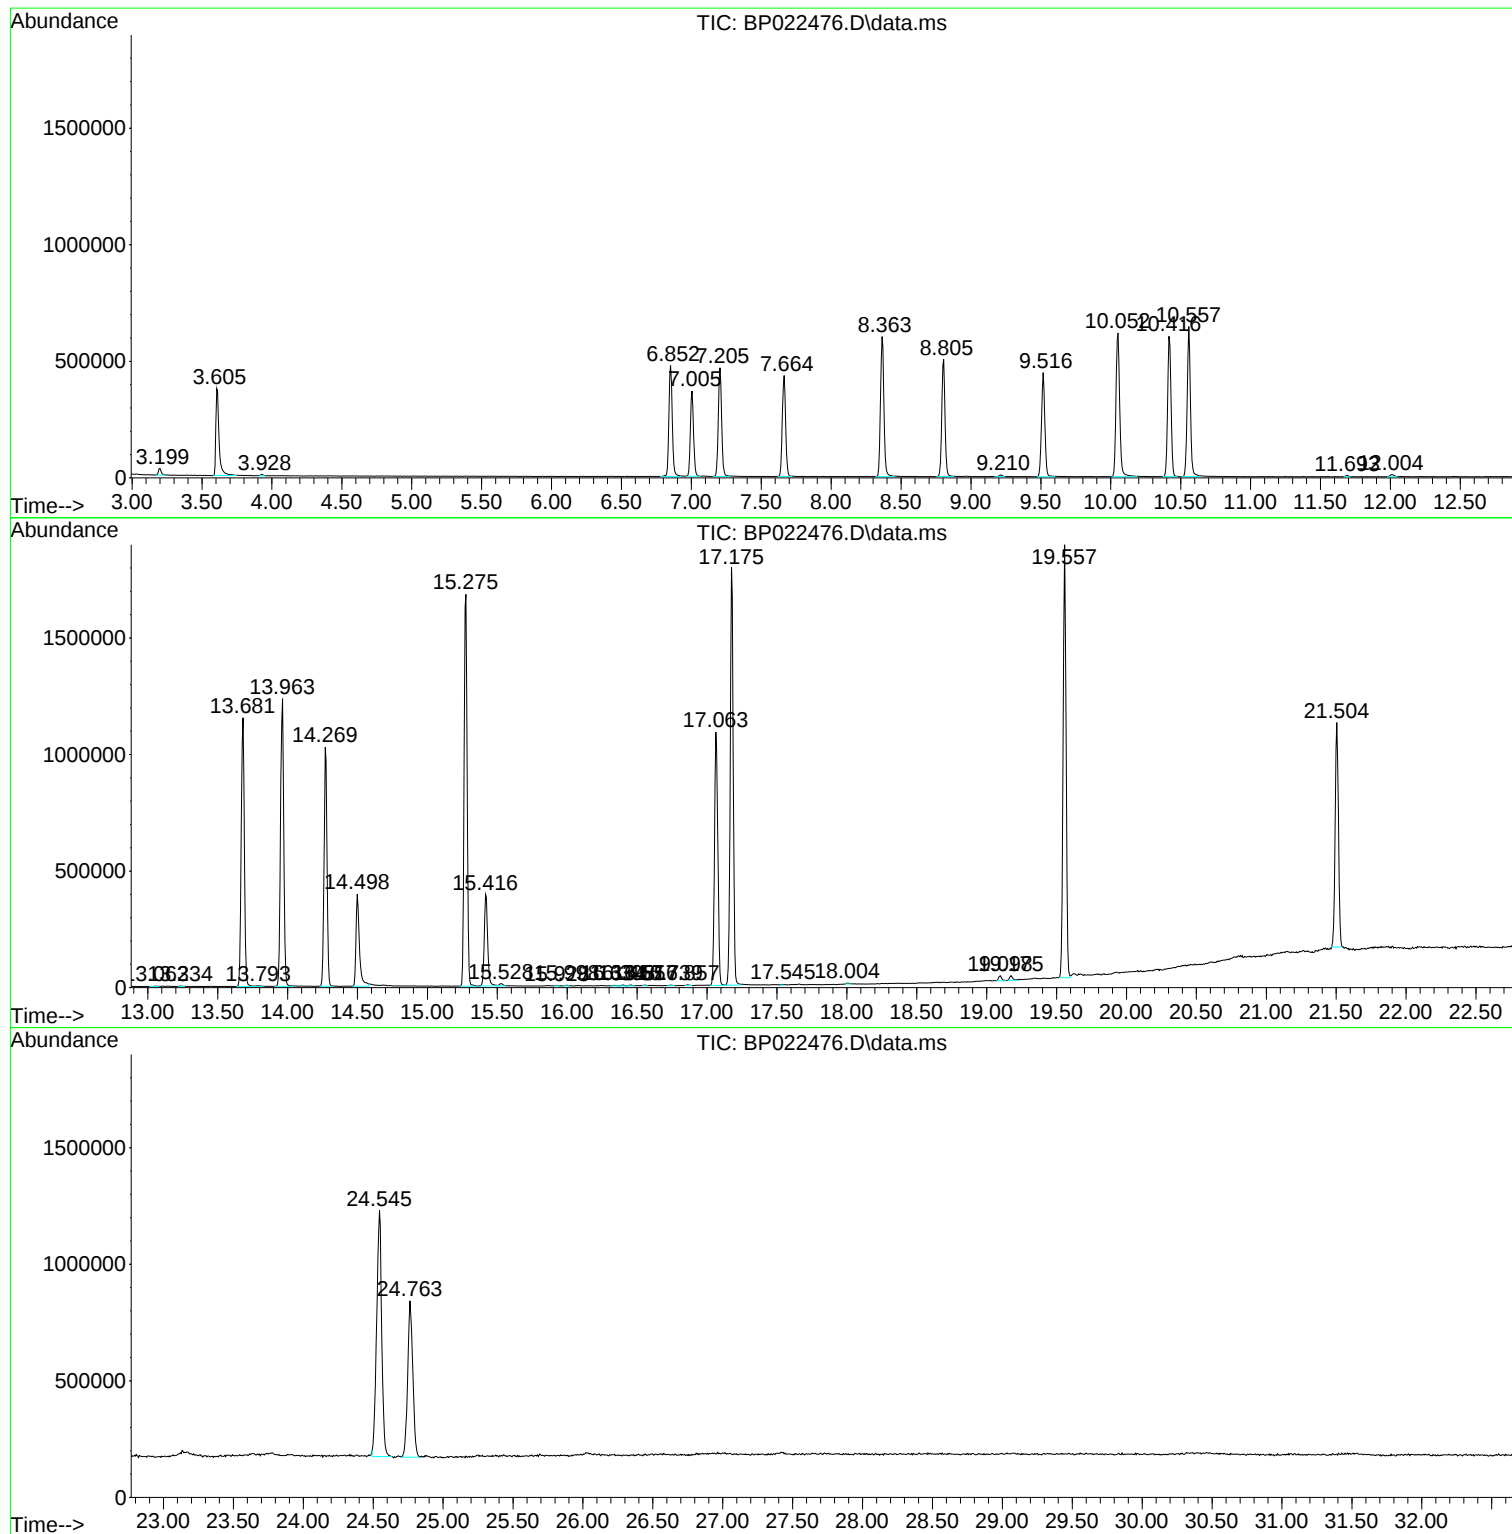

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022476.D
Acq On : 19 Oct 2024 14:57
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022476.D
Acq On : 19 Oct 2024 14:57
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------