

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022483.D
 Acq On : 19 Oct 2024 19:40
 Operator : RC/JU
 Sample : P4361-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	42	rVB	4893	6938	0.27%	0.040%
2	3.622	104	108	118	rBV2	14152	26758	1.04%	0.153%
3	3.710	119	123	130	rVB	18013	24198	0.94%	0.138%
4	3.928	156	160	164	rVB	10738	15562	0.60%	0.089%
5	4.293	217	222	227	rVB8	3993	6855	0.27%	0.039%
6	4.446	241	248	249	rBV6	2741	4068	0.16%	0.023%
7	4.475	251	253	258	rVB5	4704	5938	0.23%	0.034%
8	4.522	258	261	265	rBV6	1889	2961	0.11%	0.017%
9	4.710	289	293	297	rBV7	3032	4443	0.17%	0.025%
10	4.822	306	312	318	rBV	7463	14083	0.54%	0.080%
11	5.699	456	461	465	rBV6	2779	4298	0.17%	0.025%
12	6.057	515	522	523	rBV7	1569	3113	0.12%	0.018%
13	6.081	523	526	531	rVB7	2297	3489	0.13%	0.020%
14	6.334	561	569	574	rBV5	2749	6079	0.24%	0.035%
15	6.546	600	605	610	rBV8	1373	2793	0.11%	0.016%
16	6.816	645	651	653	rBV2	11385	19244	0.74%	0.110%
17	6.857	653	658	672	rVB	75264	149301	5.78%	0.853%
18	7.004	678	683	692	rVV	67078	105992	4.10%	0.606%
19	7.210	709	718	726	rBV	77627	135043	5.22%	0.772%
20	7.287	728	731	744	rVB	3024	6243	0.24%	0.036%
21	7.487	761	765	770	rBV4	2423	3771	0.15%	0.022%
22	7.663	787	795	805	rBV	433841	723939	28.01%	4.137%
23	8.193	882	885	889	rVB6	2013	3345	0.13%	0.019%
24	8.369	908	915	925	rBV	61068	111897	4.33%	0.640%
25	8.475	927	933	944	rVB	81486	132485	5.13%	0.757%
26	8.610	951	956	962	rBV8	2235	5302	0.21%	0.030%
27	8.804	983	989	1000	rBV	82982	147567	5.71%	0.843%
28	9.216	1052	1059	1063	rBV	19763	32639	1.26%	0.187%
29	9.363	1079	1084	1094	rVV4	6204	12205	0.47%	0.070%
30	9.510	1103	1109	1117	rBV	70470	123876	4.79%	0.708%
31	9.710	1131	1143	1148	rBV5	6647	16399	0.63%	0.094%
32	9.769	1149	1153	1160	rVV10	2901	6384	0.25%	0.036%
33	9.863	1164	1169	1177	rVB5	6504	15008	0.58%	0.086%
34	10.010	1187	1194	1195	rBV6	3021	5540	0.21%	0.032%
35	10.057	1195	1202	1216	rVV	104650	192709	7.46%	1.101%
36	10.422	1253	1264	1278	rBV	659656	1038999	40.20%	5.938%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	10.563	1281	1288	1300	rVV	53569	115735	4.48%	0.661%
38	10.898	1337	1345	1349	rBV	2386	4961	0.19%	0.028%
39	10.963	1349	1356	1362	rVV	5144	13213	0.51%	0.076%
40	11.222	1393	1400	1410	rBV8	5840	18311	0.71%	0.105%
41	11.440	1431	1437	1445	rBV9	6050	14302	0.55%	0.082%
42	11.692	1474	1480	1486	rBV3	9020	15342	0.59%	0.088%
43	11.804	1493	1499	1502	rVV8	3540	8098	0.31%	0.046%
44	11.834	1502	1504	1509	rVB6	3412	4737	0.18%	0.027%
45	11.922	1512	1519	1524	rVB8	3430	6198	0.24%	0.035%
46	12.010	1531	1534	1538	rVB5	2349	3015	0.12%	0.017%
47	12.292	1579	1582	1591	rVB5	2611	6538	0.25%	0.037%
48	12.475	1608	1613	1617	rBV8	1927	3345	0.13%	0.019%
49	12.698	1648	1651	1656	rVB7	2724	4302	0.17%	0.025%
50	12.804	1664	1669	1673	rVB3	7009	10869	0.42%	0.062%
51	12.857	1673	1678	1682	rBV6	2011	4592	0.18%	0.026%
52	13.069	1709	1714	1716	rBV6	2951	4566	0.18%	0.026%
53	13.251	1743	1745	1750	rVB6	2859	3521	0.14%	0.020%
54	13.316	1754	1756	1764	rVB9	2878	4989	0.19%	0.029%
55	13.428	1769	1775	1776	rBV4	2115	3482	0.13%	0.020%
56	13.592	1796	1803	1808	rBV10	9134	17560	0.68%	0.100%
57	13.675	1808	1817	1826	rVV	266039	393883	15.24%	2.251%
58	13.751	1826	1830	1836	rVV6	10389	16523	0.64%	0.094%
59	13.969	1860	1867	1877	rVV	267669	408809	15.82%	2.336%
60	14.192	1900	1905	1907	rBV6	4250	7173	0.28%	0.041%
61	14.281	1912	1920	1926	rVV	1196615	1712279	66.25%	9.786%
62	14.339	1926	1930	1934	rVB2	13362	18557	0.72%	0.106%
63	14.528	1958	1962	1969	rBV2	21617	44596	1.73%	0.255%
64	14.698	1985	1991	1999	rVB7	22298	48199	1.86%	0.275%
65	14.810	2006	2010	2017	rBV10	5499	10214	0.40%	0.058%
66	14.898	2021	2025	2026	rBV4	3023	3595	0.14%	0.021%
67	15.286	2084	2091	2096	rBV	386246	561221	21.71%	3.207%
68	15.339	2096	2100	2107	rVB	17395	27967	1.08%	0.160%
69	15.416	2107	2113	2121	rBV	22166	45070	1.74%	0.258%
70	15.498	2125	2127	2131	rVB4	3402	3538	0.14%	0.020%
71	15.563	2134	2138	2143	rBV3	17082	23727	0.92%	0.136%
72	15.651	2148	2153	2159	rVB	79290	100002	3.87%	0.572%
73	16.045	2212	2220	2226	rVB3	20400	44389	1.72%	0.254%
74	16.622	2315	2318	2320	rBV4	7240	7842	0.30%	0.045%
75	16.898	2360	2365	2373	rVB3	26083	41240	1.60%	0.236%
76	17.063	2387	2393	2398	rBV	1492692	2227434	86.18%	12.730%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022483.D
 Acq On : 19 Oct 2024 19:40
 Operator : RC/JU
 Sample : P4361-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

77	17.110	2398	2401	2407	rVB	128583	199107	7.70%	1.138%
78	17.180	2407	2413	2419	rBV	348004	601082	23.26%	3.435%
79	17.286	2427	2431	2436	rVB7	23902	32107	1.24%	0.183%
80	17.386	2442	2448	2455	rVB4	18008	39108	1.51%	0.224%
81	17.492	2462	2466	2467	rBV3	10605	14038	0.54%	0.080%
82	17.980	2545	2549	2550	rBV	25503	29477	1.14%	0.168%
83	18.004	2550	2553	2556	rBV2	45398	62980	2.44%	0.360%
84	18.104	2568	2570	2575	rVB3	15211	17819	0.69%	0.102%
85	18.174	2577	2582	2586	rBV3	39265	66531	2.57%	0.380%
86	18.492	2633	2636	2641	rVB	21441	27819	1.08%	0.159%
87	18.598	2651	2654	2658	rBV2	19912	30109	1.16%	0.172%
88	18.751	2677	2680	2682	rVB4	18101	19876	0.77%	0.114%
89	18.933	2707	2711	2715	rBV2	17005	22434	0.87%	0.128%
90	19.198	2751	2756	2762	rVB	363825	488333	18.89%	2.791%
91	19.257	2764	2766	2771	rVB4	27038	38641	1.50%	0.221%
92	19.545	2810	2815	2818	rBV2	489766	723265	27.98%	4.134%
93	19.574	2818	2820	2824	rVB	190301	227409	8.80%	1.300%
94	20.104	2906	2910	2914	rVB	94232	122036	4.72%	0.697%
95	20.204	2923	2927	2932	rBV	107739	144887	5.61%	0.828%
96	21.498	3139	3147	3152	rBV	1373779	2584610	100.00%	14.772%
97	21.545	3152	3155	3166	rVB	235741	376003	14.55%	2.149%
98	23.721	3522	3525	3532	rVB	83945	166274	6.43%	0.950%
99	24.521	3656	3661	3668	rVB	140806	274420	10.62%	1.568%
100	24.751	3692	3700	3711	rVB	774068	2055465	79.53%	11.747%




Sum of corrected areas: 17497228

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

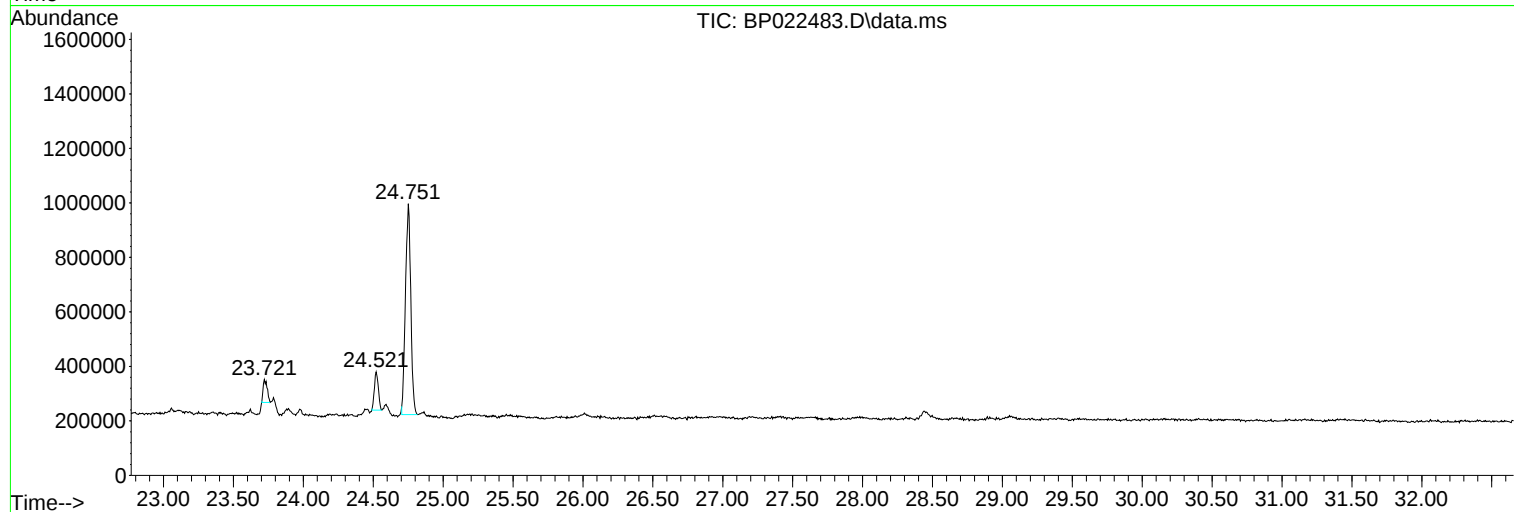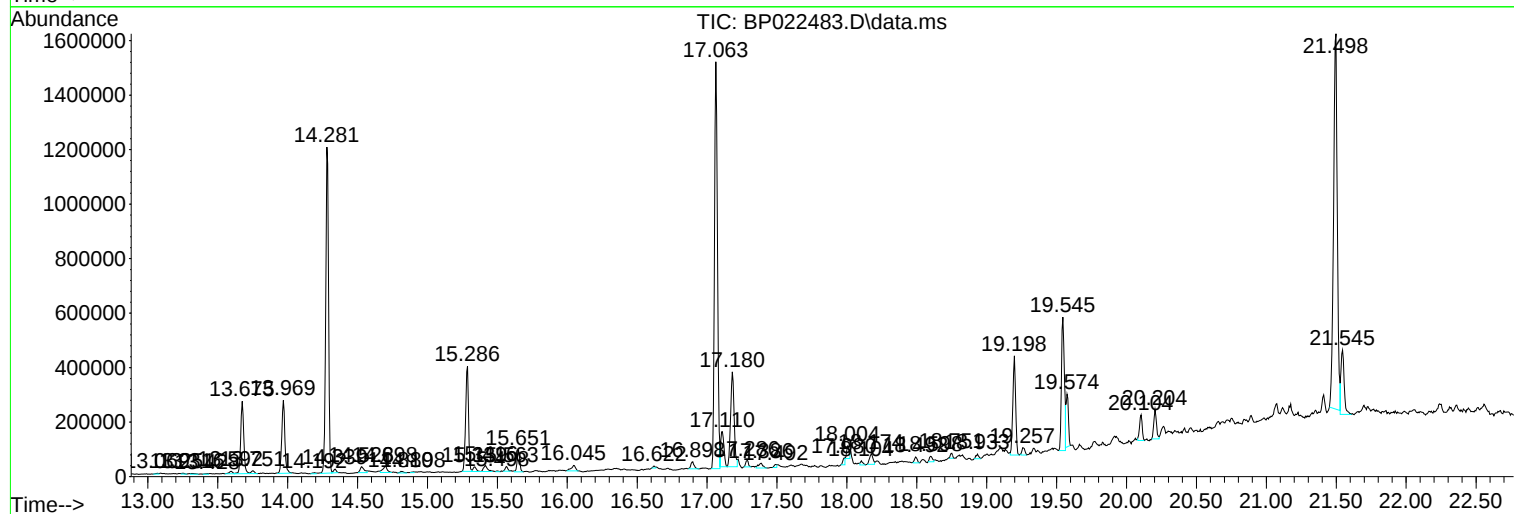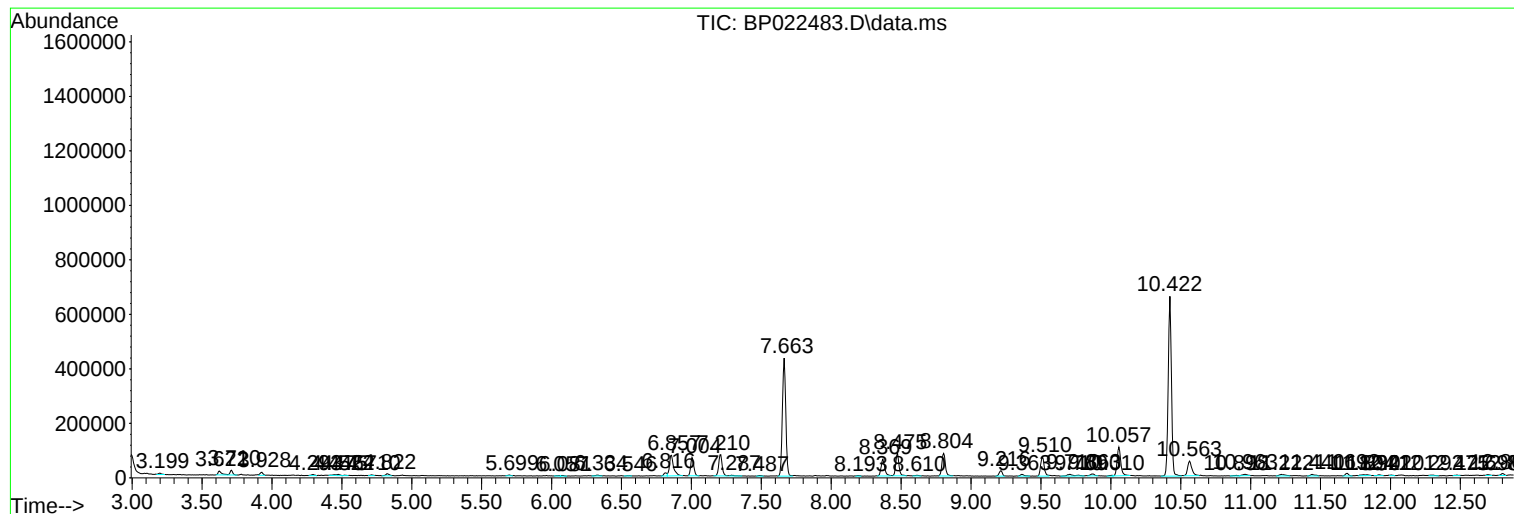

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022483.D
Acq On : 19 Oct 2024 19:40
Operator : RC/JU
Sample : P4361-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------