

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022497.D
 Acq On : 20 Oct 2024 05:50
 Operator : RC/JU
 Sample : P4361-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	41	rVB	25699	33259	1.13%	0.092%
2	3.605	101	105	119	rBV	344219	513967	17.40%	1.419%
3	3.928	155	160	164	rBV	17277	25801	0.87%	0.071%
4	4.822	307	312	315	rBV7	2031	3728	0.13%	0.010%
5	5.069	349	354	361	rBV5	5752	9758	0.33%	0.027%
6	6.611	610	616	622	rBV10	3023	6513	0.22%	0.018%
7	6.852	645	657	673	rBV	480806	851927	28.84%	2.352%
8	7.005	675	683	693	rVB	376403	593034	20.08%	1.637%
9	7.205	710	717	729	rBV	497402	804397	27.23%	2.221%
10	7.663	787	795	802	rBV	560356	906783	30.70%	2.504%
11	7.734	803	807	812	rVB	8281	12871	0.44%	0.036%
12	7.881	826	832	836	rBV8	2348	3665	0.12%	0.010%
13	8.363	906	914	930	rBV	645157	1095956	37.10%	3.026%
14	8.799	981	988	998	rBV	502349	842771	28.53%	2.327%
15	8.869	998	1000	1004	rVV5	3132	4018	0.14%	0.011%
16	8.957	1008	1015	1020	rBV10	3023	5458	0.18%	0.015%
17	9.210	1052	1058	1064	rBV2	19388	30989	1.05%	0.086%
18	9.357	1075	1083	1090	rBV2	50865	83447	2.83%	0.230%
19	9.516	1101	1110	1122	rBV	423352	765997	25.93%	2.115%
20	10.052	1192	1201	1215	rBV	711995	1225025	41.47%	3.382%
21	10.422	1255	1264	1278	rVB	738478	1285409	43.52%	3.549%
22	10.552	1278	1286	1302	rBV	569937	1083188	36.67%	2.991%
23	10.710	1310	1313	1318	rVB6	1988	3009	0.10%	0.008%
24	10.887	1340	1343	1349	rVB7	1805	3267	0.11%	0.009%
25	10.963	1349	1356	1363	rBV7	9856	23544	0.80%	0.065%
26	11.222	1396	1400	1403	rBV6	2657	4317	0.15%	0.012%
27	11.693	1473	1480	1486	rBV3	8988	15932	0.54%	0.044%
28	11.828	1497	1503	1510	rVB8	4941	9477	0.32%	0.026%
29	11.928	1513	1520	1523	rBV8	2937	5984	0.20%	0.017%
30	12.004	1526	1533	1539	rVB	12689	22939	0.78%	0.063%
31	12.075	1539	1545	1548	rBV7	1516	3247	0.11%	0.009%
32	12.246	1565	1574	1580	rBV3	3969	8577	0.29%	0.024%
33	12.416	1598	1603	1607	rBV8	1762	3307	0.11%	0.009%
34	13.093	1716	1718	1725	rVB8	2733	4109	0.14%	0.011%
35	13.228	1737	1741	1748	rVB8	4177	7484	0.25%	0.021%
36	13.587	1798	1802	1807	rVB8	2600	5088	0.17%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022497.D
 Acq On : 20 Oct 2024 05:50
 Operator : RC/JU
 Sample : P4361-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	13.675	1810	1817	1827	rBV	1307145	1977116	66.94%	5.459%
38	13.781	1833	1835	1843	rVB9	3110	5710	0.19%	0.016%
39	13.963	1855	1866	1883	rBV	1512822	2175128	73.64%	6.006%
40	14.269	1908	1918	1926	rBV	1243510	1863439	63.09%	5.145%
41	14.340	1926	1930	1935	rVV4	5596	9176	0.31%	0.025%
42	14.398	1937	1940	1944	rBV6	2740	3306	0.11%	0.009%
43	14.498	1950	1957	1972	rBV	246384	435846	14.76%	1.203%
44	14.704	1987	1992	2000	rVB3	20058	32029	1.08%	0.088%
45	15.275	2080	2089	2097	rBV	1841837	2777736	94.04%	7.669%
46	15.334	2097	2099	2104	rVB5	4237	6002	0.20%	0.017%
47	15.422	2107	2114	2122	rBV	236920	366320	12.40%	1.011%
48	15.516	2127	2130	2139	rVB8	8534	18994	0.64%	0.052%
49	15.651	2146	2153	2161	rBV	313590	531227	17.98%	1.467%
50	15.769	2169	2173	2176	rBV6	2423	3768	0.13%	0.010%
51	15.851	2185	2187	2192	rVB6	3571	4405	0.15%	0.012%
52	16.022	2210	2216	2218	rBV7	5010	10068	0.34%	0.028%
53	16.075	2223	2225	2230	rVB	7075	9518	0.32%	0.026%
54	16.469	2288	2292	2295	rVV5	9004	12610	0.43%	0.035%
55	16.551	2304	2306	2310	rVB5	3411	3617	0.12%	0.010%
56	16.828	2350	2353	2355	rBV4	4595	5133	0.17%	0.014%
57	17.075	2387	2395	2401	rBV	1283454	2050782	69.43%	5.662%
58	17.122	2401	2403	2407	rVV	45288	58668	1.99%	0.162%
59	17.175	2407	2412	2424	rVV	2135229	2741402	92.81%	7.569%
60	17.275	2425	2429	2434	rVB5	19994	34374	1.16%	0.095%
61	17.392	2445	2449	2455	rVB7	9098	19160	0.65%	0.053%
62	18.010	2549	2554	2564	rBV	304325	456915	15.47%	1.262%
63	19.098	2735	2739	2744	rBV3	20438	30894	1.05%	0.085%
64	19.198	2747	2756	2764	rBV2	96157	186760	6.32%	0.516%
65	19.339	2775	2780	2788	rBV	134625	232649	7.88%	0.642%
66	19.545	2809	2815	2824	rBV	1972659	2870325	97.18%	7.925%
67	21.504	3142	3148	3154	rBV	1299364	1971776	66.76%	5.444%
68	24.527	3653	3662	3673	rBV	1154571	2953750	100.00%	8.155%
69	24.751	3692	3700	3711	rVB	764542	2051735	69.46%	5.665%




Sum of corrected areas: 36218580

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022497.D
Acq On : 20 Oct 2024 05:50
Operator : RC/JU
Sample : P4361-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

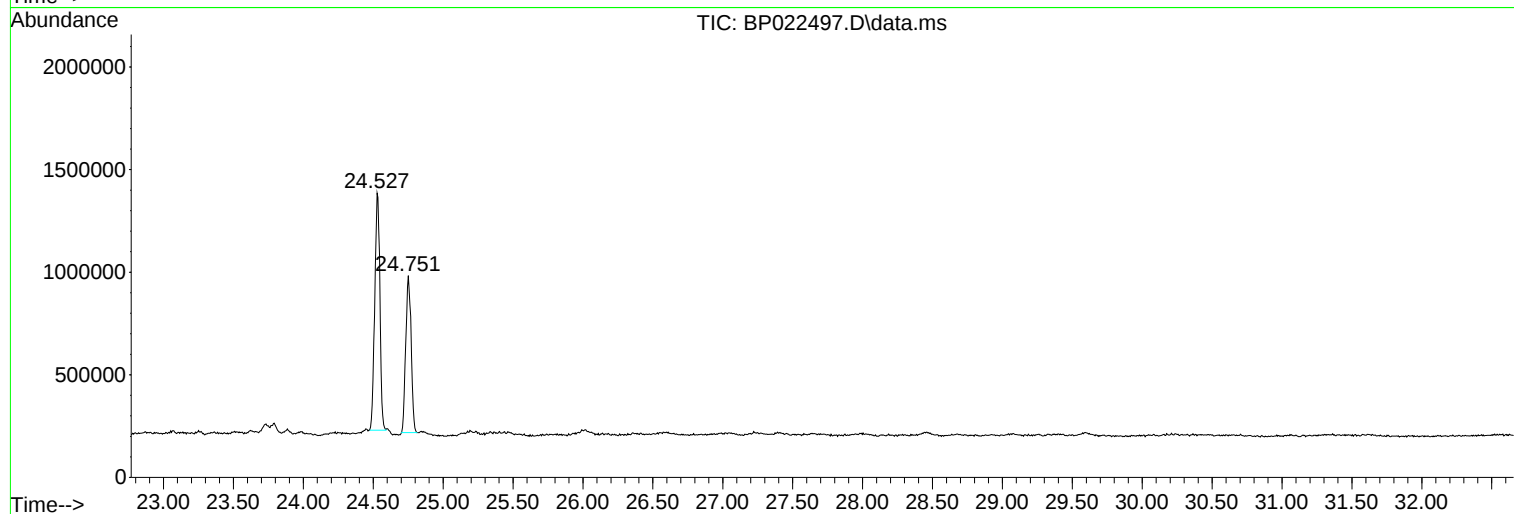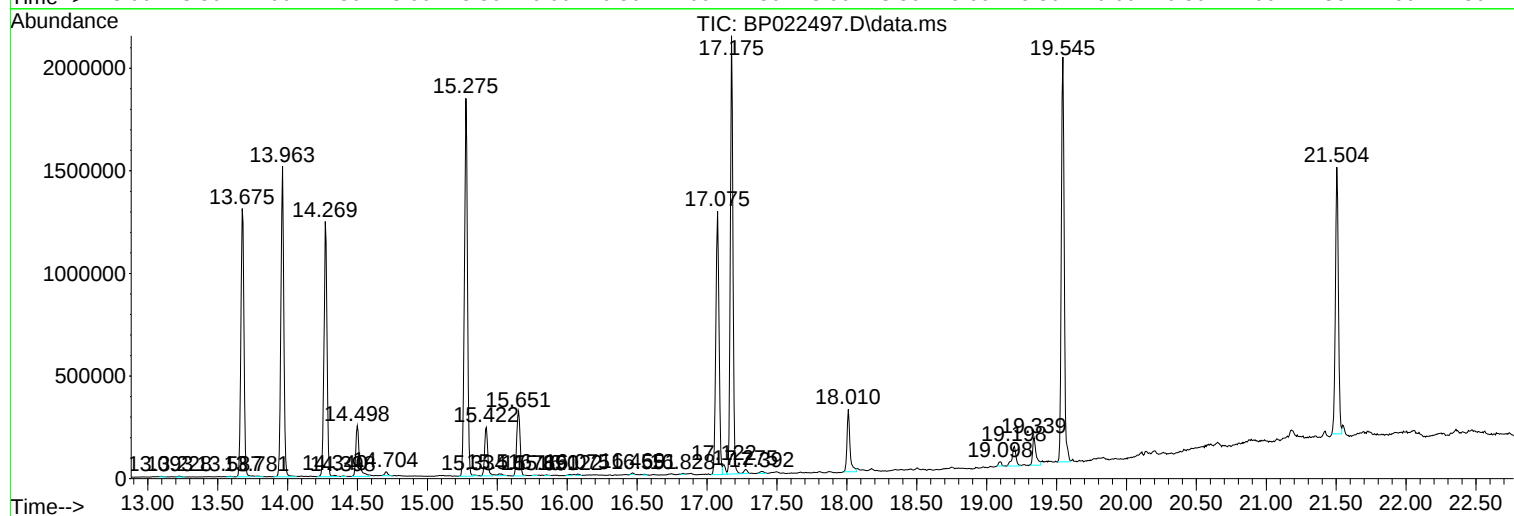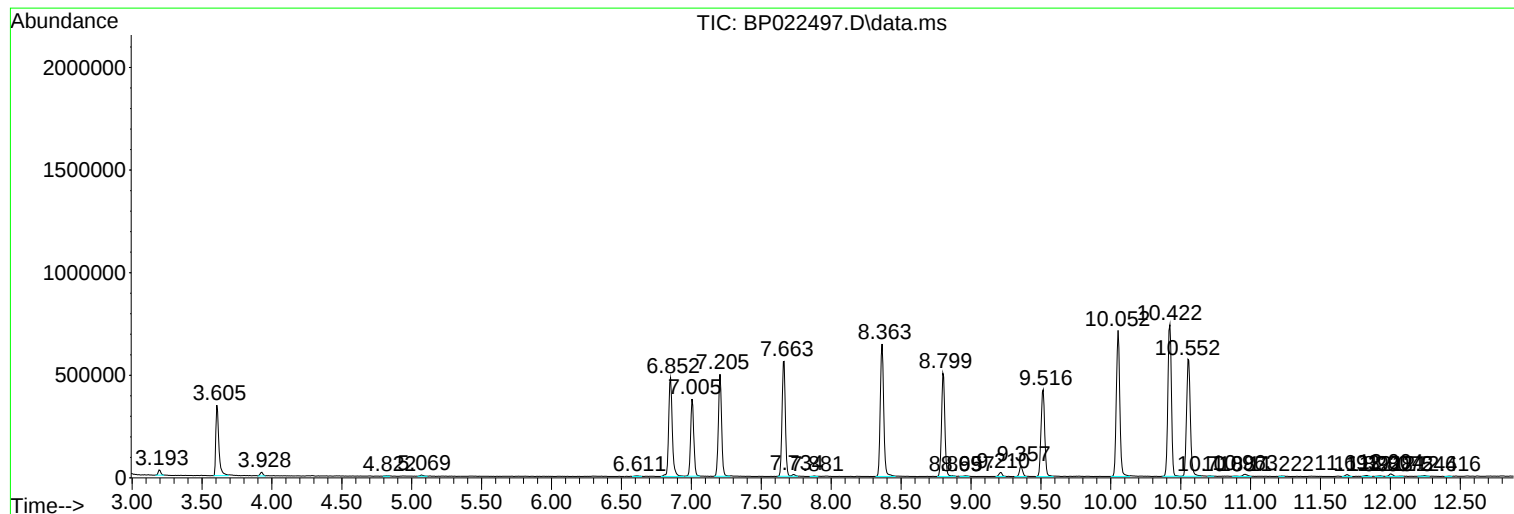

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022497.D
Acq On : 20 Oct 2024 05:50
Operator : RC/JU
Sample : P4361-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022497.D
Acq On : 20 Oct 2024 05:50
Operator : RC/JU
Sample : P4361-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------