

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022499.D
Acq On : 20 Oct 2024 07:10
Operator : RC/JU
Sample : P4361-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BP022499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	16	18	24	rVB7	3797	6435	0.34%	0.048%
2	3.199	33	36	41	rVB3	5211	6554	0.35%	0.049%
3	3.617	103	107	110	rBV5	2553	4084	0.22%	0.030%
4	3.711	120	123	131	rVB	11455	15834	0.84%	0.118%
5	3.893	151	154	155	rVV3	3210	3382	0.18%	0.025%
6	3.928	157	160	167	rVB	7798	10967	0.58%	0.082%
7	4.093	184	188	192	rVB7	1273	2085	0.11%	0.015%
8	4.293	217	222	227	rBV6	3698	7021	0.37%	0.052%
9	4.452	245	249	251	rVV5	3087	5325	0.28%	0.040%
10	4.475	251	253	259	rVB5	3887	5259	0.28%	0.039%
11	4.717	290	294	298	rBV7	3229	4337	0.23%	0.032%
12	4.828	307	313	321	rBV2	8305	16998	0.90%	0.126%
13	4.928	325	330	332	rBV6	1620	2970	0.16%	0.022%
14	5.693	455	460	467	rBV6	2193	5015	0.27%	0.037%
15	6.046	515	520	521	rBV5	1790	2431	0.13%	0.018%
16	6.070	521	524	529	rVB7	2570	4362	0.23%	0.032%
17	6.328	563	568	576	rVB2	4143	7037	0.37%	0.052%
18	6.540	601	604	611	rBV8	1694	3157	0.17%	0.023%
19	6.669	623	626	629	rVB5	1544	2024	0.11%	0.015%
20	6.858	653	658	673	rVB2	79146	157622	8.33%	1.172%
21	7.005	676	683	691	rBV	66410	106127	5.61%	0.789%
22	7.211	710	718	728	rBV	82783	140523	7.43%	1.045%
23	7.293	728	732	734	rVB5	1497	1981	0.10%	0.015%
24	7.481	761	764	770	rBV5	2586	4892	0.26%	0.036%
25	7.664	787	795	804	rBV	497484	803326	42.46%	5.971%
26	7.781	812	815	820	rVB7	1107	1915	0.10%	0.014%
27	7.887	829	833	837	rBV7	1887	2310	0.12%	0.017%
28	7.964	842	846	847	rBV4	2078	2061	0.11%	0.015%
29	7.975	847	848	851	rVB3	2342	1927	0.10%	0.014%
30	8.187	881	884	888	rBV6	2103	3673	0.19%	0.027%
31	8.369	908	915	925	rVV2	55426	106091	5.61%	0.789%
32	8.475	927	933	945	rVB2	66888	111132	5.87%	0.826%
33	8.616	950	957	959	rBV8	2094	4220	0.22%	0.031%
34	8.805	982	989	998	rBV	82177	141851	7.50%	1.054%
35	8.958	1011	1015	1016	rBV4	2572	2583	0.14%	0.019%
36	9.211	1052	1058	1064	rBV2	15947	25166	1.33%	0.187%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022499.D
Acq On : 20 Oct 2024 07:10
Operator : RC/JU
Sample : P4361-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	9.363	1076	1084	1092	rVB8	6454	13964	0.74%	0.104%
38	9.516	1103	1110	1119	rBV2	69586	121875	6.44%	0.906%
39	9.710	1134	1143	1145	rBV8	4483	9604	0.51%	0.071%
40	9.763	1150	1152	1160	rVB9	2557	4685	0.25%	0.035%
41	9.869	1165	1170	1176	rVB2	6850	13614	0.72%	0.101%
42	10.058	1195	1202	1213	rVV	100513	187837	9.93%	1.396%
43	10.134	1213	1215	1222	rVB8	2454	5012	0.26%	0.037%
44	10.422	1255	1264	1277	rBV	706942	1144020	60.46%	8.503%
45	10.563	1281	1288	1299	rBV2	50792	110928	5.86%	0.825%
46	10.899	1341	1345	1350	rVB7	2859	4337	0.23%	0.032%
47	10.975	1353	1358	1365	rVV7	3744	8085	0.43%	0.060%
48	11.093	1373	1378	1379	rBV3	1470	1954	0.10%	0.015%
49	11.222	1394	1400	1406	rBV7	5271	12059	0.64%	0.090%
50	11.310	1414	1415	1422	rVB7	1442	2261	0.12%	0.017%
51	11.446	1432	1438	1440	rBV5	4507	8038	0.42%	0.060%
52	11.599	1461	1464	1468	rBV6	1875	2592	0.14%	0.019%
53	11.687	1474	1479	1487	rBV5	8294	15786	0.83%	0.117%
54	11.793	1491	1497	1499	rBV6	2967	5553	0.29%	0.041%
55	11.834	1499	1504	1507	rVB7	1857	3340	0.18%	0.025%
56	12.010	1530	1534	1540	rVB7	2199	4521	0.24%	0.034%
57	12.469	1610	1612	1619	rVB8	2741	4249	0.22%	0.032%
58	12.710	1646	1653	1659	rBV10	3023	6552	0.35%	0.049%
59	12.804	1665	1669	1673	rVV5	7141	10800	0.57%	0.080%
60	12.863	1674	1679	1682	rVV7	2096	4302	0.23%	0.032%
61	13.087	1711	1717	1722	rVV10	2660	6599	0.35%	0.049%
62	13.193	1729	1735	1736	rVB5	1461	2216	0.12%	0.016%
63	13.599	1800	1804	1810	rVB9	4422	8086	0.43%	0.060%
64	13.681	1811	1818	1828	rVV	199352	343491	18.15%	2.553%
65	13.757	1828	1831	1836	rVB4	6646	9908	0.52%	0.074%
66	13.969	1860	1867	1878	rVB	228622	360106	19.03%	2.677%
67	14.099	1885	1889	1890	rBV4	2897	3086	0.16%	0.023%
68	14.187	1900	1904	1907	rBV5	2762	3918	0.21%	0.029%
69	14.275	1911	1919	1926	rVV	1250723	1665202	88.01%	12.377%
70	14.340	1928	1930	1934	rVB5	4134	4794	0.25%	0.036%
71	14.528	1954	1962	1969	rBV5	19658	48450	2.56%	0.360%
72	14.704	1987	1992	2000	rVB7	13809	28506	1.51%	0.212%
73	14.810	2008	2010	2020	rVB7	2912	5315	0.28%	0.040%
74	15.281	2084	2090	2098	rBV	322648	477363	25.23%	3.548%
75	15.440	2111	2117	2123	rVB8	13544	25578	1.35%	0.190%
76	15.557	2134	2137	2141	rBV4	6211	9000	0.48%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
 Data File : BP022499.D
 Acq On : 20 Oct 2024 07:10
 Operator : RC/JU
 Sample : P4361-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

77	15.645	2148	2152	2160	rVB	47822	75529	3.99%	0.561%
78	15.781	2169	2175	2176	rBV6	2905	5116	0.27%	0.038%
79	15.875	2185	2191	2192	rBV6	4676	8682	0.46%	0.065%
80	16.022	2214	2216	2218	rBV3	3028	3237	0.17%	0.024%
81	16.610	2312	2316	2322	rBV4	13625	23436	1.24%	0.174%
82	16.851	2353	2357	2358	rBV3	5954	7617	0.40%	0.057%
83	16.887	2358	2363	2372	rVB7	13825	29154	1.54%	0.217%
84	17.069	2387	2394	2400	rBV	1003476	1781479	94.16%	13.242%
85	17.116	2400	2402	2407	rVV	30397	45883	2.43%	0.341%
86	17.175	2407	2412	2423	rVV2	304470	463110	24.48%	3.442%
87	17.275	2425	2429	2436	rVB9	19085	28986	1.53%	0.215%
88	17.375	2444	2446	2451	rVB5	7869	11985	0.63%	0.089%
89	17.487	2463	2465	2466	rBV2	4429	3747	0.20%	0.028%
90	17.887	2529	2533	2536	rBV5	7325	13425	0.71%	0.100%
91	17.992	2547	2551	2563	rVB9	36376	82997	4.39%	0.617%
92	18.175	2579	2582	2587	rBV4	8563	15379	0.81%	0.114%
93	18.598	2651	2654	2658	rVB5	11695	15217	0.80%	0.113%
94	18.834	2692	2694	2700	rVB5	9935	9722	0.51%	0.072%
95	19.204	2752	2757	2762	rBV	96412	136495	7.21%	1.015%
96	19.328	2776	2778	2781	rBV4	11618	13631	0.72%	0.101%
97	19.551	2811	2816	2825	rBV3	259192	493722	26.09%	3.670%
98	21.492	3140	3146	3153	rBV2	1020975	1613892	85.30%	11.996%
99	24.527	3658	3662	3670	rVB	116214	238802	12.62%	1.775%
100	24.757	3693	3701	3713	rVB	733125	1892052	100.00%	14.064%




Sum of corrected areas: 13453558

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022499.D
Acq On : 20 Oct 2024 07:10
Operator : RC/JU
Sample : P4361-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

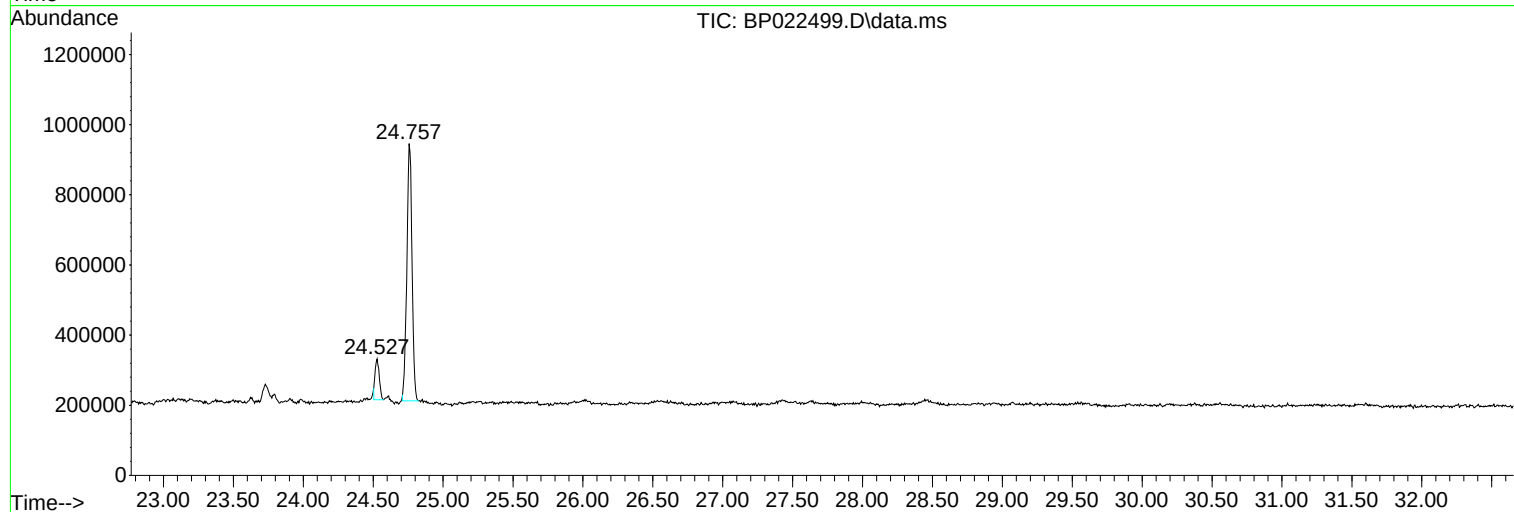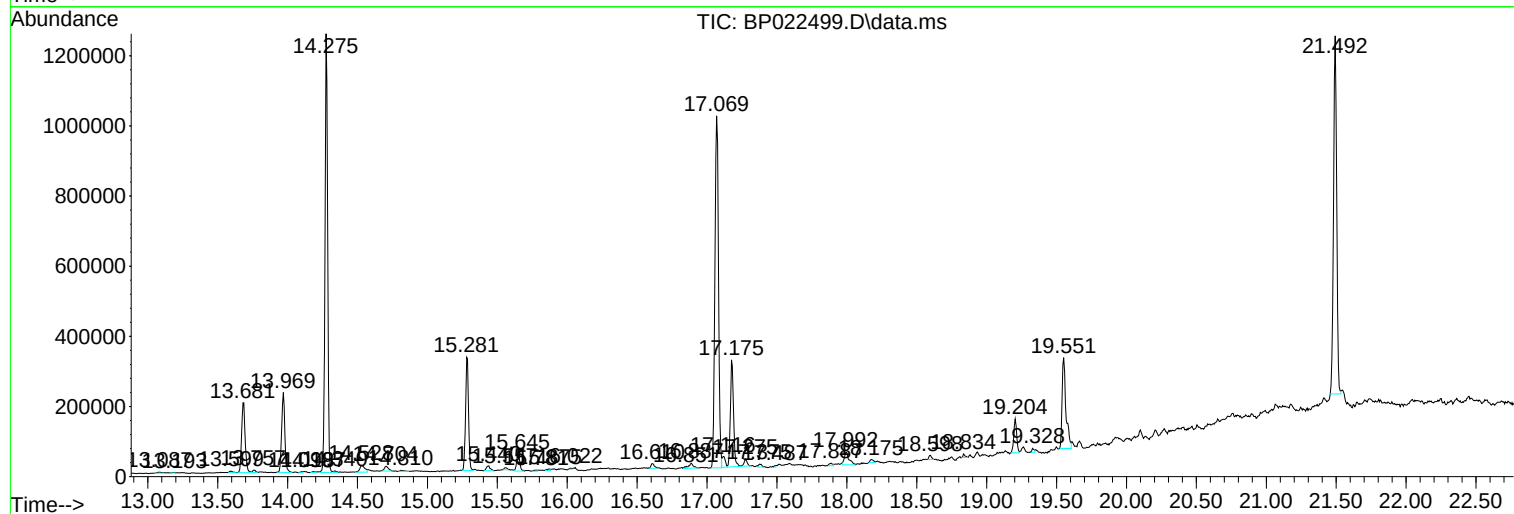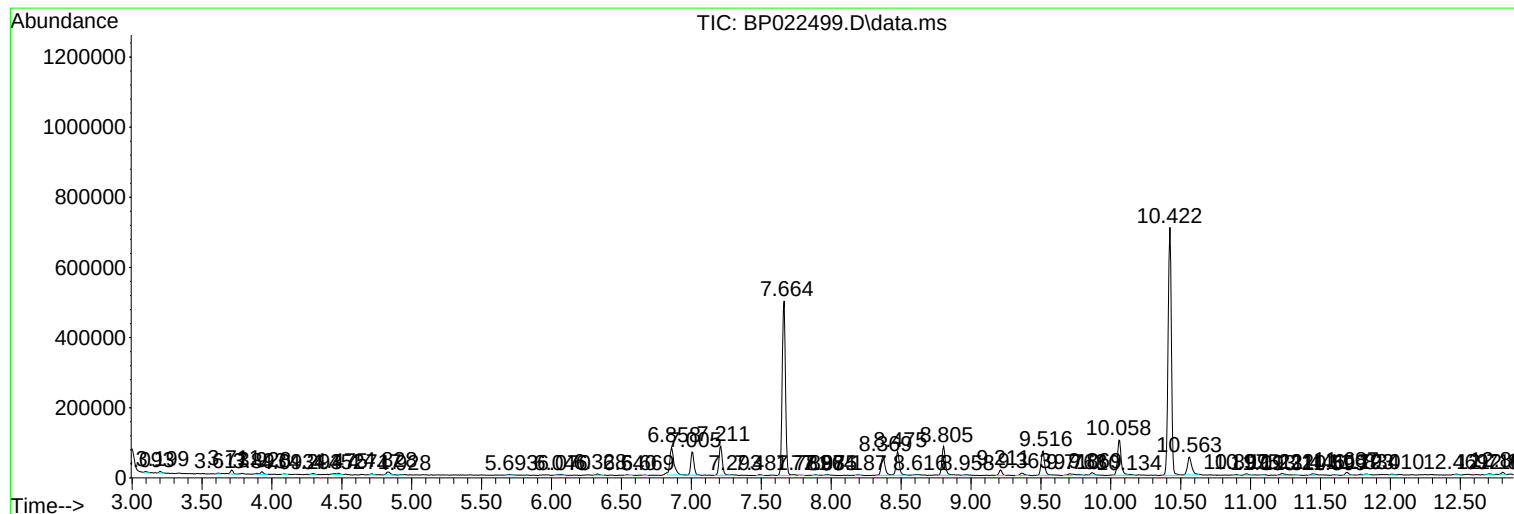

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022499.D
Acq On : 20 Oct 2024 07:10
Operator : RC/JU
Sample : P4361-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101924\
Data File : BP022499.D
Acq On : 20 Oct 2024 07:10
Operator : RC/JU
Sample : P4361-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------