

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102020\
 Data File : BP003674.D
 Acq On : 20 Oct 2020 10:50
 Operator : CG/JU
 Sample : PB132380BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132380BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	32	37	56	rVB	3695543	4543925	40.07%	9.331%
2	3.264	56	64	77	rVB3	43831	124709	1.10%	0.256%
3	6.022	525	533	544	rBV	2839298	4217368	37.19%	8.660%
4	7.675	801	814	830	rBV	2632185	4265939	37.62%	8.760%
5	8.528	951	959	967	rVB	544842	872096	7.69%	1.791%
6	9.693	1148	1157	1169	rBV	1774758	2954899	26.06%	6.068%
7	11.369	1433	1442	1453	rBV	662587	1128920	9.96%	2.318%
8	13.757	1840	1848	1860	rBV	4845381	6787231	59.86%	13.937%
9	15.128	2073	2081	2091	rBV2	1010738	1518956	13.40%	3.119%
10	16.598	2323	2331	2346	rBV	3491866	4870844	42.96%	10.002%
11	17.845	2535	2543	2552	rBV	1329997	1864087	16.44%	3.828%
12	20.310	2956	2962	2967	rBV	9716342	11338992	100.00%	23.284%
13	21.851	3218	3224	3235	rVB	1727134	2210888	19.50%	4.540%
14	24.427	3653	3662	3675	rVB	955117	1999998	17.64%	4.107%

Sum of corrected areas: 48698852

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102020\
Data File : BP003674.D
Acq On : 20 Oct 2020 10:50
Operator : CG/JU
Sample : PB132380BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132380BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.10 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.105	104.21 ng	4543930	1,4-Dichlorobenzene-d4	8.528

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	45
2			1-Hexen-4-ol, 1-chloro-3,5-dimet...	162	C8H15ClO	100244-09-5	9
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9
4			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
5			2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9

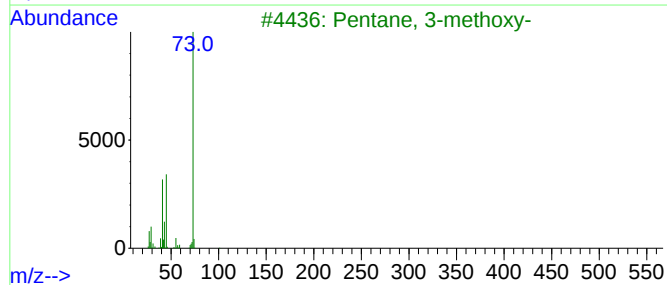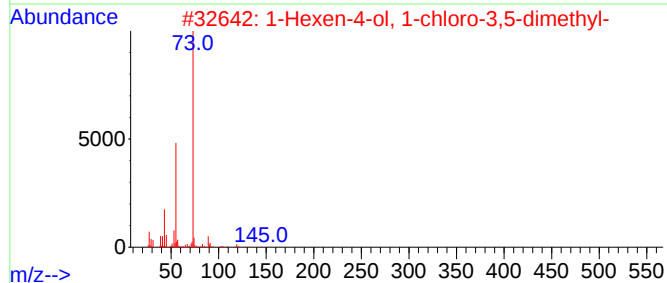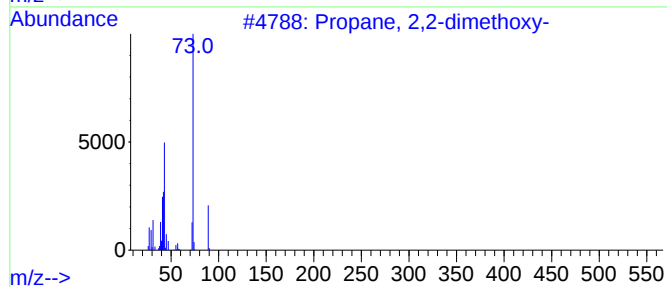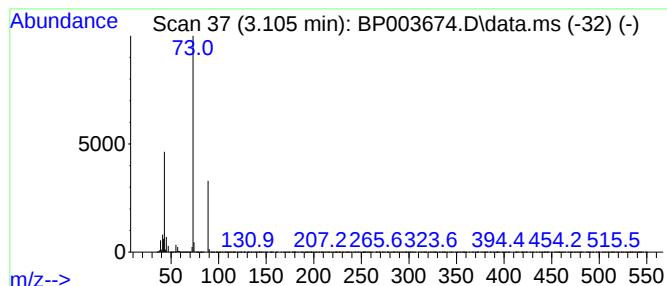

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102020\
Data File : BP003674.D
Acq On : 20 Oct 2020 10:50
Operator : CG/JU
Sample : PB132380BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132380BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.10	3.105	104.2	ng	4543930	1	8.528	872096	20.0