
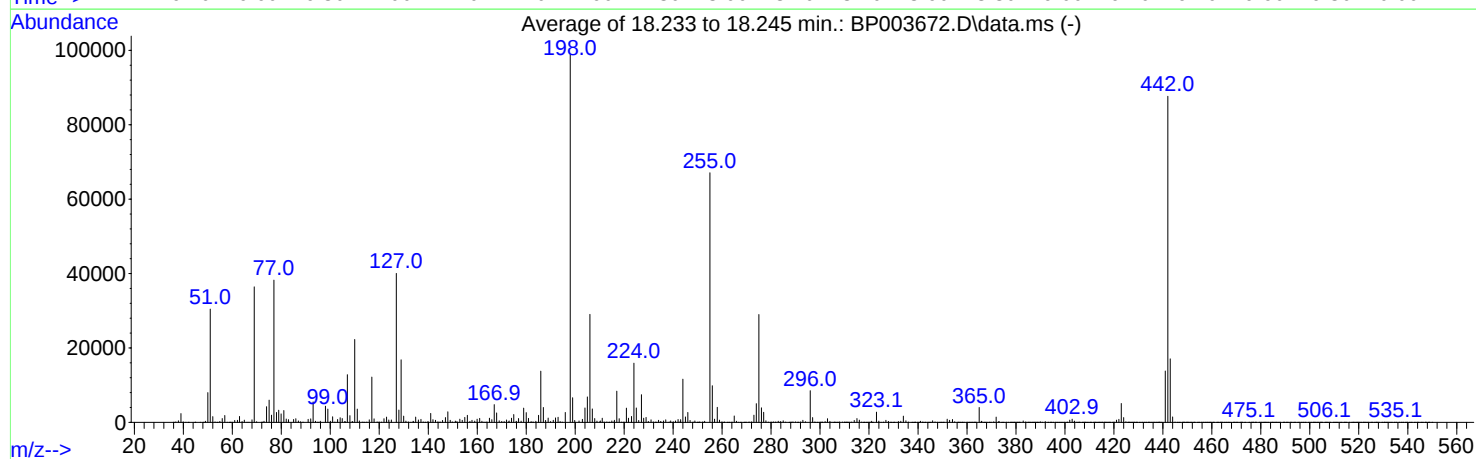


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102020\
 Data File : BP003672.D
 Acq On : 20 Oct 2020 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 19 14:54:24 2020

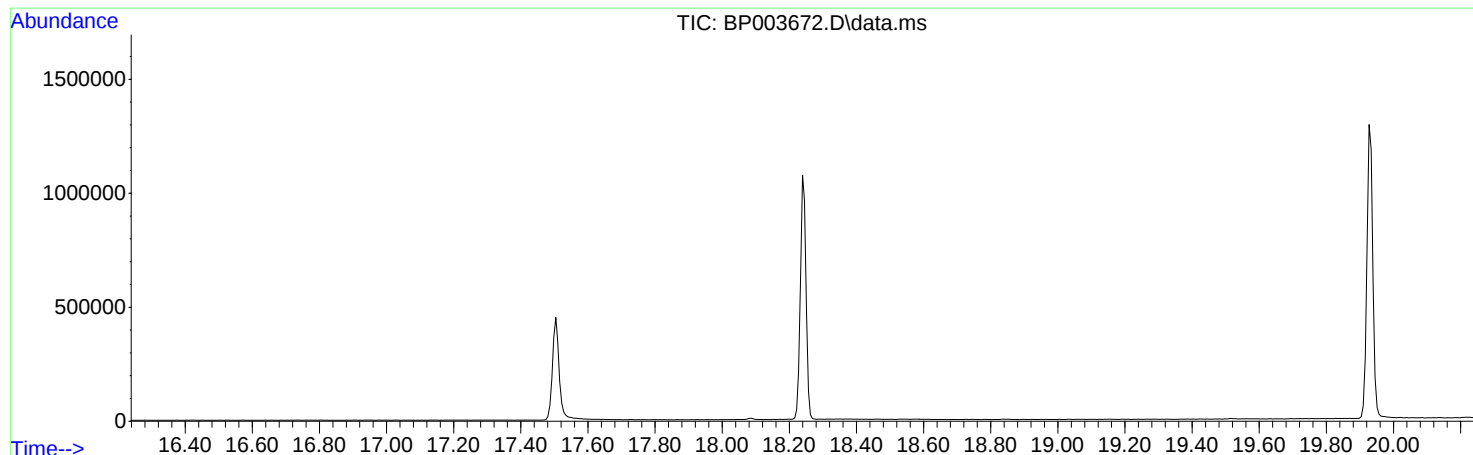

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	30466	PASS
68	69	0.00	2	1.9	675	PASS
69	198	0.00	100	36.8	36413	PASS
70	69	0.00	2	0.5	195	PASS
127	198	10	80	40.5	40043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98869	PASS
199	198	5	9	6.7	6642	PASS
275	198	10	60	29.3	28973	PASS
365	198	1	100	4.0	3996	PASS
441	198	0.01	100	14.0	13827	PASS
442	198	50	100	88.6	87643	PASS
443	442	15	24	19.5	17093	PASS