

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022503.D
 Acq On : 21 Oct 2024 13:24
 Operator : RC/JU
 Sample : PB164283BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK283

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	42	rVB	23151	30255	1.18%	0.132%
2	3.611	102	106	118	rBV	260393	392381	15.34%	1.713%
3	3.928	157	160	166	rVB3	4855	7081	0.28%	0.031%
4	6.857	650	658	669	rBV	314655	516261	20.18%	2.254%
5	7.005	677	683	694	rVB	240715	381341	14.90%	1.665%
6	7.210	709	718	732	rBV	321976	528528	20.66%	2.307%
7	7.663	785	795	803	rBV	286867	468085	18.29%	2.043%
8	8.369	906	915	929	rBV	374482	647595	25.31%	2.827%
9	8.804	980	989	1006	rBV	299900	523381	20.46%	2.285%
10	9.516	1102	1110	1125	rBV	257728	455515	17.80%	1.988%
11	10.051	1193	1201	1224	rBV	395325	693242	27.09%	3.026%
12	10.422	1256	1264	1274	rBV	346727	617225	24.12%	2.694%
13	10.557	1277	1287	1308	rBV	341996	652298	25.49%	2.848%
14	12.016	1528	1535	1541	rBV3	4983	10550	0.41%	0.046%
15	12.251	1570	1575	1582	rBV2	8400	16436	0.64%	0.072%
16	13.681	1811	1818	1832	rBV	756727	1118828	43.73%	4.884%
17	13.963	1859	1866	1878	rBV2	780161	1215924	47.52%	5.308%
18	14.275	1912	1919	1929	rBV	596533	916984	35.84%	4.003%
19	14.516	1953	1960	1975	rBV	234570	484148	18.92%	2.113%
20	15.286	2085	2091	2105	rBV	1272660	1596142	62.38%	6.968%
21	15.416	2105	2113	2121	rBV	341385	526001	20.56%	2.296%
22	15.533	2130	2133	2140	rVB6	4287	7306	0.29%	0.032%
23	15.863	2185	2189	2193	rBV5	1631	2711	0.11%	0.012%
24	16.251	2250	2255	2256	rBV5	1823	2697	0.11%	0.012%
25	17.075	2389	2395	2404	rBV	980399	1219637	47.67%	5.324%
26	17.169	2404	2411	2422	rVV	1054225	1818544	71.07%	7.939%
27	18.016	2552	2555	2561	rBV6	4804	8549	0.33%	0.037%
28	19.110	2737	2741	2747	rVB4	14038	21840	0.85%	0.095%
29	19.186	2750	2754	2758	rBV	18809	25849	1.01%	0.113%
30	19.563	2812	2818	2827	rBV	1695665	2285808	89.34%	9.978%
31	21.504	3142	3148	3158	rVB2	966867	1543717	60.33%	6.739%
32	24.551	3657	3666	3678	rVB	1053884	2558678	100.00%	11.170%
33	24.762	3694	3702	3715	rVB	592686	1614041	63.08%	7.046%


Sum of corrected areas: 22907578

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022503.D
Acq On : 21 Oct 2024 13:24
Operator : RC/JU
Sample : PB164283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK283

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

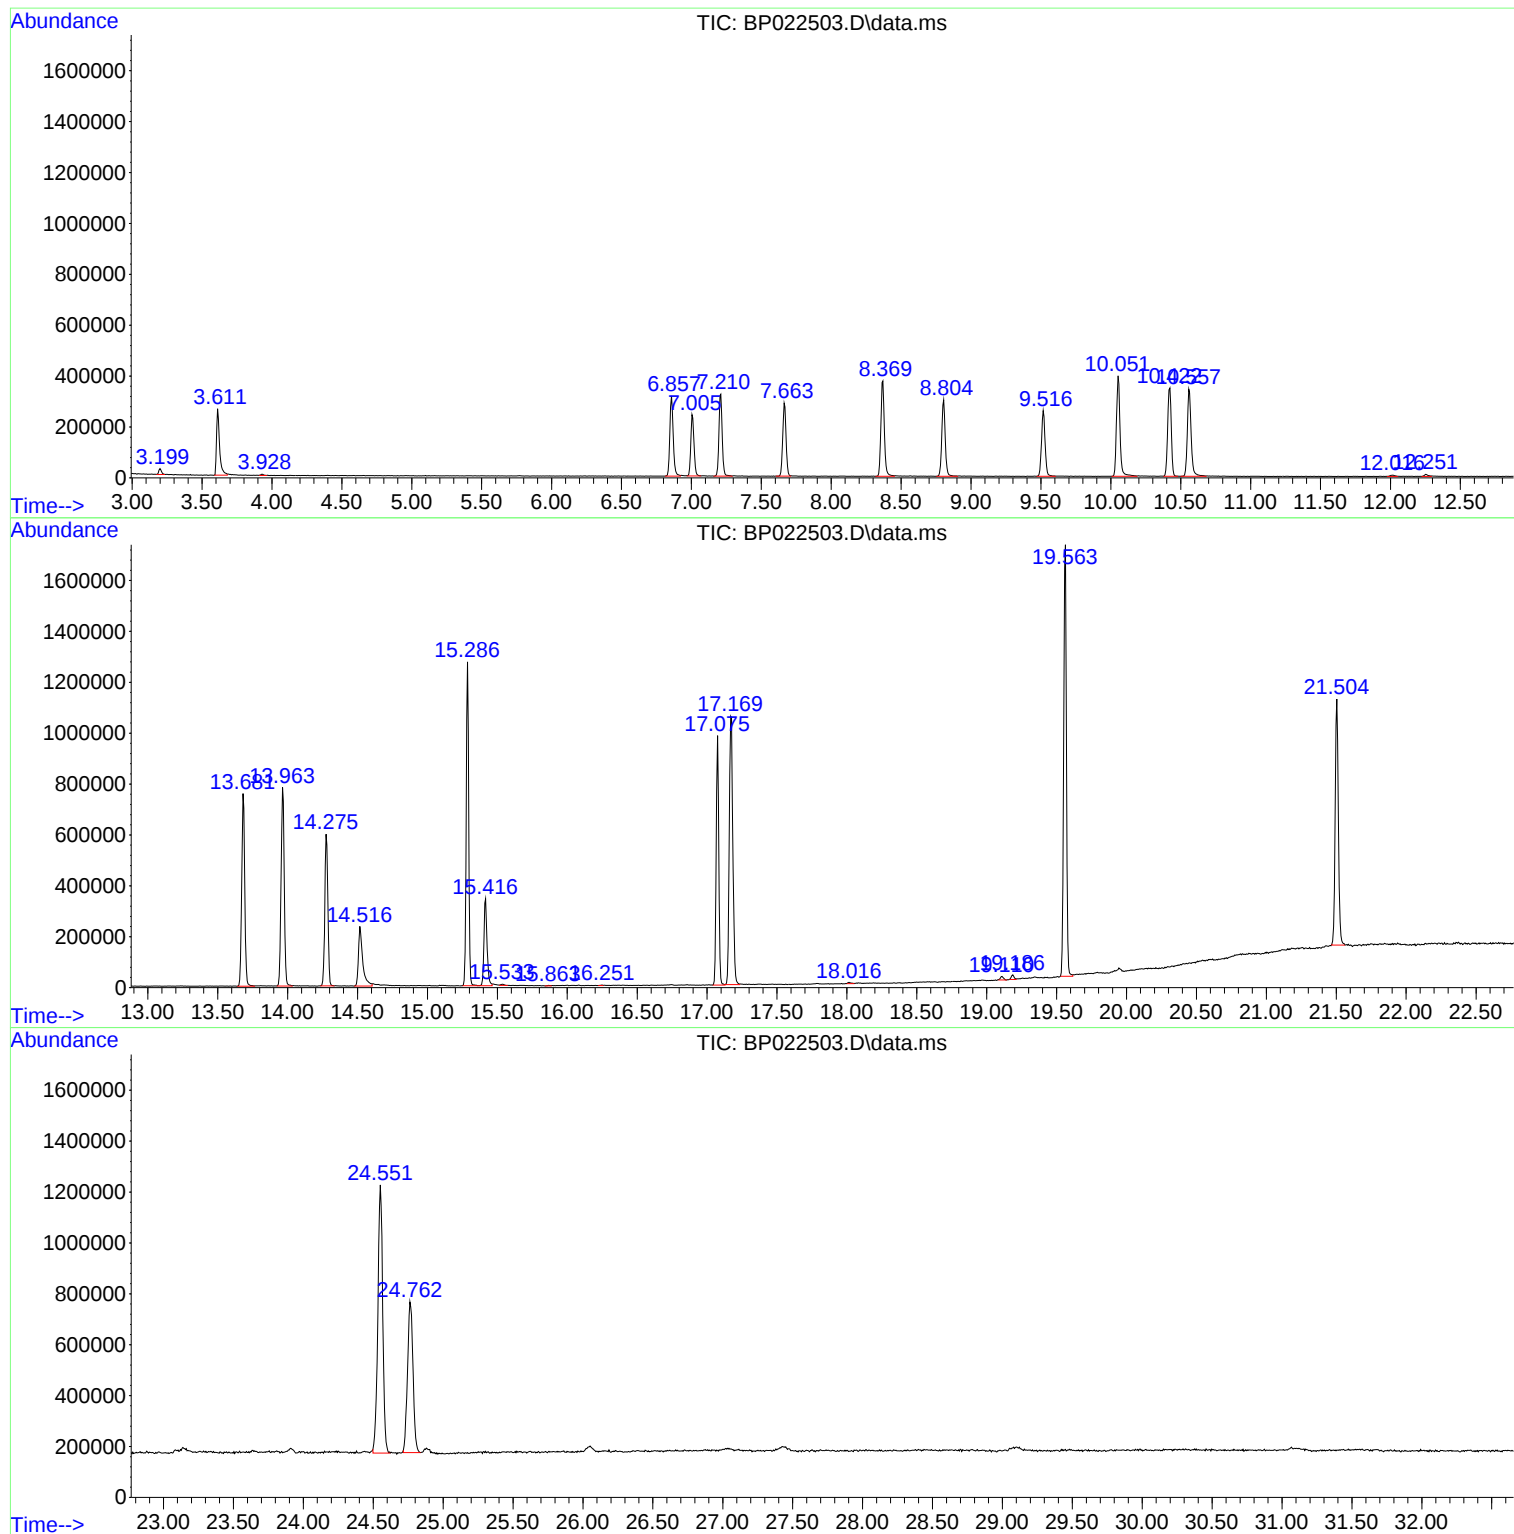

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022503.D
Acq On : 21 Oct 2024 13:24
Operator : RC/JU
Sample : PB164283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK283

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022503.D
Acq On : 21 Oct 2024 13:24
Operator : RC/JU
Sample : PB164283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK283

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc