

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022514.D
 Acq On : 21 Oct 2024 20:52
 Operator : RC/JU
 Sample : PB164300BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK300

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	42	rVB	24530	32243	1.07%	0.113%
2	3.611	102	106	123	rBV	290485	447801	14.92%	1.573%
3	3.928	155	160	164	rBV	6122	8401	0.28%	0.030%
4	6.810	644	650	653	rBV	37645	58199	1.94%	0.204%
5	6.857	653	658	676	rVV	366174	596985	19.89%	2.097%
6	7.005	676	683	697	rVV	276515	438402	14.61%	1.540%
7	7.205	708	717	733	rBV	365223	602324	20.07%	2.116%
8	7.663	788	795	804	rBV	390702	599316	19.97%	2.105%
9	8.363	902	914	929	rBV	451040	769363	25.64%	2.703%
10	8.799	980	988	998	rBV	359901	601683	20.05%	2.114%
11	9.210	1051	1058	1066	rBV	21788	33773	1.13%	0.119%
12	9.510	1103	1109	1121	rBV	323305	541652	18.05%	1.903%
13	10.051	1194	1201	1219	rBV	441787	820904	27.35%	2.884%
14	10.416	1255	1263	1278	rVB	490576	830524	27.68%	2.917%
15	10.557	1278	1287	1300	rBV	450963	770110	25.66%	2.705%
16	11.681	1475	1478	1484	rVB6	5513	8596	0.29%	0.030%
17	12.010	1529	1534	1542	rBV5	7396	14943	0.50%	0.052%
18	13.681	1809	1818	1829	rBV	969945	1328398	44.27%	4.666%
19	13.963	1859	1866	1878	rBV2	933655	1472943	49.08%	5.174%
20	14.275	1909	1919	1928	rBV	822272	1256935	41.88%	4.415%
21	14.498	1950	1957	1974	rBV	258338	592973	19.76%	2.083%
22	15.081	2052	2056	2059	rBV6	2099	3137	0.10%	0.011%
23	15.275	2082	2089	2102	rBV	1097445	1911041	63.68%	6.713%
24	15.416	2107	2113	2127	rBV	458086	630774	21.02%	2.216%
25	15.522	2127	2131	2135	rVB3	6679	11015	0.37%	0.039%
26	15.851	2184	2187	2194	rVB9	1784	3554	0.12%	0.012%
27	16.851	2352	2357	2361	rBV7	3770	7385	0.25%	0.026%
28	17.080	2386	2396	2403	rBV	1091789	1673727	55.77%	5.879%
29	17.175	2406	2412	2424	rVV	1666077	2244584	74.80%	7.885%
30	17.375	2444	2446	2448	rBV3	3019	3408	0.11%	0.012%
31	19.104	2736	2740	2746	rVB3	18365	26075	0.87%	0.092%
32	19.180	2749	2753	2757	rBV	27127	34001	1.13%	0.119%
33	19.557	2811	2817	2822	rBV	2265111	2853137	95.07%	10.022%
34	21.504	3142	3148	3155	rVB	1326572	2065837	68.84%	7.257%
35	24.551	3655	3666	3676	rVB	1105695	3000972	100.00%	10.542%
36	24.768	3695	3703	3715	rVB	853202	2172872	72.41%	7.633%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022514.D
Acq On : 21 Oct 2024 20:52
Operator : RC/JU
Sample : PB164300BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 28467987

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022514.D
Acq On : 21 Oct 2024 20:52
Operator : RC/JU
Sample : PB164300BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

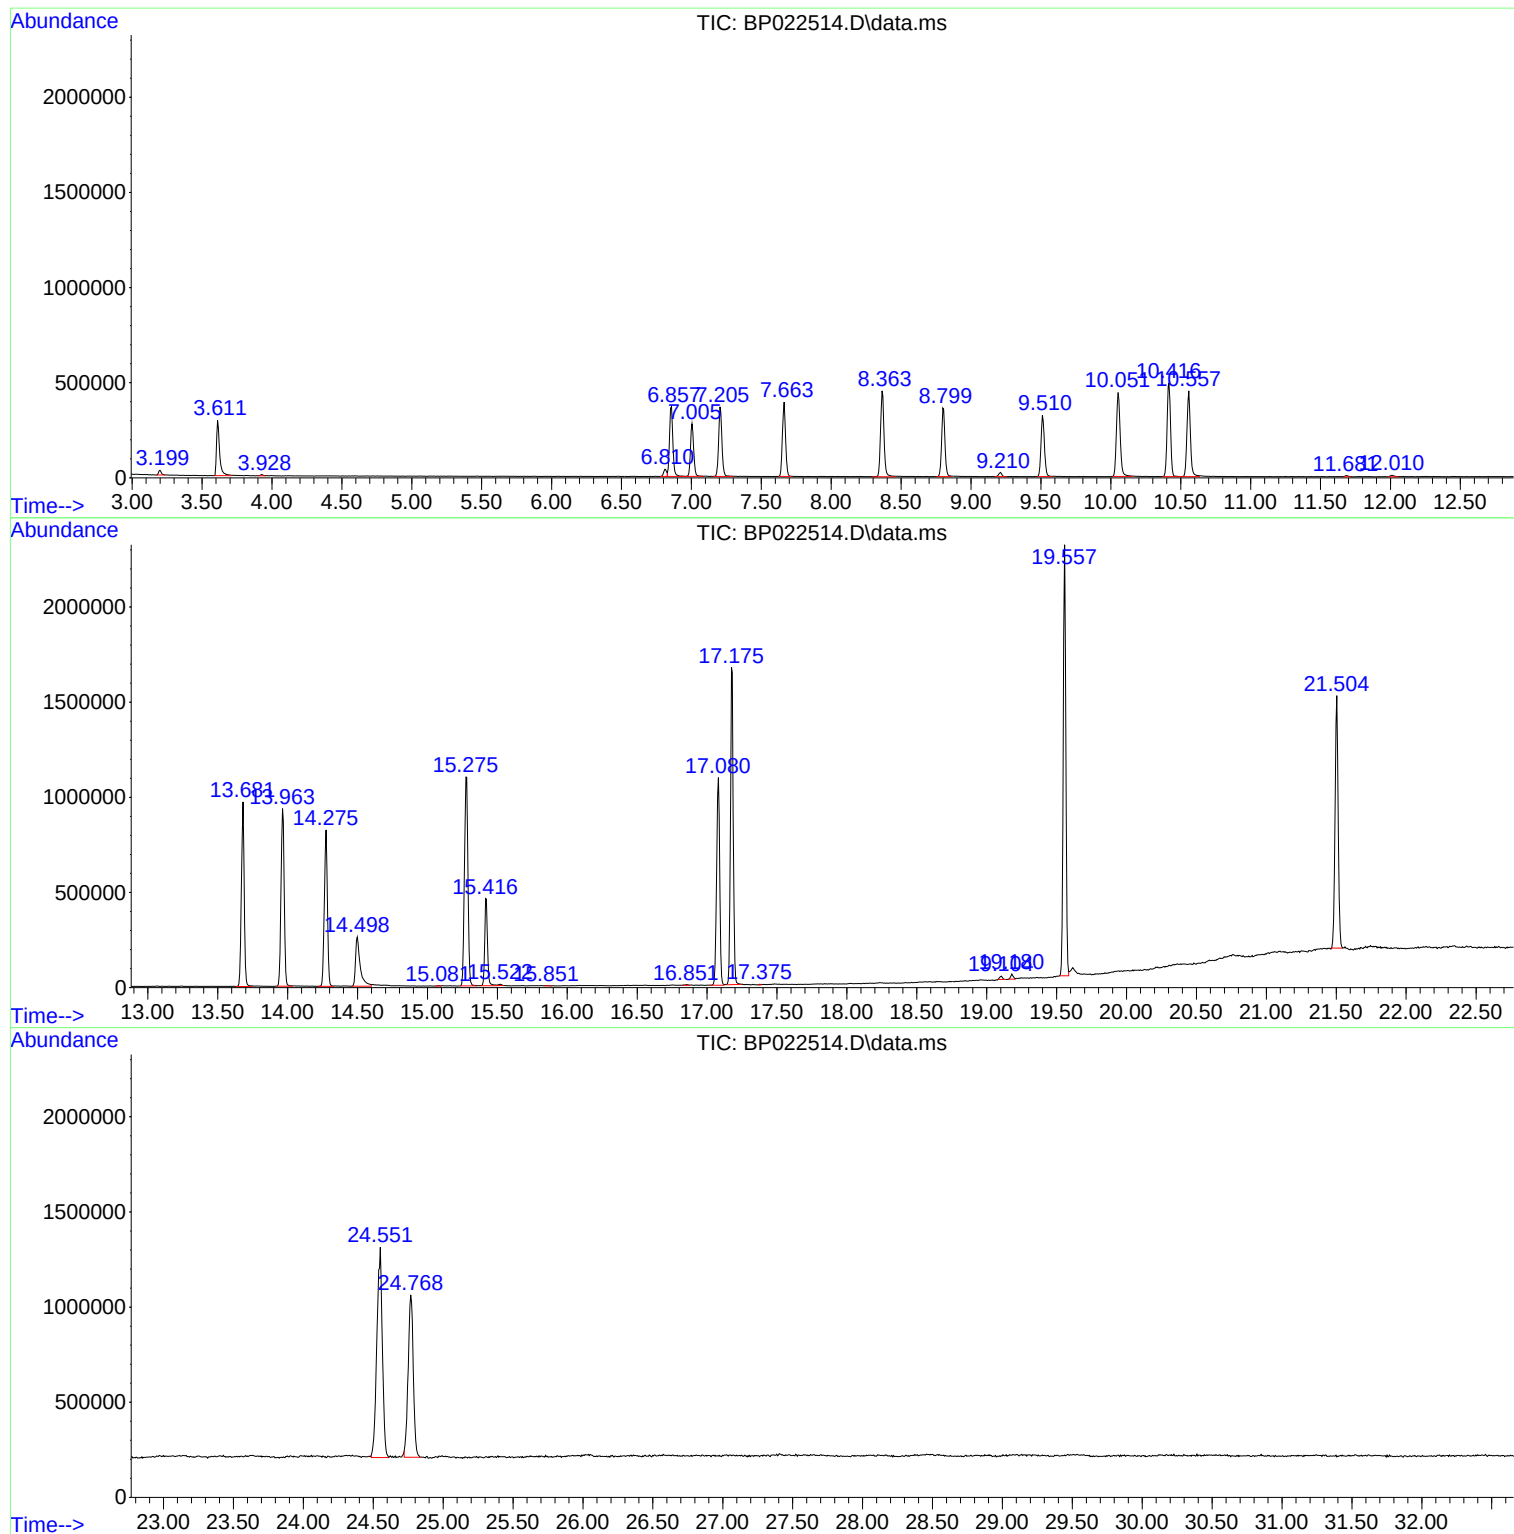

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022514.D
Acq On : 21 Oct 2024 20:52
Operator : RC/JU
Sample : PB164300BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022514.D
Acq On : 21 Oct 2024 20:52
Operator : RC/JU
Sample : PB164300BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc