

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022540.D
 Acq On : 22 Oct 2024 17:06
 Operator : RC/JU
 Sample : PB164219BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	30	35	41	rVB	28829	39496	1.04%	0.109%
2	3.605	101	105	128	rVB	357316	531395	13.95%	1.470%
3	3.916	156	158	163	rVB2	5929	7789	0.20%	0.022%
4	4.358	229	233	238	rBV	12384	16077	0.42%	0.044%
5	6.810	643	650	653	rBV	342938	489911	12.86%	1.355%
6	6.852	653	657	673	rVV	462479	735899	19.32%	2.036%
7	7.005	675	683	696	rVB	362186	542139	14.23%	1.500%
8	7.205	710	717	727	rBV	463066	726837	19.08%	2.011%
9	7.657	786	794	808	rBV	439080	693360	18.20%	1.918%
10	8.357	906	913	930	rBV	519274	943234	24.76%	2.610%
11	8.799	980	988	1002	rBV	456054	759360	19.94%	2.101%
12	9.204	1051	1057	1065	rBV	140931	229754	6.03%	0.636%
13	9.510	1101	1109	1121	rBV	426985	678236	17.81%	1.877%
14	10.051	1193	1201	1214	rBV	588301	1033934	27.14%	2.861%
15	10.416	1255	1263	1272	rBV	566997	969409	25.45%	2.682%
16	10.551	1276	1286	1300	rBV	530326	970993	25.49%	2.687%
17	11.687	1473	1479	1489	rVB	26843	42594	1.12%	0.118%
18	12.010	1528	1534	1542	rBV2	8228	16998	0.45%	0.047%
19	13.687	1811	1819	1829	rBV	1179795	1711376	44.93%	4.735%
20	13.969	1858	1867	1879	rBV	1186091	1881853	49.40%	5.207%
21	14.275	1909	1919	1929	rBV	940756	1530036	40.17%	4.233%
22	14.504	1951	1958	1971	rBV	416509	787747	20.68%	2.180%
23	15.281	2083	2090	2101	rBV	1611556	2488511	65.33%	6.885%
24	15.428	2108	2115	2127	rBV	479958	720477	18.91%	1.993%
25	15.528	2127	2132	2141	rVB4	10816	20408	0.54%	0.056%
26	16.098	2223	2229	2232	rBV8	2731	4732	0.12%	0.013%
27	16.557	2303	2307	2311	rBV6	3068	4995	0.13%	0.014%
28	16.757	2336	2341	2343	rBV6	2972	4973	0.13%	0.014%
29	16.863	2356	2359	2365	rVB2	5094	5989	0.16%	0.017%
30	17.086	2389	2397	2405	rBV	1292737	2115112	55.53%	5.852%
31	17.186	2407	2414	2426	rVV	2130723	2910628	76.41%	8.053%
32	17.386	2443	2448	2449	rBV5	4458	6715	0.18%	0.019%
33	19.098	2735	2739	2746	rVB2	26078	43019	1.13%	0.119%
34	19.180	2748	2753	2758	rVV	26387	38693	1.02%	0.107%
35	19.557	2811	2817	2824	rBV	2389631	3597913	94.45%	9.955%
36	21.516	3144	3150	3158	rVB2	1669558	2480126	65.11%	6.862%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022540.D
Acq On : 22 Oct 2024 17:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.545	3656	3665	3681	rVB	1497251	3809174	100.00%	10.539%
38	24.780	3696	3705	3715	rVB	1025443	2552723	67.02%	7.063%




Sum of corrected areas: 36142615

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022540.D
Acq On : 22 Oct 2024 17:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

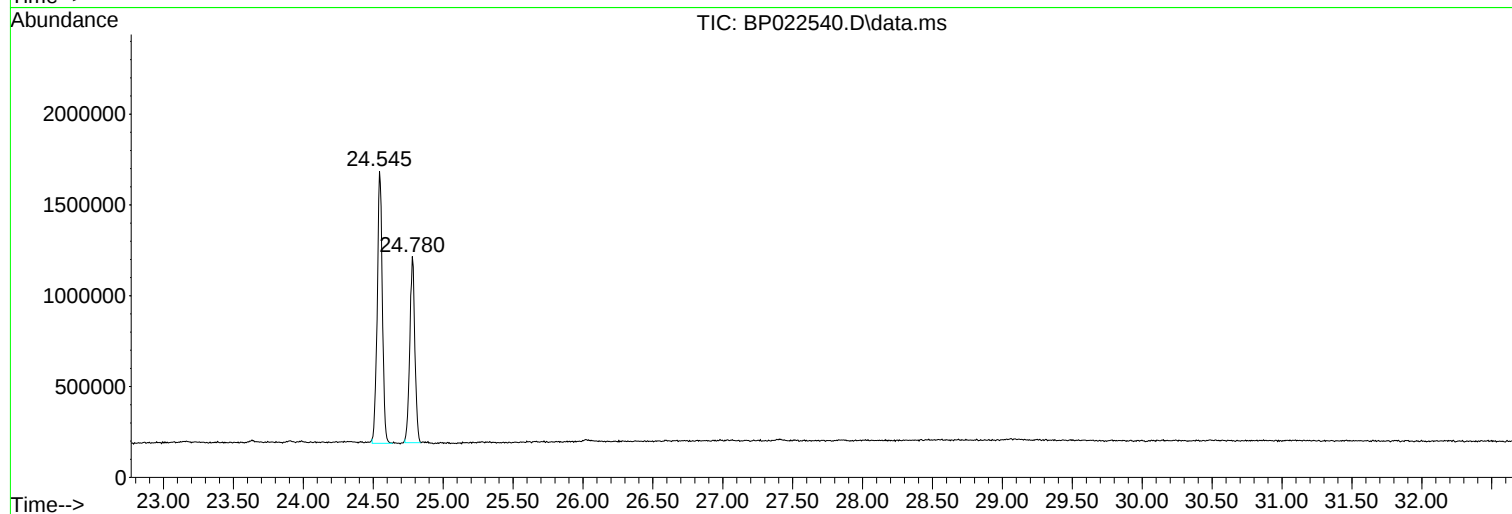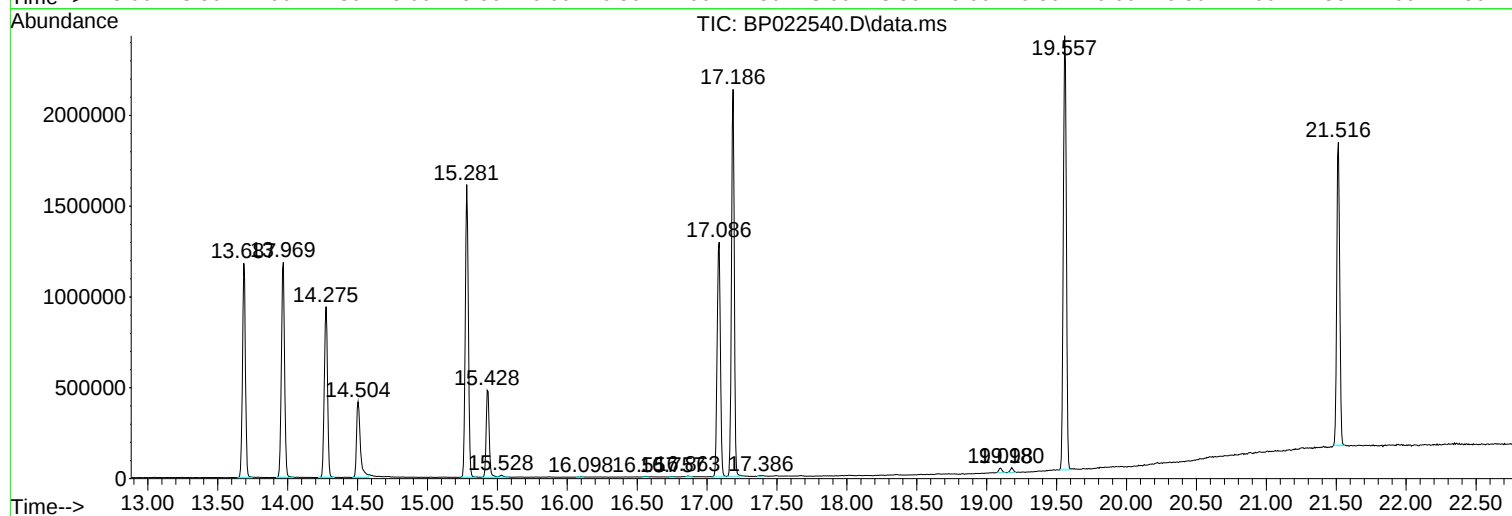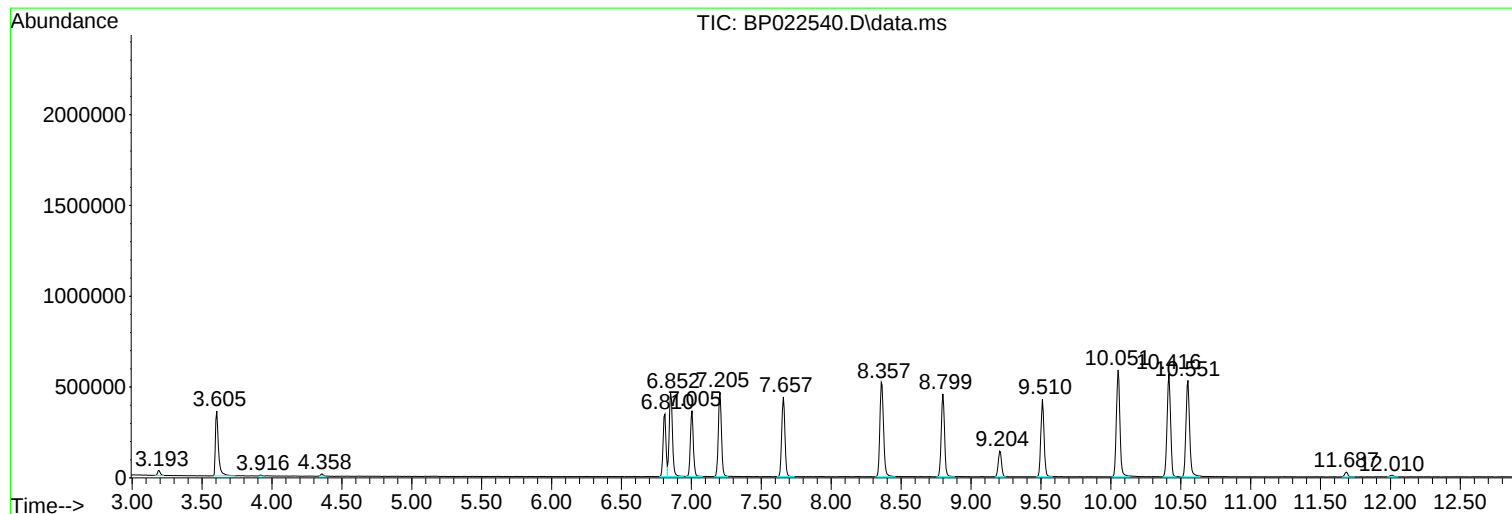

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022540.D
Acq On : 22 Oct 2024 17:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022540.D
Acq On : 22 Oct 2024 17:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------