

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022556.D
 Acq On : 23 Oct 2024 10:06
 Operator : RC/JU
 Sample : PB164219BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	39	rVB	31415	42110	1.38%	0.136%
2	3.563	94	98	117	rBV	319050	509185	16.68%	1.646%
3	3.869	147	150	154	rBV2	6575	8809	0.29%	0.028%
4	6.728	632	636	639	rBV2	3560	5264	0.17%	0.017%
5	6.781	639	645	658	rVB	404843	669997	21.95%	2.166%
6	6.940	663	672	681	rVV	318207	483254	15.83%	1.563%
7	7.134	697	705	715	rBV	416354	665000	21.78%	2.150%
8	7.593	776	783	792	rBV	440866	700825	22.96%	2.266%
9	8.298	893	903	915	rBV	479757	838276	27.46%	2.711%
10	8.734	970	977	989	rBV	367849	659177	21.59%	2.131%
11	9.140	1040	1046	1054	rBV6	5489	10752	0.35%	0.035%
12	9.451	1088	1099	1111	rBV	308687	573257	18.78%	1.854%
13	9.987	1183	1190	1201	rBV	549796	886333	29.03%	2.866%
14	10.363	1244	1254	1265	rBV	563923	945557	30.97%	3.058%
15	10.504	1268	1278	1294	rBV	393857	839094	27.48%	2.713%
16	11.651	1467	1473	1476	rBV6	3835	6977	0.23%	0.023%
17	11.957	1520	1525	1530	rBV3	10538	17031	0.56%	0.055%
18	13.651	1804	1813	1824	rBV	964320	1387992	45.46%	4.488%
19	13.922	1853	1859	1871	rBV2	994971	1594985	52.24%	5.157%
20	14.233	1903	1912	1920	rBV	971156	1471420	48.20%	4.758%
21	14.475	1946	1953	1972	rBV	304080	698107	22.87%	2.257%
22	15.251	2079	2085	2094	rVB	1501040	2129369	69.75%	6.885%
23	15.404	2104	2111	2121	rBV	371830	524998	17.20%	1.698%
24	15.504	2125	2128	2134	rVB6	8952	13316	0.44%	0.043%
25	16.533	2296	2303	2309	rVB6	6122	13164	0.43%	0.043%
26	16.722	2328	2335	2338	rBV8	3198	6751	0.22%	0.022%
27	16.816	2347	2351	2352	rBV4	4681	5316	0.17%	0.017%
28	17.057	2385	2392	2400	rVB	1277435	1976585	64.74%	6.391%
29	17.157	2402	2409	2419	rBV2	1603124	2452118	80.32%	7.929%
30	17.351	2437	2442	2448	rBV9	5467	11755	0.39%	0.038%
31	17.986	2546	2550	2555	rBV7	6168	12857	0.42%	0.042%
32	18.551	2644	2646	2651	rVB6	6187	7820	0.26%	0.025%
33	19.086	2734	2737	2741	rBV	25415	29917	0.98%	0.097%
34	19.163	2746	2750	2753	rBV	25032	39286	1.29%	0.127%
35	19.545	2809	2815	2821	rBV	2225738	3052985	100.00%	9.872%
36	19.604	2821	2825	2834	rVB3	31304	67241	2.20%	0.217%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022556.D
Acq On : 23 Oct 2024 10:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	21.504	3142	3148	3155	rVB2	1263697	2264862	74.19%	7.324%
38	24.539	3655	3664	3678	rVB	1195896	2982760	97.70%	9.645%
39	24.762	3694	3702	3717	rVB	752272	2321268	76.03%	7.506%




Sum of corrected areas: 30925770

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022556.D
Acq On : 23 Oct 2024 10:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

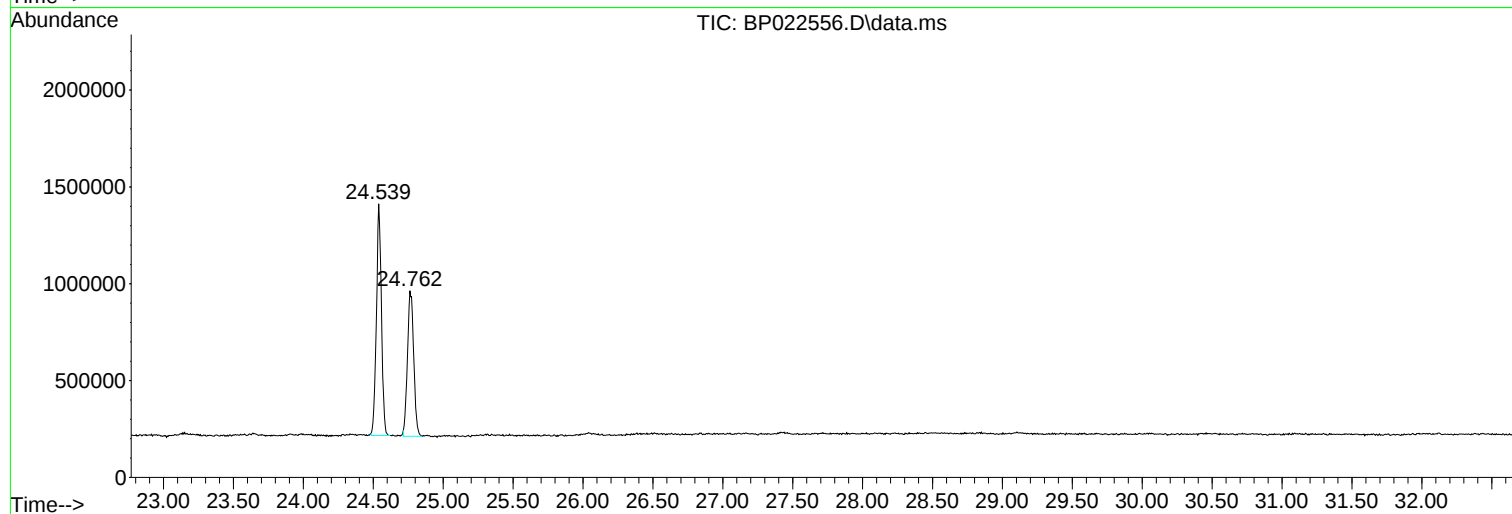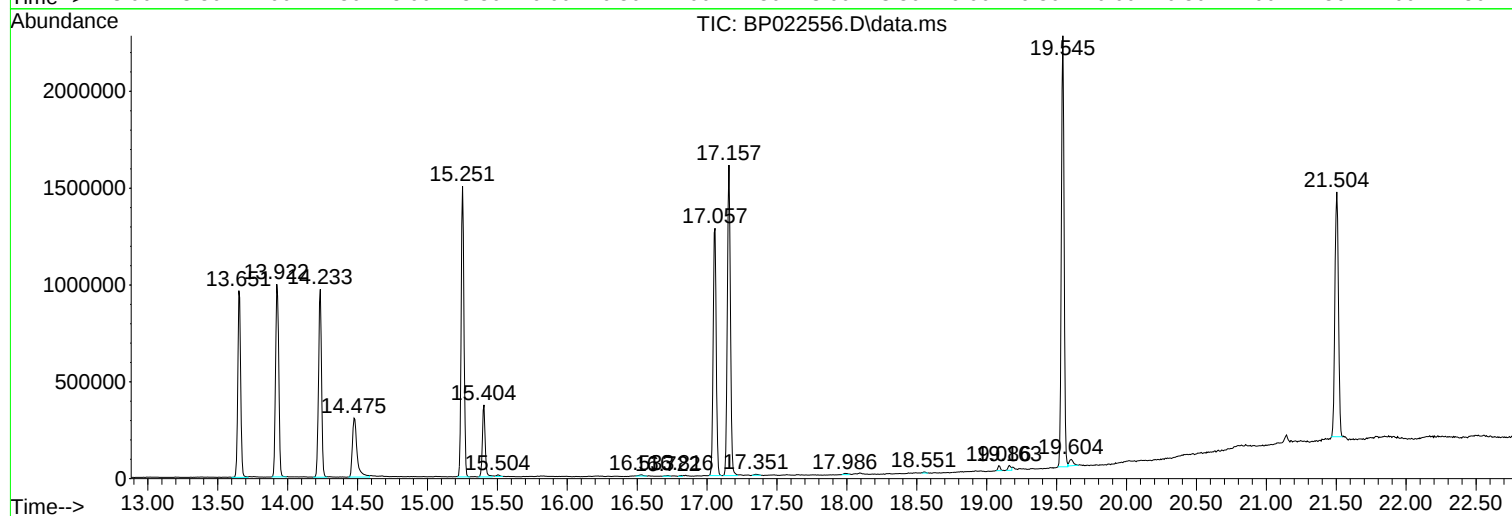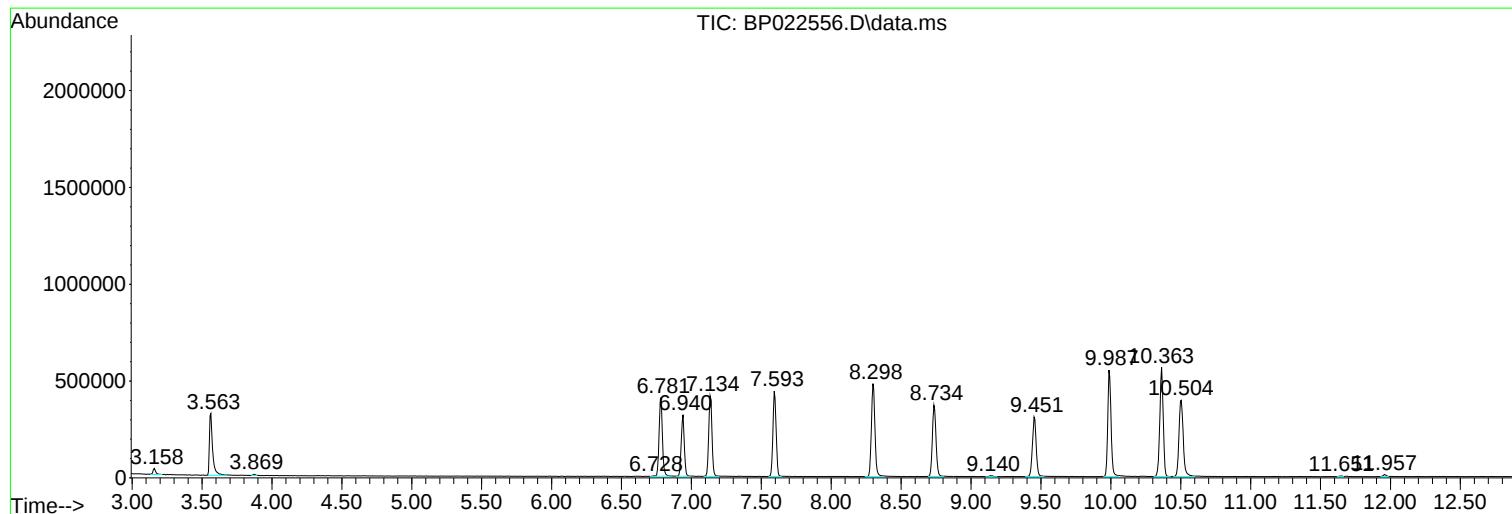

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022556.D
Acq On : 23 Oct 2024 10:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022556.D
Acq On : 23 Oct 2024 10:06
Operator : RC/JU
Sample : PB164219BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------