

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022560.D
 Acq On : 23 Oct 2024 12:48
 Operator : RC/JU
 Sample : P4361-14RX
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ5RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	34	37	45	rVB2	8181	11105	0.47%	0.068%
2	3.628	106	109	116	rBV2	14292	24787	1.06%	0.151%
3	3.928	156	160	165	rBV3	7352	10742	0.46%	0.065%
4	4.299	219	223	228	rVB8	2817	3543	0.15%	0.022%
5	4.716	287	294	295	rBV6	2433	3707	0.16%	0.023%
6	4.828	308	313	318	rBV2	5046	8746	0.37%	0.053%
7	5.698	455	461	470	rBV10	2113	5359	0.23%	0.033%
8	6.810	645	650	652	rBV2	11784	16632	0.71%	0.101%
9	6.851	652	657	670	rVB	93460	187493	8.01%	1.143%
10	7.004	677	683	694	rVB	78917	130607	5.58%	0.796%
11	7.204	710	717	727	rBV	107514	178598	7.63%	1.088%
12	7.481	759	764	770	rVB6	1931	3556	0.15%	0.022%
13	7.657	785	794	804	rBV	411036	642126	27.44%	3.913%
14	7.728	804	806	811	rVB6	2531	4233	0.18%	0.026%
15	7.869	827	830	837	rBV7	3887	7030	0.30%	0.043%
16	8.187	880	884	890	rBV9	2897	5775	0.25%	0.035%
17	8.363	907	914	926	rBV2	114993	215908	9.23%	1.316%
18	8.475	927	933	945	rVB	57181	93974	4.02%	0.573%
19	8.634	955	960	963	rBV7	1525	2599	0.11%	0.016%
20	8.798	982	988	997	rBV	97008	171214	7.32%	1.043%
21	9.204	1049	1057	1063	rVB	24734	41130	1.76%	0.251%
22	9.357	1077	1083	1088	rBV5	8019	15757	0.67%	0.096%
23	9.510	1101	1109	1122	rBV	83954	149474	6.39%	0.911%
24	9.704	1134	1142	1145	rBV8	4112	8481	0.36%	0.052%
25	9.863	1165	1169	1176	rVB5	5651	9387	0.40%	0.057%
26	10.051	1194	1201	1214	rBV	123712	233165	9.96%	1.421%
27	10.410	1249	1262	1276	rBV	495303	876561	37.46%	5.341%
28	10.557	1279	1287	1304	rVV	85347	187849	8.03%	1.145%
29	10.892	1338	1344	1348	rBV8	2162	3548	0.15%	0.022%
30	10.969	1351	1357	1364	rBV8	4194	11254	0.48%	0.069%
31	11.086	1376	1377	1381	rVB4	2452	2738	0.12%	0.017%
32	11.222	1395	1400	1409	rBV4	4106	10855	0.46%	0.066%
33	11.422	1429	1434	1437	rBV5	3956	7151	0.31%	0.044%
34	11.592	1458	1463	1466	rBV7	1682	2590	0.11%	0.016%
35	11.675	1472	1477	1483	rBV3	8460	14429	0.62%	0.088%
36	11.822	1500	1502	1509	rVB8	4343	6202	0.27%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022560.D
 Acq On : 23 Oct 2024 12:48
 Operator : RC/JU
 Sample : P4361-14RX
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ5RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	11.998	1528	1532	1537	rVV6	1756	3253	0.14%	0.020%
38	12.069	1538	1544	1552	rVB2	6822	12425	0.53%	0.076%
39	12.286	1575	1581	1589	rVB5	6522	13173	0.56%	0.080%
40	12.416	1596	1603	1606	rBV9	1206	2820	0.12%	0.017%
41	12.463	1606	1611	1615	rVV8	2426	4066	0.17%	0.025%
42	12.692	1645	1650	1653	rBV7	1892	3097	0.13%	0.019%
43	12.792	1663	1667	1672	rVB3	7231	9818	0.42%	0.060%
44	13.063	1708	1713	1714	rBV5	2752	3560	0.15%	0.022%
45	13.086	1714	1717	1723	rVV7	5163	9016	0.39%	0.055%
46	13.157	1726	1729	1735	rVV8	1867	3299	0.14%	0.020%
47	13.280	1746	1750	1753	rBV5	2797	4014	0.17%	0.024%
48	13.439	1769	1777	1780	rBV8	4854	11313	0.48%	0.069%
49	13.575	1796	1800	1804	rBV6	9119	15398	0.66%	0.094%
50	13.669	1807	1816	1826	rVV	241240	394569	16.86%	2.404%
51	13.751	1826	1830	1834	rVB3	8806	11962	0.51%	0.073%
52	13.792	1834	1837	1839	rBV4	2688	3558	0.15%	0.022%
53	13.951	1858	1864	1874	rBV	285576	450554	19.25%	2.745%
54	14.104	1885	1890	1896	rBV9	3946	9347	0.40%	0.057%
55	14.169	1896	1901	1905	rVV8	4834	9039	0.39%	0.055%
56	14.263	1907	1917	1923	rVV	907430	1284877	54.90%	7.830%
57	14.322	1923	1927	1936	rVB2	16699	28159	1.20%	0.172%
58	14.516	1949	1960	1980	rBV3	45227	140695	6.01%	0.857%
59	14.674	1982	1987	1988	rBV2	7344	10797	0.46%	0.066%
60	14.804	2005	2009	2014	rBV7	4287	7628	0.33%	0.046%
61	14.898	2022	2025	2029	rVV6	2977	3873	0.17%	0.024%
62	15.063	2050	2053	2060	rBV9	2658	6876	0.29%	0.042%
63	15.274	2080	2089	2094	rBV	441913	594292	25.39%	3.621%
64	15.327	2094	2098	2104	rVB	19760	28837	1.23%	0.176%
65	15.421	2108	2114	2124	rVB	51312	89850	3.84%	0.548%
66	15.545	2124	2135	2140	rBV7	15231	37066	1.58%	0.226%
67	15.639	2147	2151	2159	rVB	51107	82840	3.54%	0.505%
68	15.751	2168	2170	2172	rBV3	2630	2859	0.12%	0.017%
69	15.774	2172	2174	2176	rVV3	3383	2733	0.12%	0.017%
70	15.863	2184	2189	2191	rBV6	3671	7155	0.31%	0.044%
71	16.039	2210	2219	2227	rVB5	16811	42462	1.81%	0.259%
72	16.398	2277	2280	2285	rVB7	5527	7541	0.32%	0.046%
73	16.598	2311	2314	2315	rBV3	5132	4331	0.19%	0.026%
74	16.716	2330	2334	2341	rVB8	9526	16446	0.70%	0.100%
75	16.880	2358	2362	2368	rBV	20084	28326	1.21%	0.173%
76	17.057	2386	2392	2397	rBV	1061876	1655790	70.75%	10.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022560.D
 Acq On : 23 Oct 2024 12:48
 Operator : RC/JU
 Sample : P4361-14RX
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EOAZ5RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

77	17.104	2397	2400	2404	rVB	189851	240582	10.28%	1.466%
78	17.163	2404	2410	2415	rBV	435232	651864	27.85%	3.972%
79	17.274	2426	2429	2434	rVB7	14668	19665	0.84%	0.120%
80	17.368	2443	2445	2452	rVB4	20145	29548	1.26%	0.180%
81	17.480	2460	2464	2472	rVB3	11983	23152	0.99%	0.141%
82	17.986	2543	2550	2553	rBV2	87368	146961	6.28%	0.896%
83	18.021	2553	2556	2560	rVB	42361	64160	2.74%	0.391%
84	18.098	2566	2569	2574	rVB2	18963	24081	1.03%	0.147%
85	18.163	2575	2580	2584	rVV3	50209	92611	3.96%	0.564%
86	18.198	2584	2586	2595	rVB2	22476	32433	1.39%	0.198%
87	18.480	2631	2634	2638	rVB	25463	32031	1.37%	0.195%
88	18.751	2677	2680	2684	rVB6	13802	17450	0.75%	0.106%
89	18.915	2704	2708	2713	rVB2	23993	36785	1.57%	0.224%
90	19.192	2750	2755	2760	rVV	358101	478904	20.46%	2.918%
91	19.251	2762	2765	2769	rVB6	25391	32526	1.39%	0.198%
92	19.321	2775	2777	2780	rBV3	16830	16471	0.70%	0.100%
93	19.539	2809	2814	2818	rBV	538189	864917	36.96%	5.270%
94	20.092	2906	2908	2913	rVB	55923	74252	3.17%	0.452%
95	20.204	2923	2927	2931	rBV	60642	86951	3.72%	0.530%
96	21.409	3129	3132	3136	rVB	70898	80919	3.46%	0.493%
97	21.492	3139	3146	3151	rVV	1300148	2340257	100.00%	14.261%
98	21.539	3152	3154	3165	rVB	173270	263305	11.25%	1.604%
99	24.527	3658	3662	3668	rVB	188476	365245	15.61%	2.226%
100	24.745	3692	3699	3714	rVB	831335	2029577	86.72%	12.367%




Sum of corrected areas: 16410666

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022560.D
Acq On : 23 Oct 2024 12:48
Operator : RC/JU
Sample : P4361-14RX
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ5RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

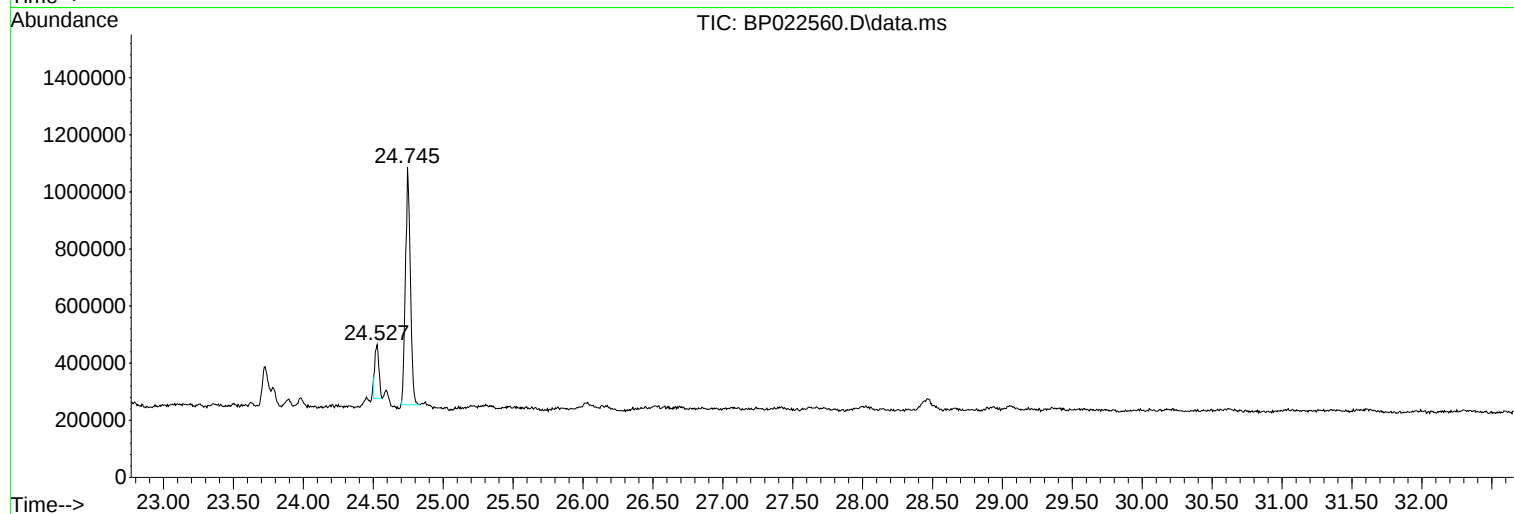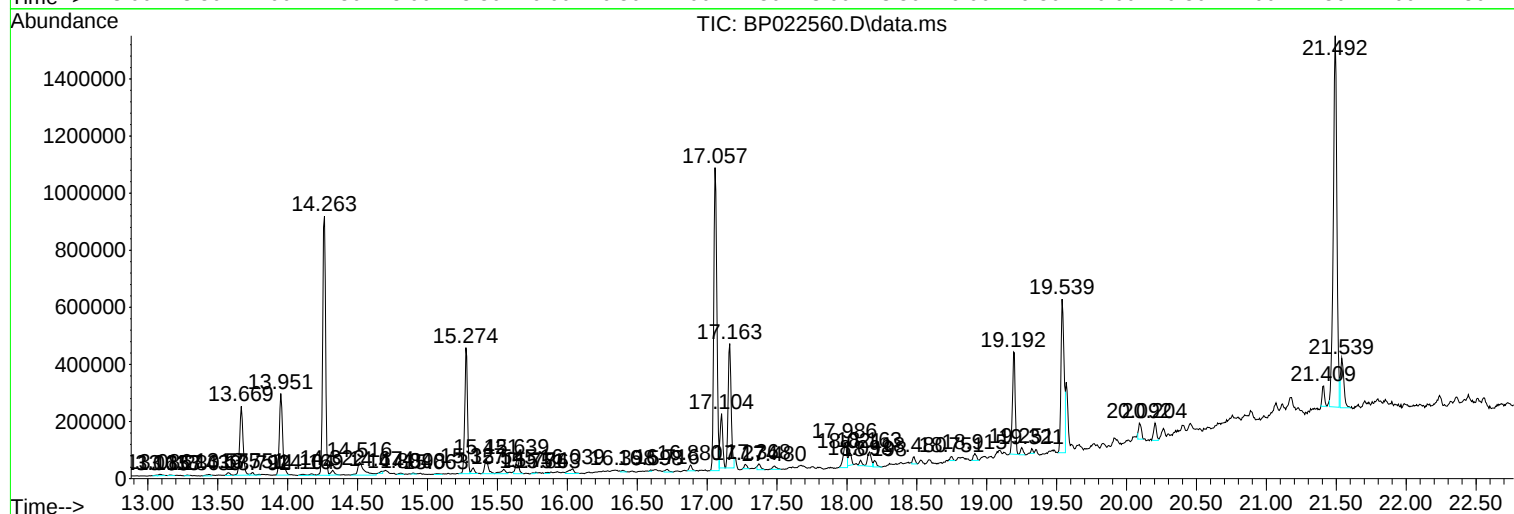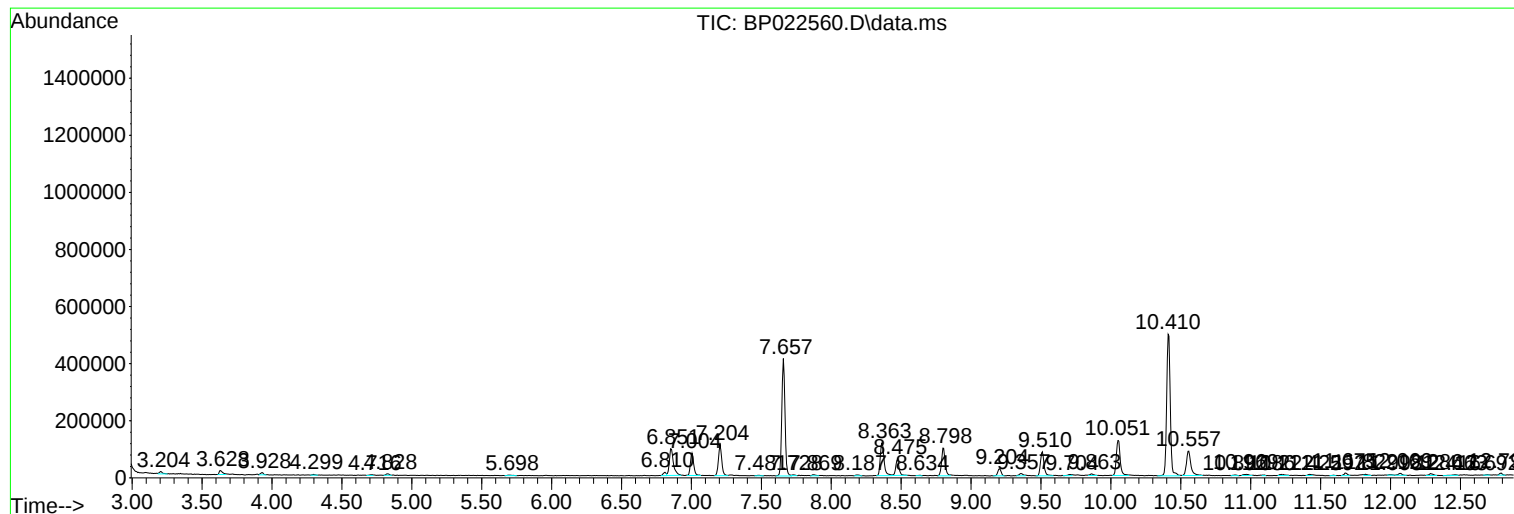

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022560.D
Acq On : 23 Oct 2024 12:48
Operator : RC/JU
Sample : P4361-14RX
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ5RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022560.D
Acq On : 23 Oct 2024 12:48
Operator : RC/JU
Sample : P4361-14RX
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOAZ5RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------