

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022563.D
 Acq On : 23 Oct 2024 14:50
 Operator : RC/JU
 Sample : P4415-16
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	40	rBV	5975	8646	0.38%	0.056%
2	3.628	105	109	115	rBV	10938	16696	0.74%	0.108%
3	3.928	157	160	164	rVB3	5884	8514	0.38%	0.055%
4	4.711	289	293	297	rBV7	2273	3274	0.14%	0.021%
5	4.828	308	313	319	rVB	5039	7755	0.34%	0.050%
6	5.693	458	460	466	rVB5	1599	2333	0.10%	0.015%
7	6.034	515	518	523	rBV7	1407	2803	0.12%	0.018%
8	6.858	646	658	671	rBV	89995	188629	8.33%	1.217%
9	6.999	677	682	689	rBV	66831	107208	4.73%	0.692%
10	7.205	709	717	727	rBV	97388	156332	6.90%	1.008%
11	7.281	727	730	734	rVB6	1929	2375	0.10%	0.015%
12	7.481	761	764	770	rVB7	1652	3544	0.16%	0.023%
13	7.658	787	794	803	rBV	369566	594291	26.25%	3.833%
14	7.734	805	807	812	rVB6	2556	3633	0.16%	0.023%
15	8.363	905	914	927	rBV	109312	211428	9.34%	1.364%
16	8.469	927	932	942	rVB2	49120	83691	3.70%	0.540%
17	8.799	982	988	998	rBV	85777	144286	6.37%	0.931%
18	8.958	1011	1015	1020	rVB7	1617	2784	0.12%	0.018%
19	9.210	1053	1058	1062	rBV3	8042	12675	0.56%	0.082%
20	9.363	1075	1084	1092	rBV5	8420	17424	0.77%	0.112%
21	9.510	1103	1109	1123	rBV	67326	129059	5.70%	0.832%
22	9.710	1138	1143	1146	rBV5	4686	8899	0.39%	0.057%
23	9.869	1165	1170	1176	rBV4	5042	8139	0.36%	0.052%
24	10.052	1194	1201	1215	rVV	110951	221673	9.79%	1.430%
25	10.410	1255	1262	1270	rBV	509808	849905	37.53%	5.482%
26	10.557	1281	1287	1303	rBV2	79989	166888	7.37%	1.076%
27	10.963	1349	1356	1357	rBV7	5182	7240	0.32%	0.047%
28	11.222	1394	1400	1407	rBV8	3135	7905	0.35%	0.051%
29	11.675	1470	1477	1482	rBV6	5353	8616	0.38%	0.056%
30	11.810	1493	1500	1503	rBV9	1889	5027	0.22%	0.032%
31	11.999	1530	1532	1537	rVB5	2307	2513	0.11%	0.016%
32	12.857	1674	1678	1685	rBV8	1763	3800	0.17%	0.025%
33	13.081	1713	1716	1720	rVB5	2625	3014	0.13%	0.019%
34	13.675	1810	1817	1828	rBV	264596	386358	17.06%	2.492%
35	13.957	1858	1865	1876	rBV	292153	417729	18.45%	2.694%
36	14.175	1899	1902	1908	rVB8	1511	2538	0.11%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022563.D
 Acq On : 23 Oct 2024 14:50
 Operator : RC/JU
 Sample : P4415-16
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	14.275	1910	1919	1926	rBV	878371	1359873	60.06%	8.771%
38	14.334	1927	1929	1935	rVB7	3386	4947	0.22%	0.032%
39	14.528	1957	1962	1976	rBV	48213	128140	5.66%	0.827%
40	14.704	1987	1992	2002	rVB6	13765	28127	1.24%	0.181%
41	15.081	2052	2056	2065	rVB9	1999	4013	0.18%	0.026%
42	15.287	2083	2091	2099	rBV	383493	600204	26.51%	3.871%
43	15.416	2107	2113	2122	rBV	48197	75863	3.35%	0.489%
44	15.663	2147	2155	2161	rBV	58365	83339	3.68%	0.538%
45	16.040	2216	2219	2222	rVB5	2498	3006	0.13%	0.019%
46	16.351	2269	2272	2275	rBV5	2521	4285	0.19%	0.028%
47	16.840	2352	2355	2359	rVV4	2713	4689	0.21%	0.030%
48	17.075	2388	2395	2400	rBV	1401116	1887298	83.35%	12.173%
49	17.116	2400	2402	2406	rVV	48871	57506	2.54%	0.371%
50	17.169	2406	2411	2423	rVB	530874	735624	32.49%	4.745%
51	17.292	2429	2432	2437	rVB7	6787	9005	0.40%	0.058%
52	17.381	2444	2447	2449	rBV4	4413	5621	0.25%	0.036%
53	17.451	2457	2459	2462	rBV4	3520	3871	0.17%	0.025%
54	17.775	2511	2514	2516	rBV3	4382	4701	0.21%	0.030%
55	17.975	2546	2548	2550	rBV3	4161	3709	0.16%	0.024%
56	18.016	2550	2555	2564	rVV2	96099	144847	6.40%	0.934%
57	18.181	2579	2583	2587	rBV4	17521	30550	1.35%	0.197%
58	18.881	2700	2702	2705	rVB4	9472	8392	0.37%	0.054%
59	19.216	2754	2759	2764	rVB	141273	177155	7.82%	1.143%
60	19.345	2778	2781	2792	rBV7	36640	60293	2.66%	0.389%
61	19.563	2812	2818	2822	rBV	594193	861125	38.03%	5.554%
62	21.186	3091	3094	3102	rVB4	65695	114236	5.05%	0.737%
63	21.328	3115	3118	3126	rVB2	65492	89420	3.95%	0.577%
64	21.510	3142	3149	3154	rBV2	1408452	2202463	97.27%	14.206%
65	23.904	3553	3556	3566	rVB3	98353	220434	9.74%	1.422%
66	24.551	3660	3666	3673	rVB	225455	518805	22.91%	3.346%
67	24.774	3695	3704	3715	rVB	854317	2264316	100.00%	14.605%




Sum of corrected areas: 15503481

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022563.D
Acq On : 23 Oct 2024 14:50
Operator : RC/JU
Sample : P4415-16
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4F97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

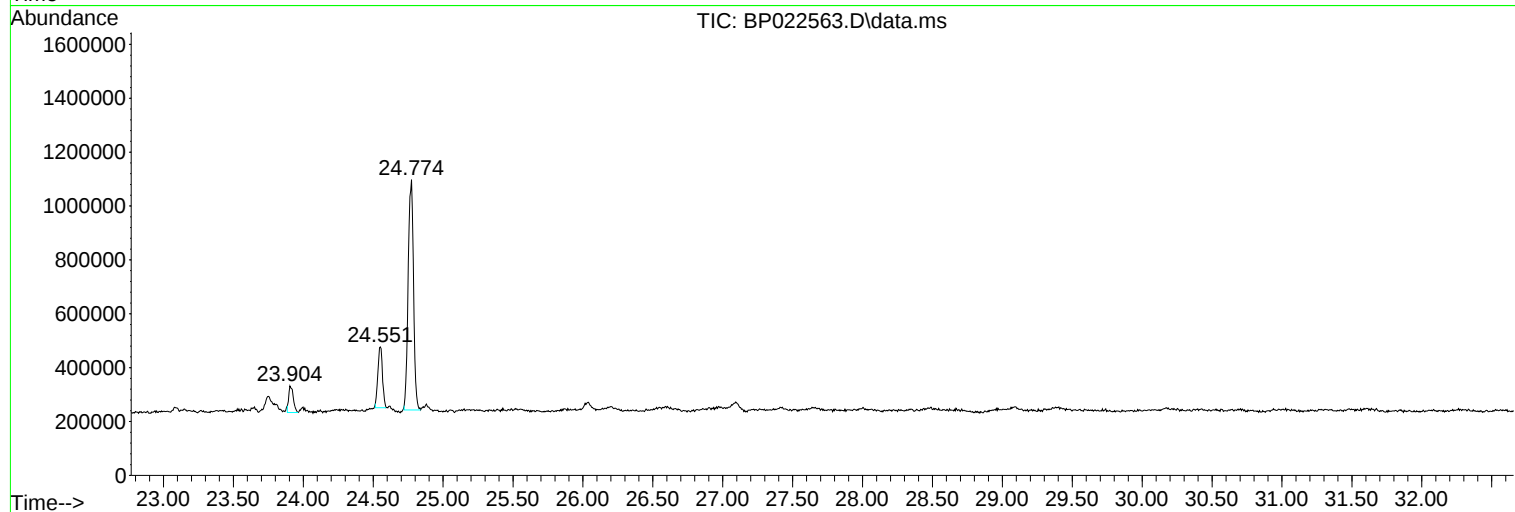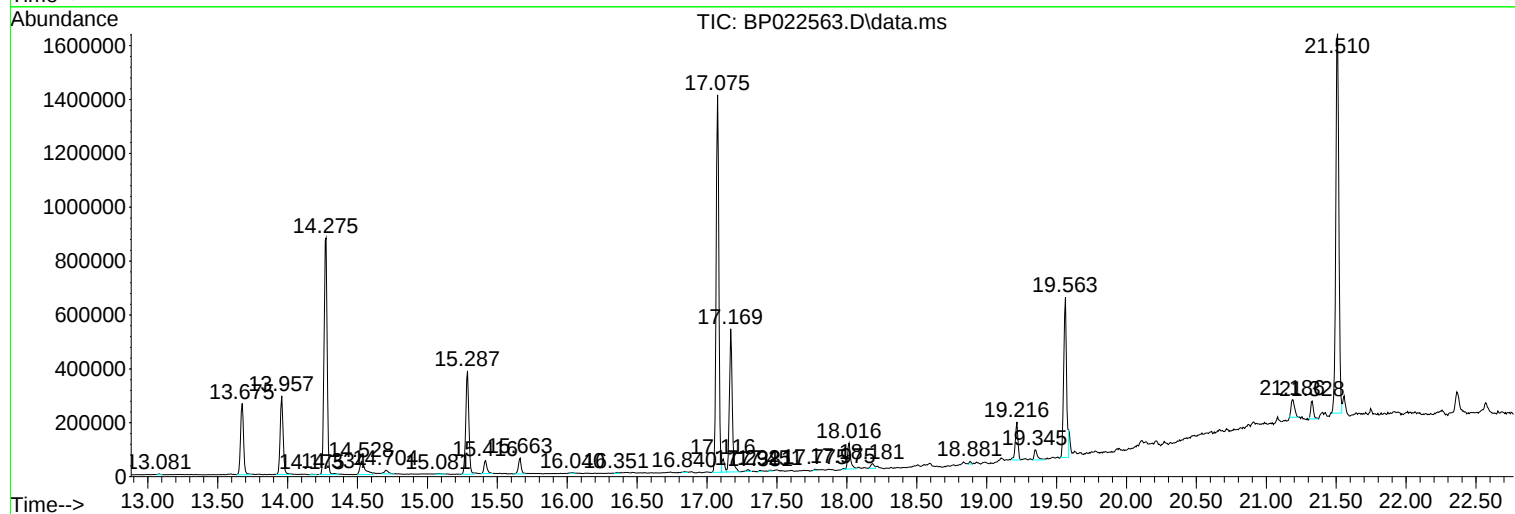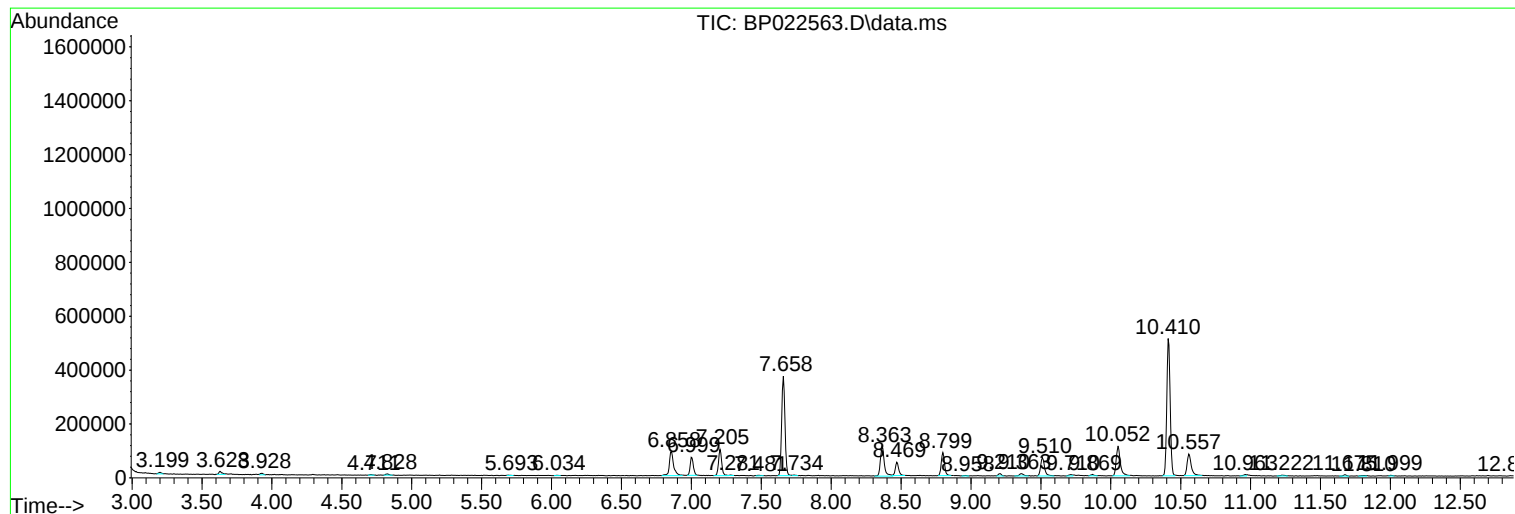

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022563.D
Acq On : 23 Oct 2024 14:50
Operator : RC/JU
Sample : P4415-16
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4F97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022563.D
Acq On : 23 Oct 2024 14:50
Operator : RC/JU
Sample : P4415-16
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4F97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc