

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022573.D
 Acq On : 23 Oct 2024 21:37
 Operator : RC/JU
 Sample : P4415-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	40	rVB	5619	7474	0.24%	0.032%
2	3.628	103	109	116	rBV3	9727	18214	0.59%	0.078%
3	3.710	119	123	128	rVB	9658	12671	0.41%	0.055%
4	3.922	156	159	164	rVB3	7038	9207	0.30%	0.040%
5	4.293	220	222	227	rVB6	4224	4431	0.14%	0.019%
6	4.822	308	312	321	rVB	6837	13236	0.43%	0.057%
7	4.934	326	331	338	rVB	2482	6556	0.21%	0.028%
8	6.810	644	650	651	rBV3	5866	8482	0.28%	0.036%
9	6.851	651	657	672	rVV	91763	189797	6.19%	0.816%
10	6.998	676	682	692	rVB	74461	123022	4.01%	0.529%
11	7.204	709	717	728	rBV	98032	171705	5.60%	0.739%
12	7.657	785	794	804	rBV	462484	754726	24.61%	3.247%
13	8.363	906	914	923	rBV	101590	184022	6.00%	0.792%
14	8.469	926	932	946	rVB	62869	104323	3.40%	0.449%
15	8.798	981	988	997	rBV	96272	165565	5.40%	0.712%
16	8.963	1011	1016	1020	rVB8	1951	3408	0.11%	0.015%
17	9.198	1050	1056	1062	rBV2	9439	16662	0.54%	0.072%
18	9.369	1078	1085	1093	rBV2	2634	6477	0.21%	0.028%
19	9.510	1100	1109	1121	rBV2	72098	144259	4.70%	0.621%
20	9.704	1134	1142	1148	rBV5	8972	24266	0.79%	0.104%
21	9.863	1164	1169	1174	rVB4	5113	9561	0.31%	0.041%
22	10.051	1193	1201	1218	rBV	115051	232148	7.57%	0.999%
23	10.410	1254	1262	1275	rBV	645052	1061592	34.62%	4.567%
24	10.557	1280	1287	1298	rBV	73497	149663	4.88%	0.644%
25	10.957	1347	1355	1362	rBV	3681	10590	0.35%	0.046%
26	11.222	1394	1400	1407	rBV8	6010	13436	0.44%	0.058%
27	11.675	1471	1477	1482	rBV4	6327	11370	0.37%	0.049%
28	11.998	1527	1532	1539	rVB8	2829	5224	0.17%	0.022%
29	12.069	1539	1544	1550	rBV4	3759	6263	0.20%	0.027%
30	12.286	1577	1581	1588	rVB7	3716	6281	0.20%	0.027%
31	13.086	1711	1717	1721	rBV9	2490	4806	0.16%	0.021%
32	13.416	1769	1773	1776	rBV6	2201	4111	0.13%	0.018%
33	13.580	1794	1801	1806	rBV7	7922	13194	0.43%	0.057%
34	13.675	1810	1817	1827	rVB	244950	380917	12.42%	1.639%
35	13.951	1857	1864	1876	rBV2	295142	445158	14.52%	1.915%
36	14.104	1883	1890	1895	rBV2	2715	5302	0.17%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022573.D
 Acq On : 23 Oct 2024 21:37
 Operator : RC/JU
 Sample : P4415-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	14.257	1907	1916	1923	rBV	1163434	1626733	53.04%	6.998%
38	14.322	1923	1927	1934	rVB	42525	74192	2.42%	0.319%
39	14.522	1950	1961	1978	rBV	45354	126156	4.11%	0.543%
40	14.663	1978	1985	1989	rBV	24631	45508	1.48%	0.196%
41	14.698	1989	1991	1998	rVB4	10777	19103	0.62%	0.082%
42	14.892	2020	2024	2027	rVV6	3748	6186	0.20%	0.027%
43	14.939	2028	2032	2038	rVB9	3921	7033	0.23%	0.030%
44	15.074	2050	2055	2059	rBV7	3431	6826	0.22%	0.029%
45	15.269	2079	2088	2093	rBV	419140	604255	19.70%	2.599%
46	15.322	2093	2097	2107	rVB	48590	82580	2.69%	0.355%
47	15.422	2107	2114	2119	rBV2	31193	64156	2.09%	0.276%
48	15.504	2124	2128	2131	rVV4	5783	8124	0.26%	0.035%
49	15.639	2145	2151	2159	rVB2	95569	145979	4.76%	0.628%
50	15.786	2168	2176	2184	rBV2	12141	29670	0.97%	0.128%
51	15.874	2184	2191	2196	rBV9	4505	10052	0.33%	0.043%
52	16.010	2208	2214	2221	rVB10	6920	15584	0.51%	0.067%
53	16.345	2261	2271	2277	rBV5	25369	47880	1.56%	0.206%
54	16.398	2277	2280	2285	rVB5	5927	8047	0.26%	0.035%
55	16.592	2310	2313	2316	rBV2	10100	13418	0.44%	0.058%
56	16.627	2317	2319	2322	rVB3	7514	8292	0.27%	0.036%
57	16.710	2329	2333	2342	rVB	21417	36712	1.20%	0.158%
58	16.786	2342	2346	2352	rBV6	10575	26672	0.87%	0.115%
59	16.886	2358	2363	2370	rVB	28763	46582	1.52%	0.200%
60	16.980	2377	2379	2382	rVB4	4126	4249	0.14%	0.018%
61	17.057	2386	2392	2396	rBV	1464097	2194295	71.55%	9.439%
62	17.104	2396	2400	2405	rVV	570591	901383	29.39%	3.878%
63	17.163	2405	2410	2415	rVV2	405082	696752	22.72%	2.997%
64	17.198	2415	2416	2423	rVB	106280	126259	4.12%	0.543%
65	17.268	2423	2428	2434	rBV10	17147	32939	1.07%	0.142%
66	17.357	2439	2443	2446	rBV6	3746	7122	0.23%	0.031%
67	17.480	2458	2464	2469	rVB	36884	61846	2.02%	0.266%
68	17.616	2484	2487	2490	rVB4	7570	8768	0.29%	0.038%
69	17.674	2494	2497	2504	rVB7	9133	18079	0.59%	0.078%
70	17.992	2543	2551	2554	rBV2	108101	212680	6.94%	0.915%
71	18.027	2554	2557	2562	rVB	103010	133053	4.34%	0.572%
72	18.104	2566	2570	2574	rVB	27486	36772	1.20%	0.158%
73	18.163	2575	2580	2584	rBV3	100234	164669	5.37%	0.708%
74	18.310	2600	2605	2608	rBV7	8428	16112	0.53%	0.069%
75	18.345	2608	2611	2615	rBV3	12985	17194	0.56%	0.074%
76	18.486	2631	2635	2639	rBV	56230	71279	2.32%	0.307%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
 Data File : BP022573.D
 Acq On : 23 Oct 2024 21:37
 Operator : RC/JU
 Sample : P4415-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

77	18.533	2639	2643	2649	rVB	49186	69249	2.26%	0.298%
78	18.592	2649	2653	2656	rBV6	14697	21740	0.71%	0.094%
79	18.757	2677	2681	2684	rBV5	24161	34277	1.12%	0.147%
80	18.810	2686	2690	2692	rBV	14854	23582	0.77%	0.101%
81	18.921	2704	2709	2713	rBV3	23937	43206	1.41%	0.186%
82	19.086	2733	2737	2745	rBV8	33664	89874	2.93%	0.387%
83	19.204	2752	2757	2762	rVB	1060024	1399366	45.63%	6.020%
84	19.327	2776	2778	2782	rVB3	25961	23837	0.78%	0.103%
85	19.551	2810	2816	2818	rBV2	663654	980246	31.96%	4.217%
86	19.580	2818	2821	2826	rVV	622326	819812	26.73%	3.527%
87	19.651	2830	2833	2841	rVB2	38339	73122	2.38%	0.315%
88	19.774	2851	2854	2860	rVB	46990	70773	2.31%	0.304%
89	19.915	2875	2878	2879	rBV2	46154	45261	1.48%	0.195%
90	20.021	2892	2896	2899	rBV3	55494	78101	2.55%	0.336%
91	20.104	2907	2910	2915	rVB	91260	117425	3.83%	0.505%
92	20.210	2924	2928	2932	rBV2	78154	97516	3.18%	0.419%
93	21.068	3071	3074	3078	rBV2	65462	79118	2.58%	0.340%
94	21.498	3139	3147	3152	rBV3	1481045	3066738	100.00%	13.192%
95	21.545	3152	3155	3166	rVB	338283	576231	18.79%	2.479%
96	23.733	3520	3527	3533	rBV	241785	656636	21.41%	2.825%
97	24.527	3658	3662	3669	rVB	155492	326380	10.64%	1.404%
98	24.756	3692	3701	3713	rVB	870291	2462276	80.29%	10.592%


Sum of corrected areas: 23246076

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022573.D
Acq On : 23 Oct 2024 21:37
Operator : RC/JU
Sample : P4415-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4F60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

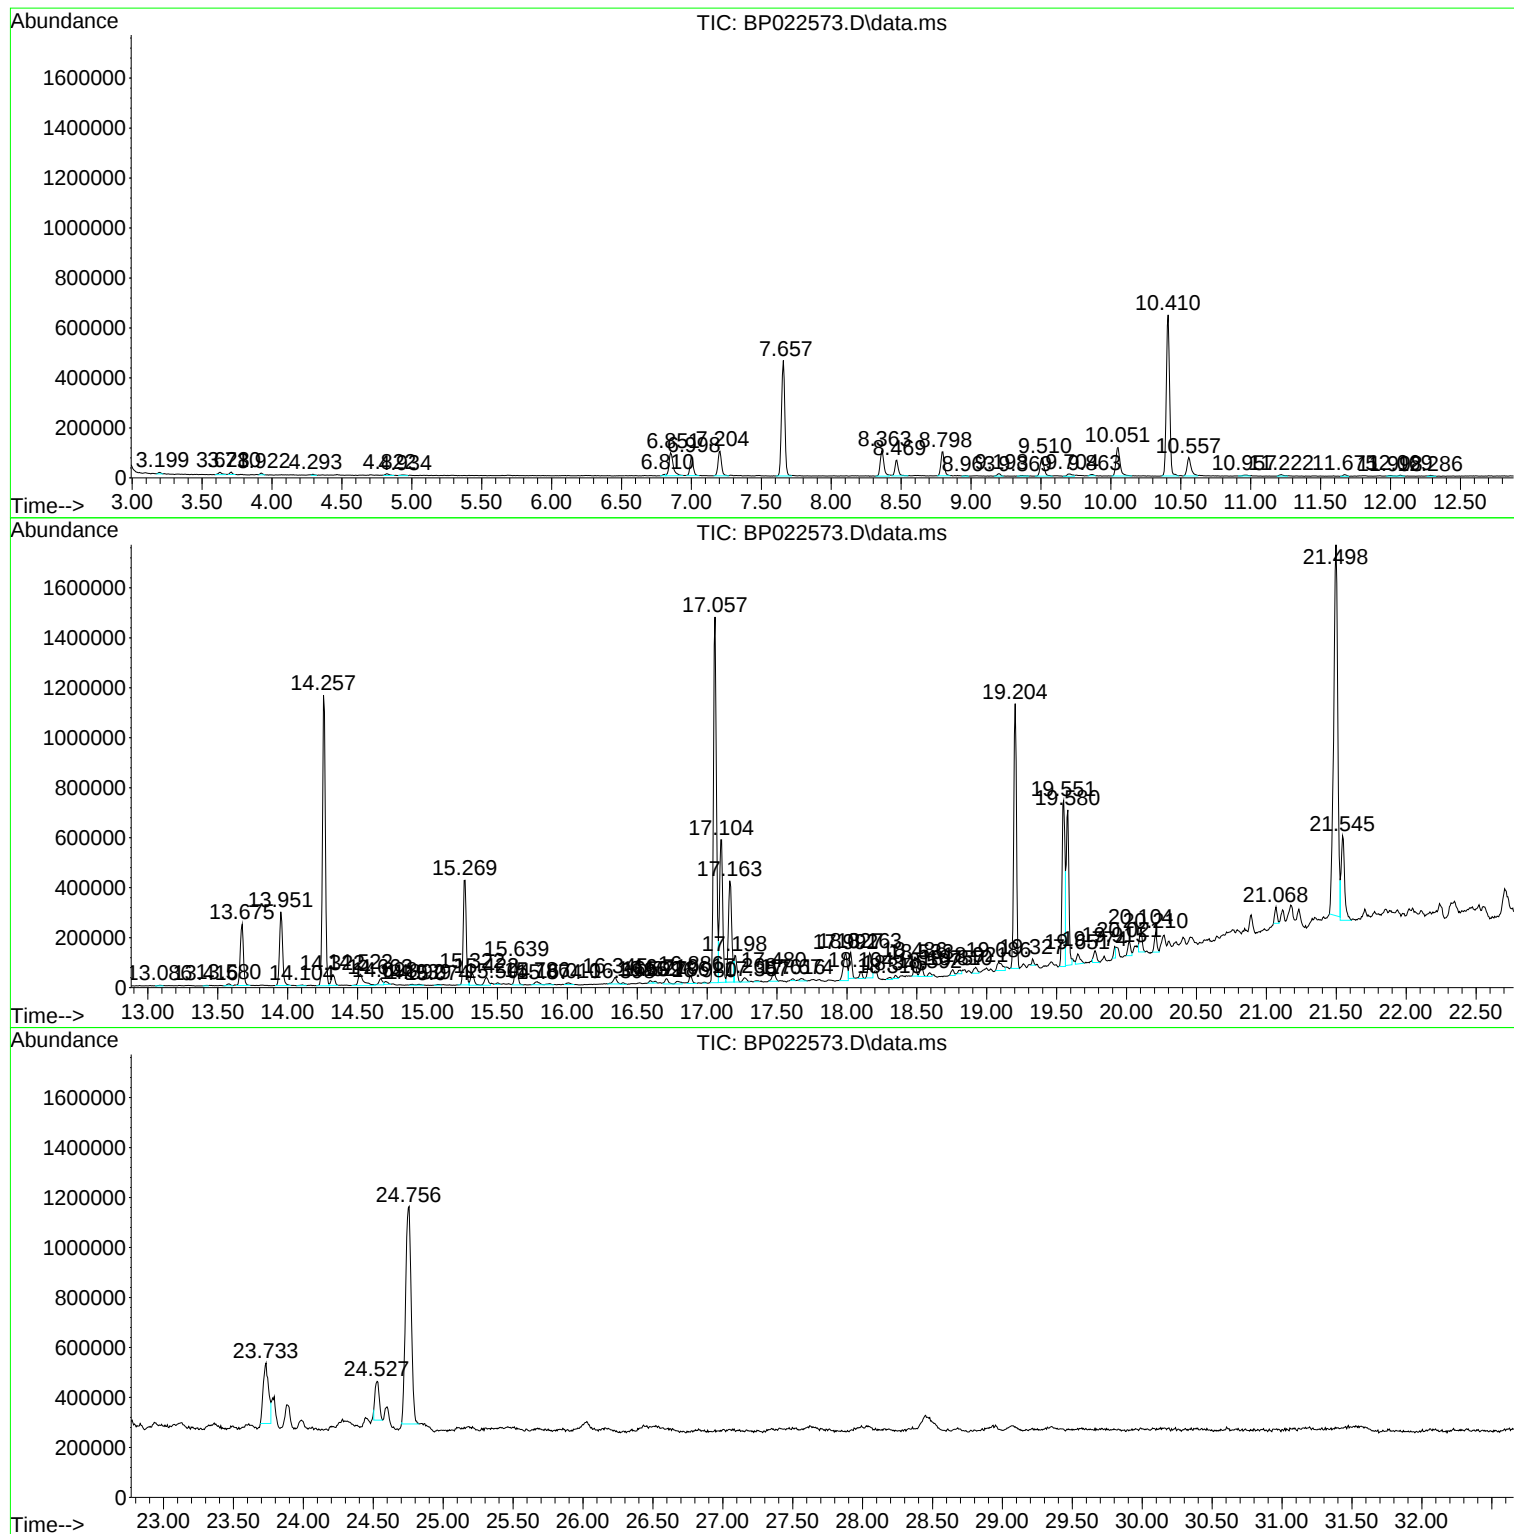

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022573.D
Acq On : 23 Oct 2024 21:37
Operator : RC/JU
Sample : P4415-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4F60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102124\
Data File : BP022573.D
Acq On : 23 Oct 2024 21:37
Operator : RC/JU
Sample : P4415-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4F60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc