
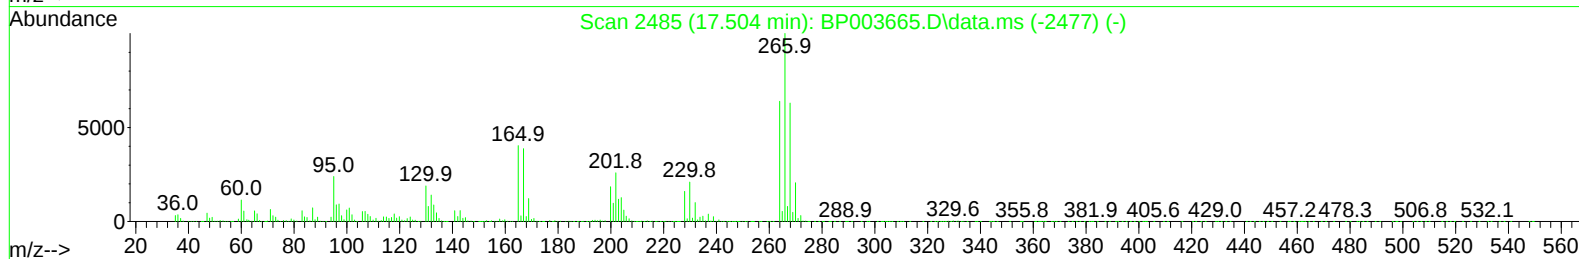
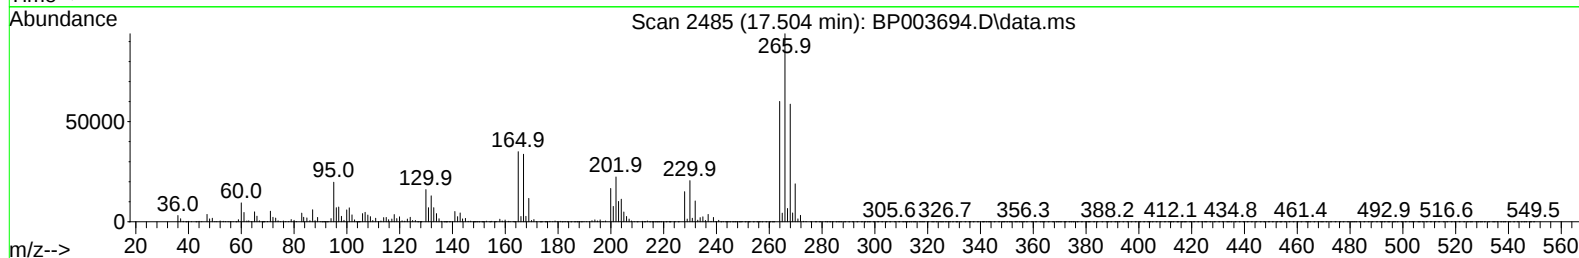


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102220\
Data File : BP003694.D
Acq On : 22 Oct 2020 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 04:07:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 14:54:24 2020
Response via : Initial Calibration

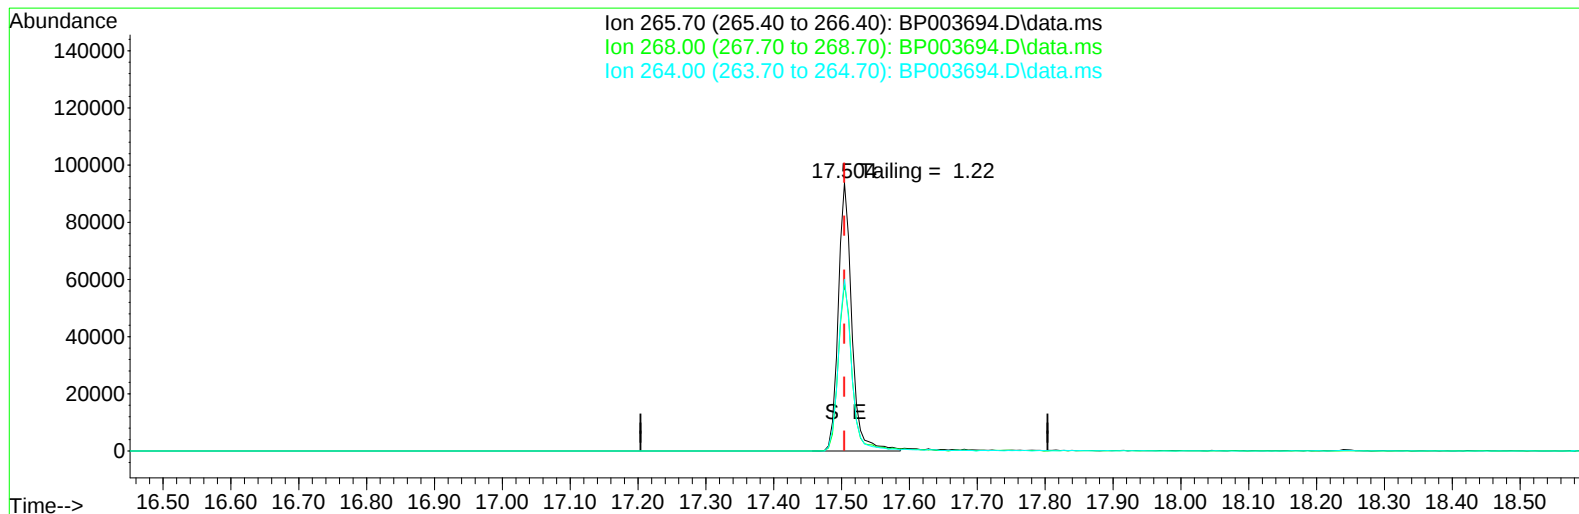

TIC: BP003694.D\data.ms

(70) Pentachlorophenol (C)




17.504min (+ 0.000) 656017.82 ng

response 129789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.56
264.00	63.30	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102220\
Data File : BP003694.D
Acq On : 22 Oct 2020 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 04:07:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 14:54:24 2020
Response via : Initial Calibration

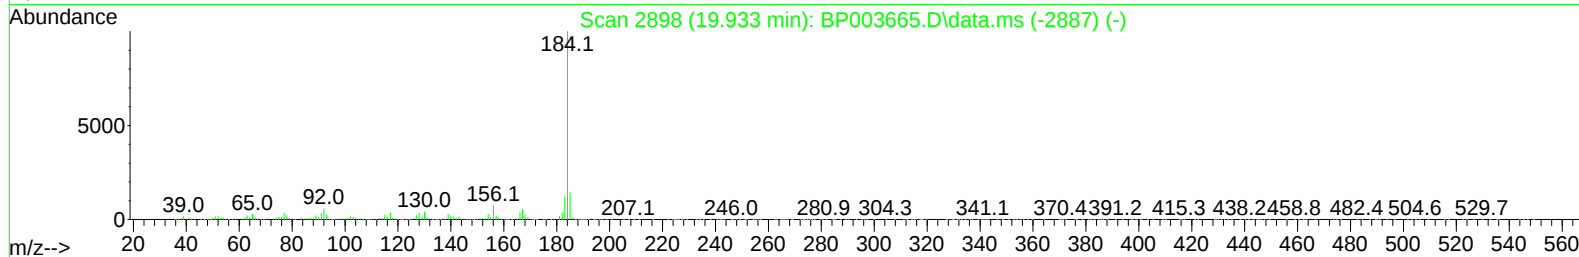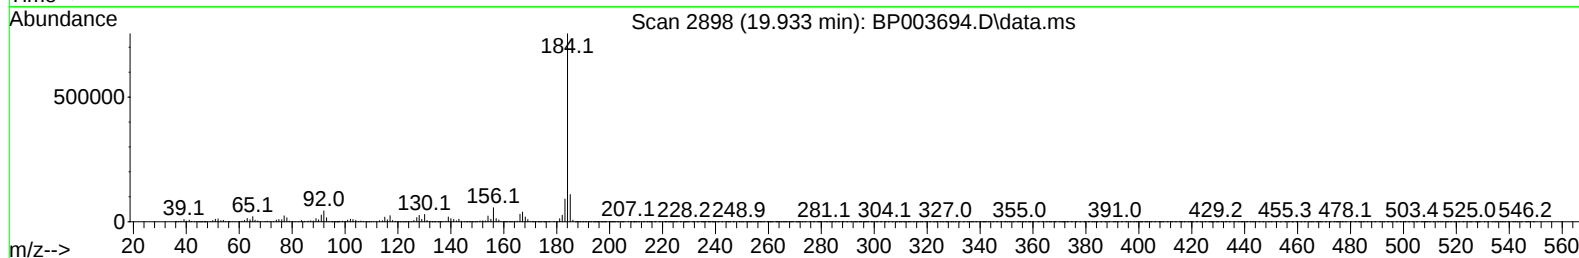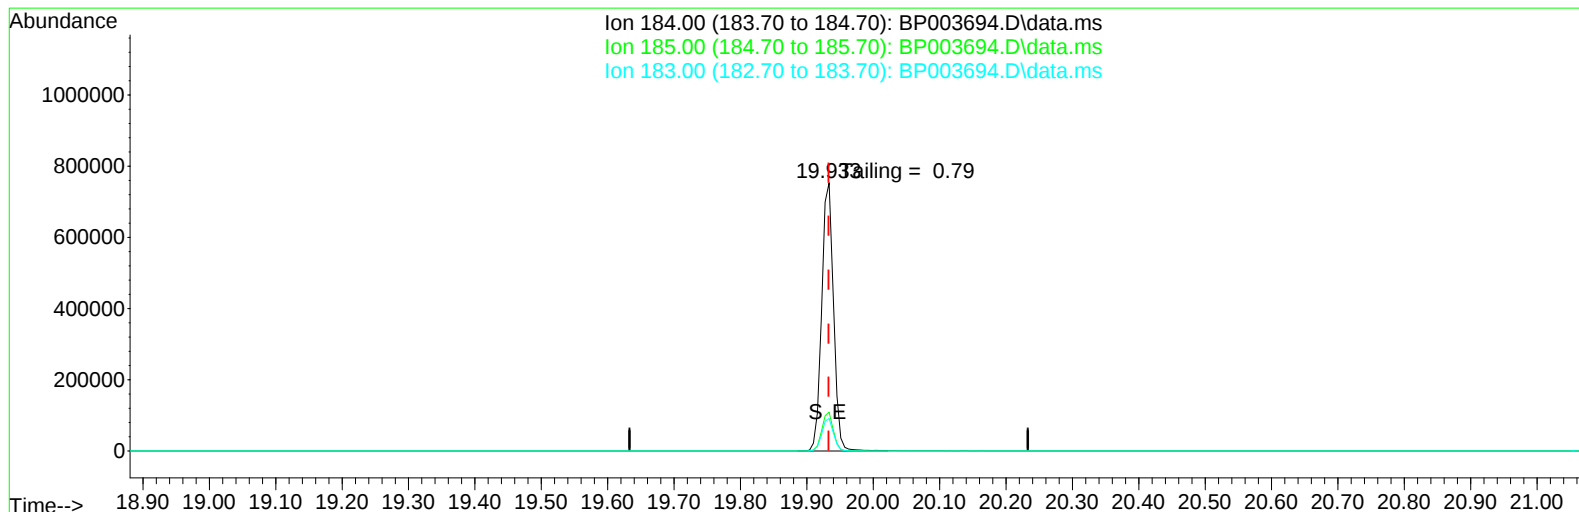

TIC: BP003694.D\data.ms

(77) Benzidine**19.933min (+ 0.000) 1391951.47 ng****response 933839**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.48
183.00	12.00	12.13
0.00	0.00	0.00