
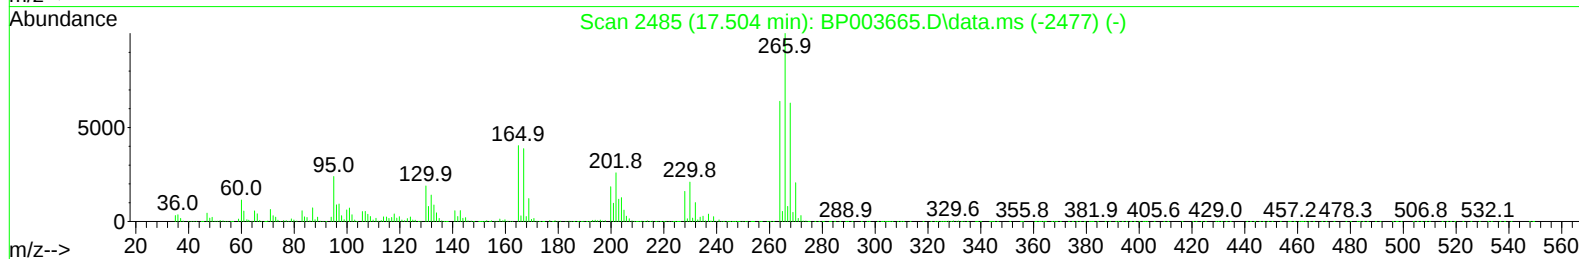
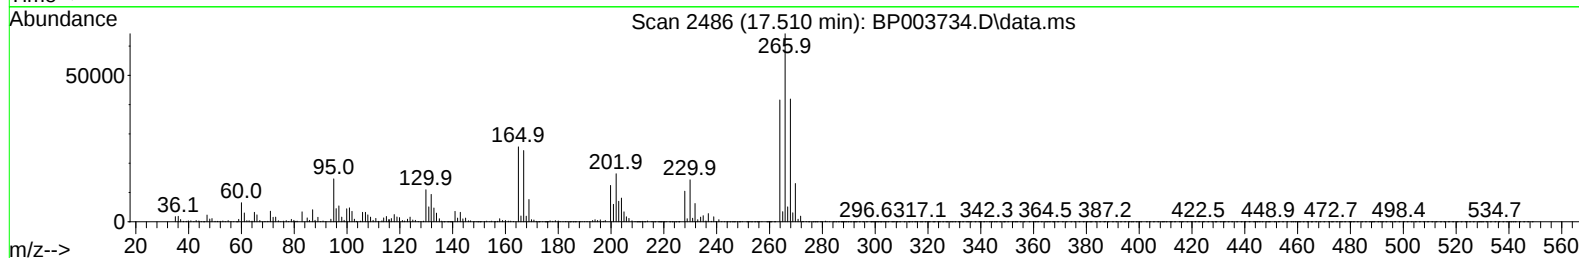


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003734.D
Acq On : 23 Oct 2020 23:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 02:38:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 14:54:24 2020
Response via : Initial Calibration

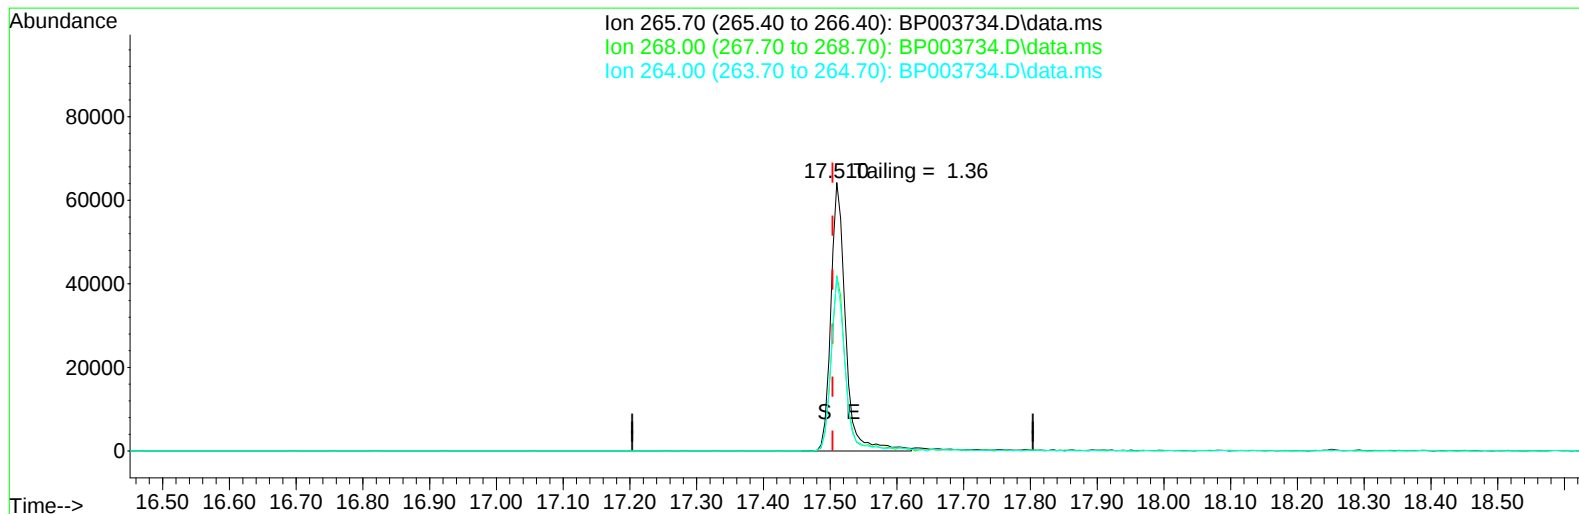

TIC: BP003734.D\data.ms

(70) Pentachlorophenol (C)




17.510min (+ 0.006) 21553.46 ng

response 98405

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.31
264.00	63.30	64.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003734.D
Acq On : 23 Oct 2020 23:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 02:38:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 14:54:24 2020
Response via : Initial Calibration

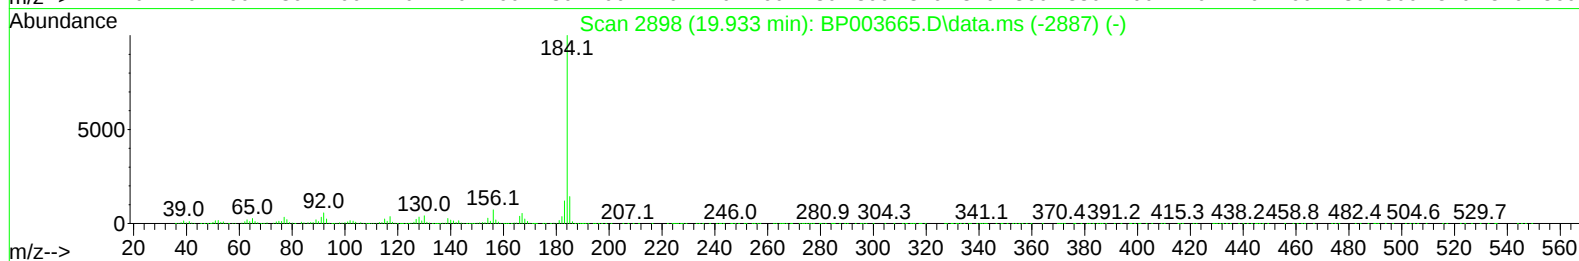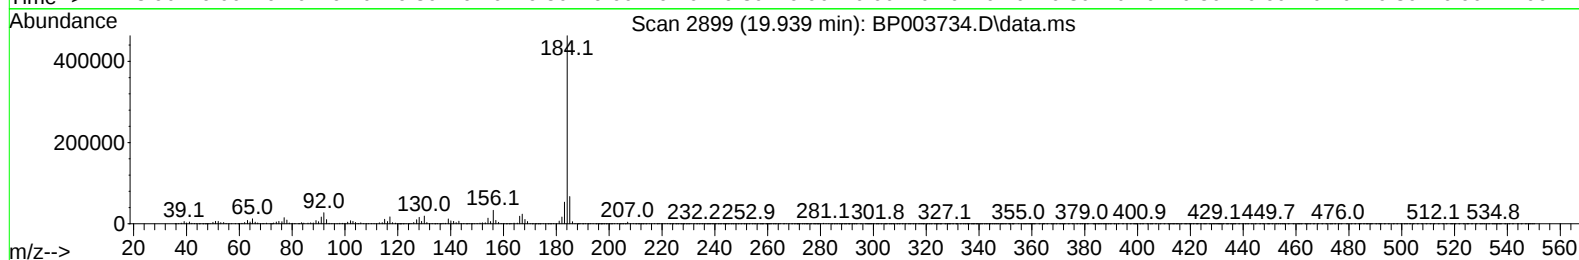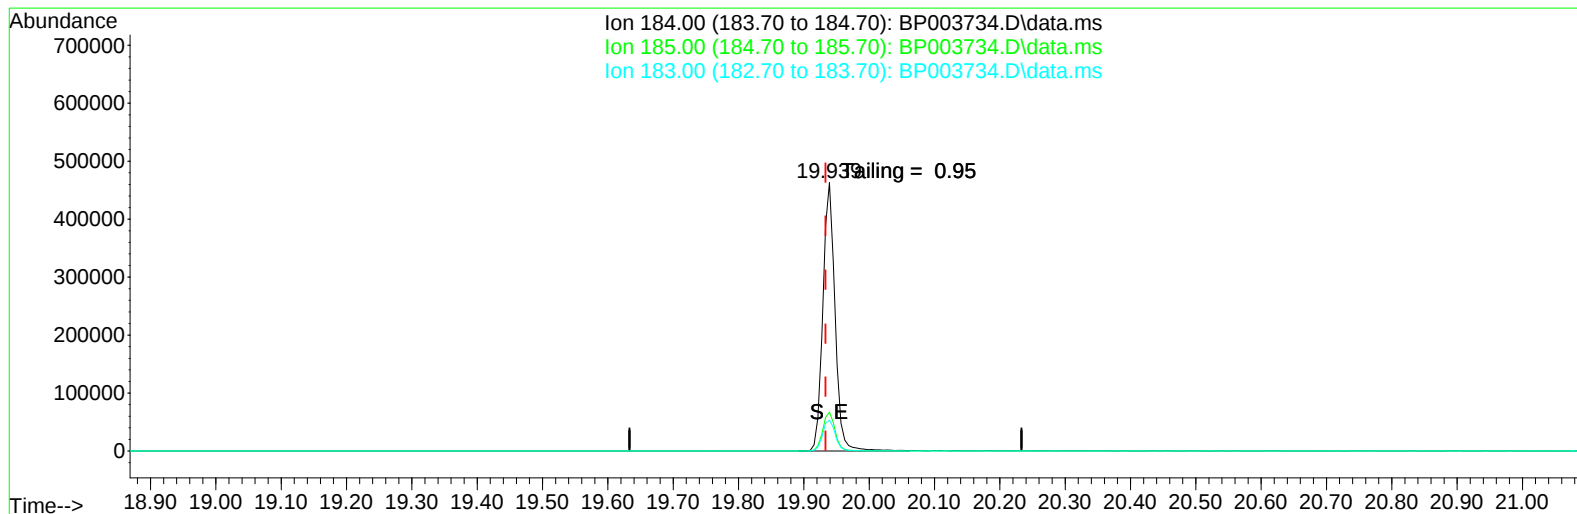

TIC: BP003734.D\data.ms

(77) Benzidine**19.939min (+ 0.006) 7211.12 ng****response 602483**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.49
183.00	12.00	11.52
0.00	0.00	0.00