

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
 Data File : BP003718.D
 Acq On : 23 Oct 2020 13:29
 Operator : CG/JU
 Sample : PB132540BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132540BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	31	37	54	rVB	3324062	4194718	44.45%	10.216%
2	3.264	57	64	75	rVB	54034	124665	1.32%	0.304%
3	6.022	525	533	550	rBV	2505968	3711362	39.33%	9.038%
4	7.675	805	814	828	rBV	2243946	3675348	38.95%	8.951%
5	8.522	951	958	967	rBV	436930	713036	7.56%	1.736%
6	9.693	1148	1157	1165	rBV	1546579	2556560	27.09%	6.226%
7	11.369	1434	1442	1451	rBV	547465	899597	9.53%	2.191%
8	13.751	1838	1847	1864	rBV	4127782	5808690	61.55%	14.146%
9	15.122	2072	2080	2090	rBV2	808923	1188205	12.59%	2.894%
10	16.592	2323	2330	2346	rBV	2743466	3949421	41.85%	9.618%
11	17.839	2536	2542	2555	rBV	1025226	1437530	15.23%	3.501%
12	20.310	2956	2962	2972	rBV	7824585	9436860	100.00%	22.982%
13	21.851	3218	3224	3236	rBV	1219259	1717135	18.20%	4.182%
14	24.433	3655	3663	3672	rVB2	789418	1648952	17.47%	4.016%




Sum of corrected areas: 41062079

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003718.D
Acq On : 23 Oct 2020 13:29
Operator : CG/JU
Sample : PB132540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132540BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

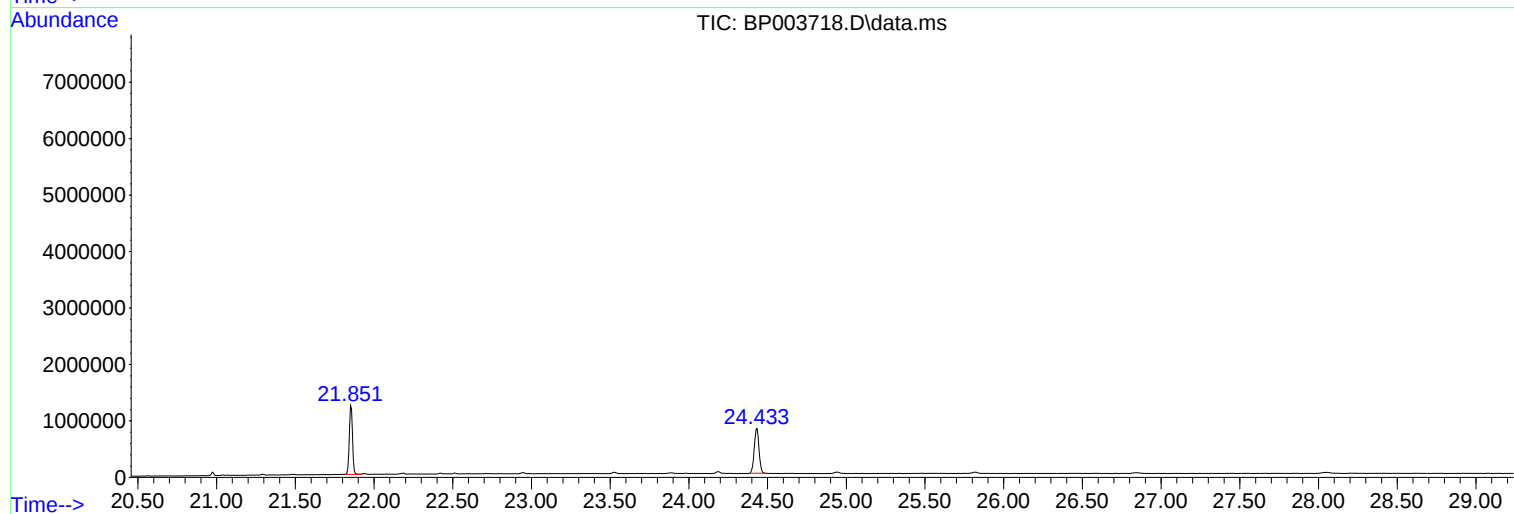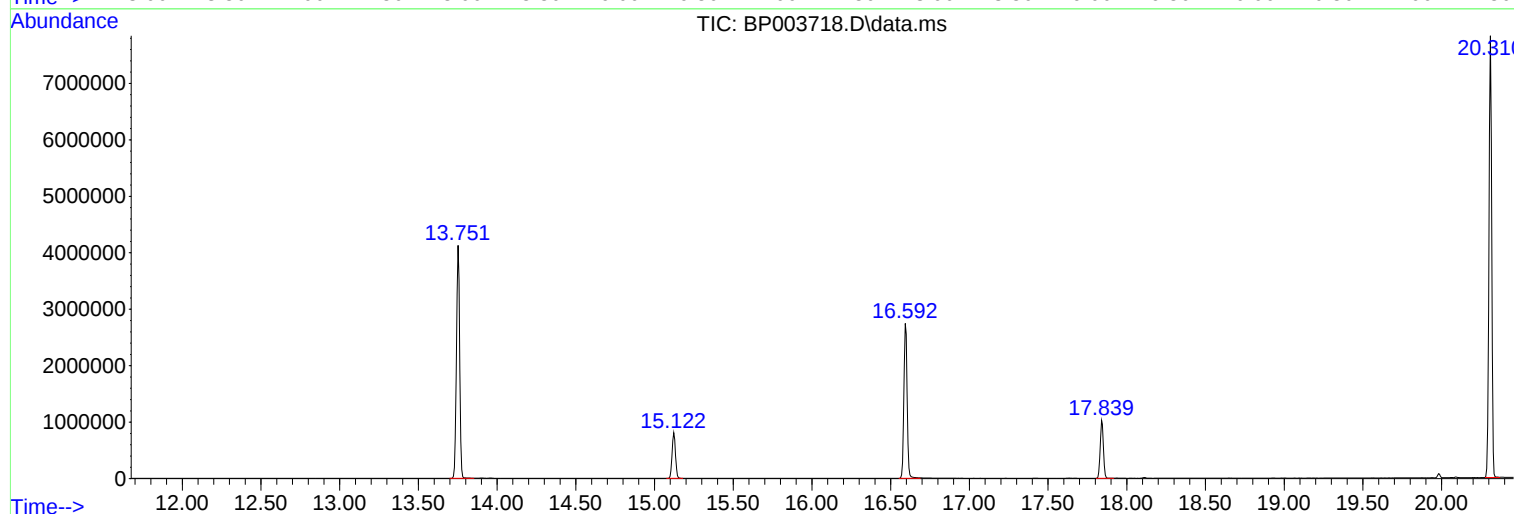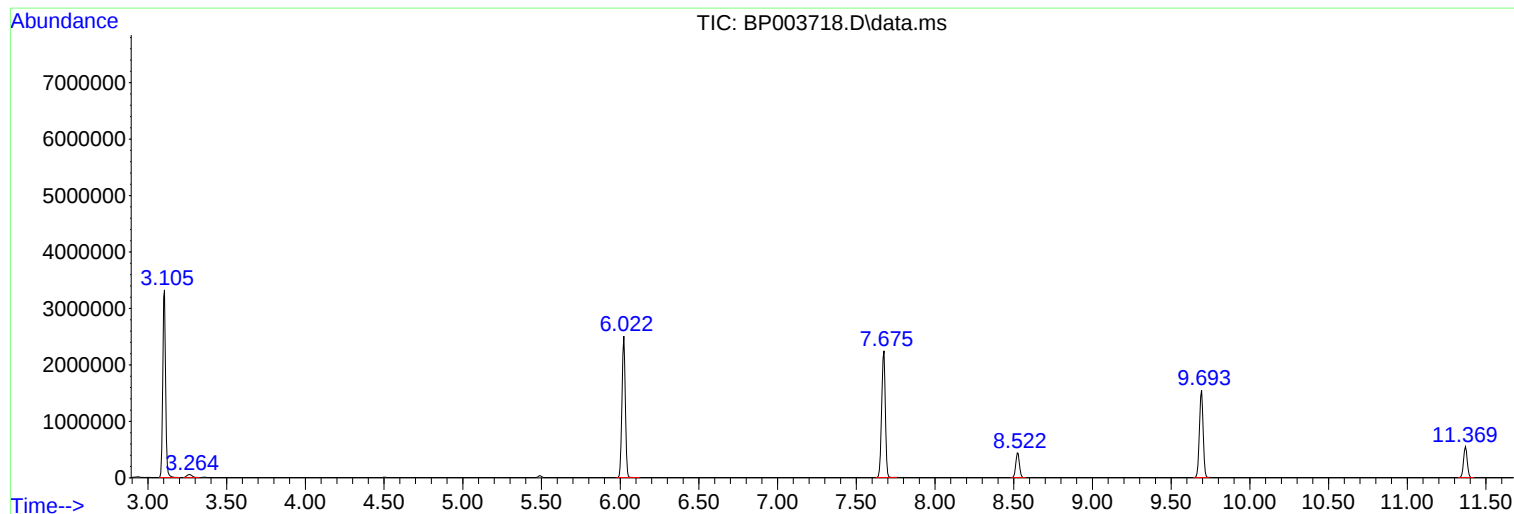

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003718.D
Acq On : 23 Oct 2020 13:29
Operator : CG/JU
Sample : PB132540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132540BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.105	117.66 ng	4194720	1,4-Dichlorobenzene-d4	8.528

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	50
2			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
3			2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9
4			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
5			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	7

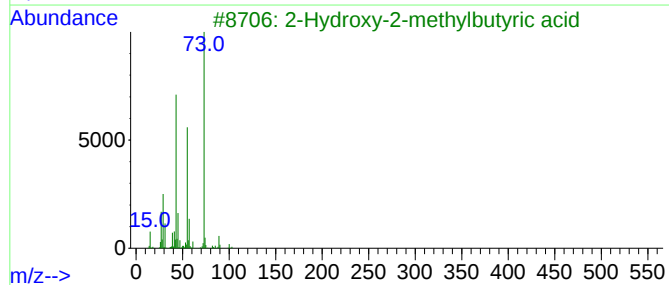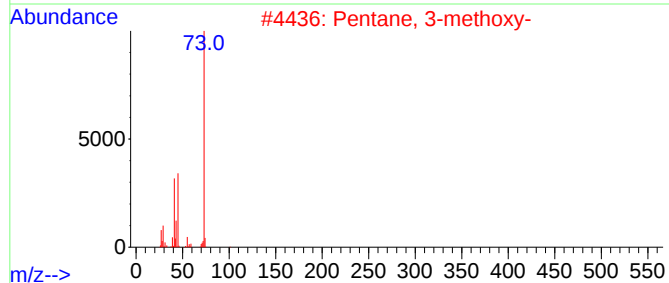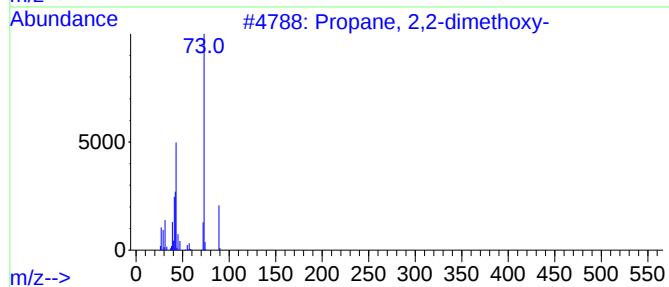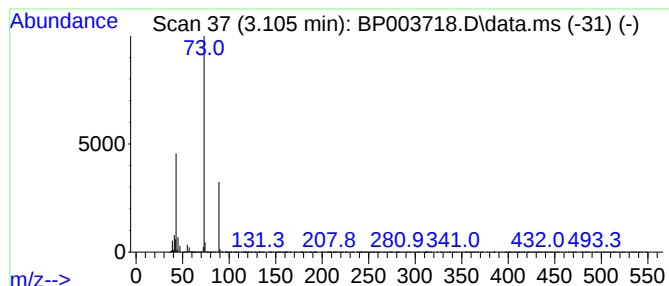

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003718.D
Acq On : 23 Oct 2020 13:29
Operator : CG/JU
Sample : PB132540BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132540BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-di...	3.105	117.7	ng	4194720	1	8.528	713036	20.0