

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
 Data File : BP003736.D
 Acq On : 24 Oct 2020 02:14
 Operator : CG/JU
 Sample : PB132603BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132603BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	31	37	55	rVB	4758695	5659210	66.68%	14.173%
2	6.028	526	534	547	rBV	2323066	3448868	40.64%	8.637%
3	7.681	806	815	823	rBV	2115671	3398464	40.04%	8.511%
4	8.528	949	959	968	rBV	441143	708175	8.34%	1.774%
5	9.693	1148	1157	1165	rBV	1443165	2391816	28.18%	5.990%
6	11.369	1431	1442	1455	rBV	520832	886708	10.45%	2.221%
7	13.751	1839	1847	1863	rBV	3658828	5383938	63.44%	13.483%
8	15.122	2074	2080	2092	rBV	776631	1140409	13.44%	2.856%
9	16.598	2323	2331	2353	rBV	2611333	3839725	45.24%	9.616%
10	17.845	2536	2543	2554	rBV	942616	1370310	16.15%	3.432%
11	20.310	2956	2962	2976	rBV	6989553	8487063	100.00%	21.255%
12	21.857	3219	3225	3235	rVB	1194968	1642807	19.36%	4.114%
13	24.433	3656	3663	3673	rVB	747657	1572703	18.53%	3.939%


Sum of corrected areas: 39930196

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003736.D
Acq On : 24 Oct 2020 02:14
Operator : CG/JU
Sample : PB132603BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132603BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

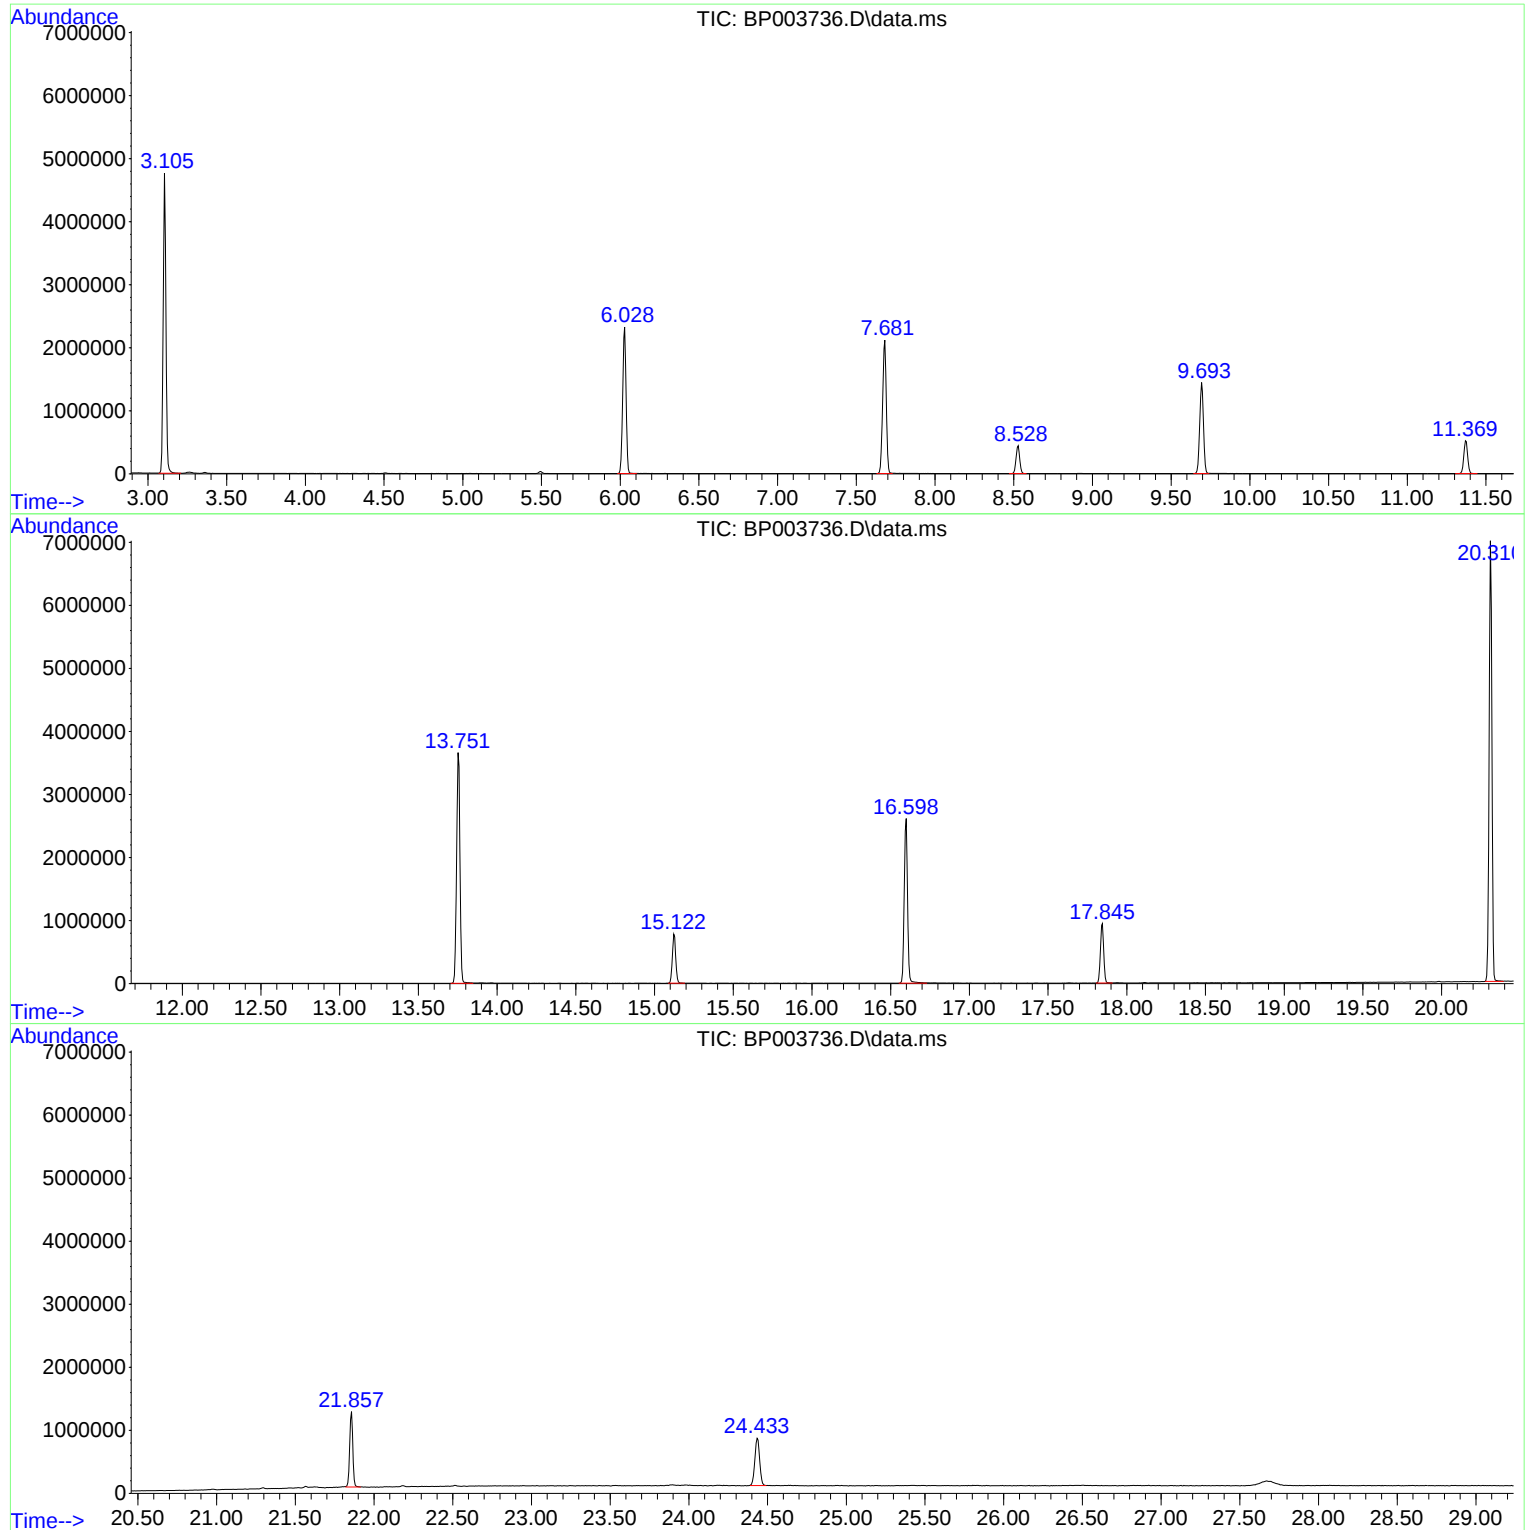

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003736.D
Acq On : 24 Oct 2020 02:14
Operator : CG/JU
Sample : PB132603BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132603BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.105	159.82 ng	5659210	1,4-Dichlorobenzene-d4	8.528

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	50
2			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
3			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
4			2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9
5			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	7

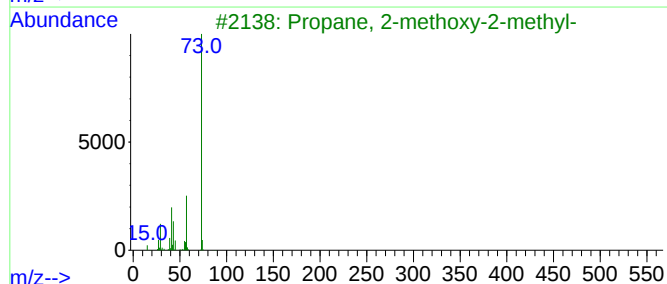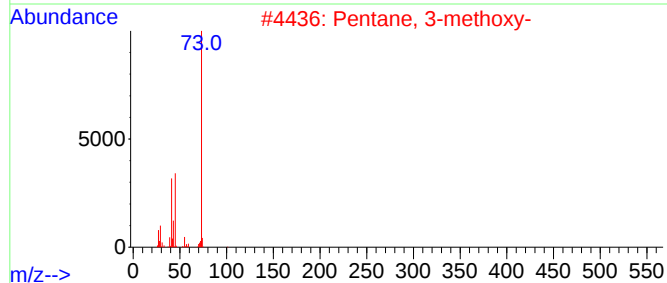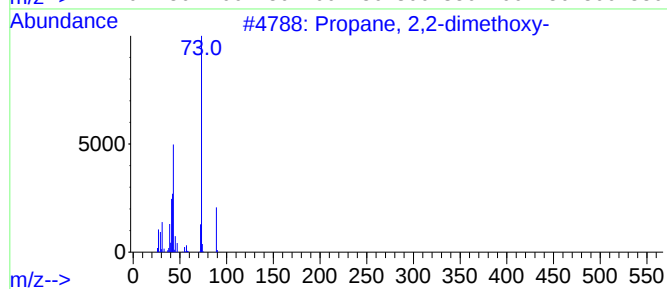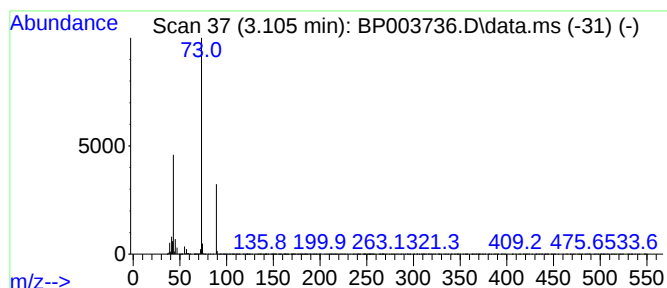

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003736.D
Acq On : 24 Oct 2020 02:14
Operator : CG/JU
Sample : PB132603BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132603BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-di...	3.105	159.8	ng	5659210	1	8.528	708175	20.0