
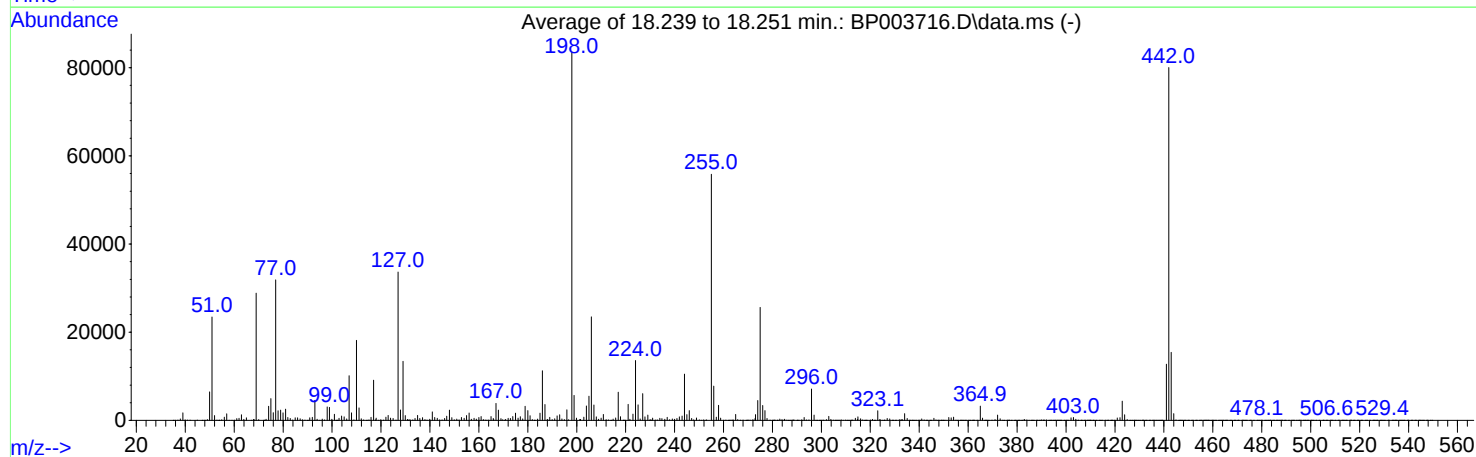


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
 Data File : BP003716.D
 Acq On : 23 Oct 2020 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 19 14:54:24 2020

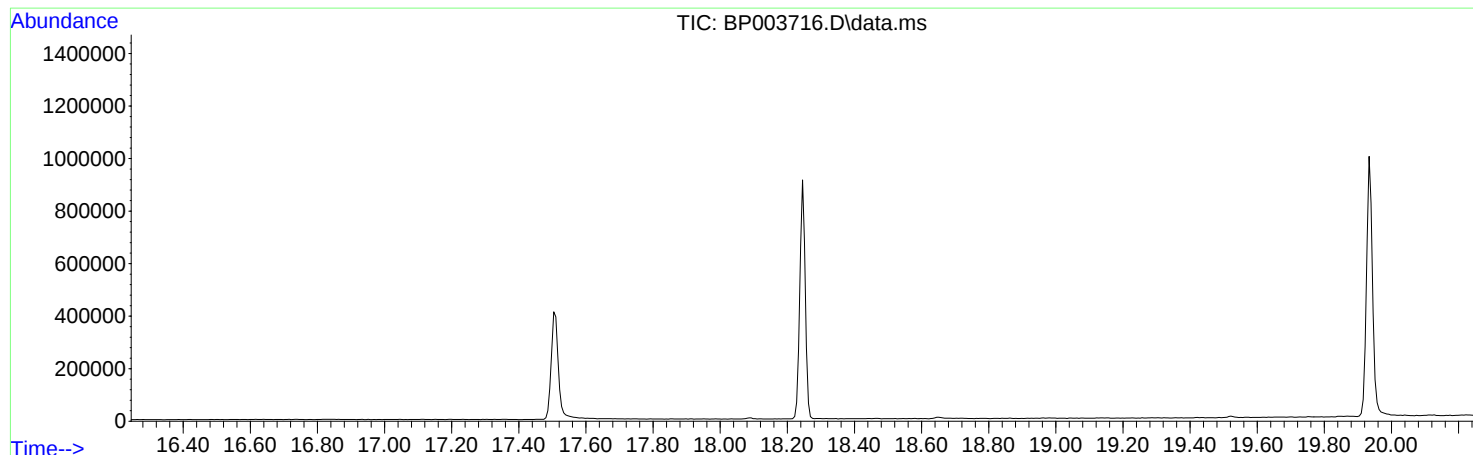

AutoFind: Scans 2610, 2611, 2612; Background Corrected with Scan 2603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	23449	PASS
68	69	0.00	2	0.8	223	PASS
69	198	0.00	100	34.6	28862	PASS
70	69	0.00	2	0.6	178	PASS
127	198	10	80	40.3	33637	PASS
197	198	0.00	2	0.2	163	PASS
198	198	100	100	100.0	83461	PASS
199	198	5	9	6.8	5667	PASS
275	198	10	60	30.7	25627	PASS
365	198	1	100	3.9	3225	PASS
441	198	0.01	100	15.3	12746	PASS
442	198	50	100	95.9	80045	PASS
443	442	15	24	19.3	15430	PASS