
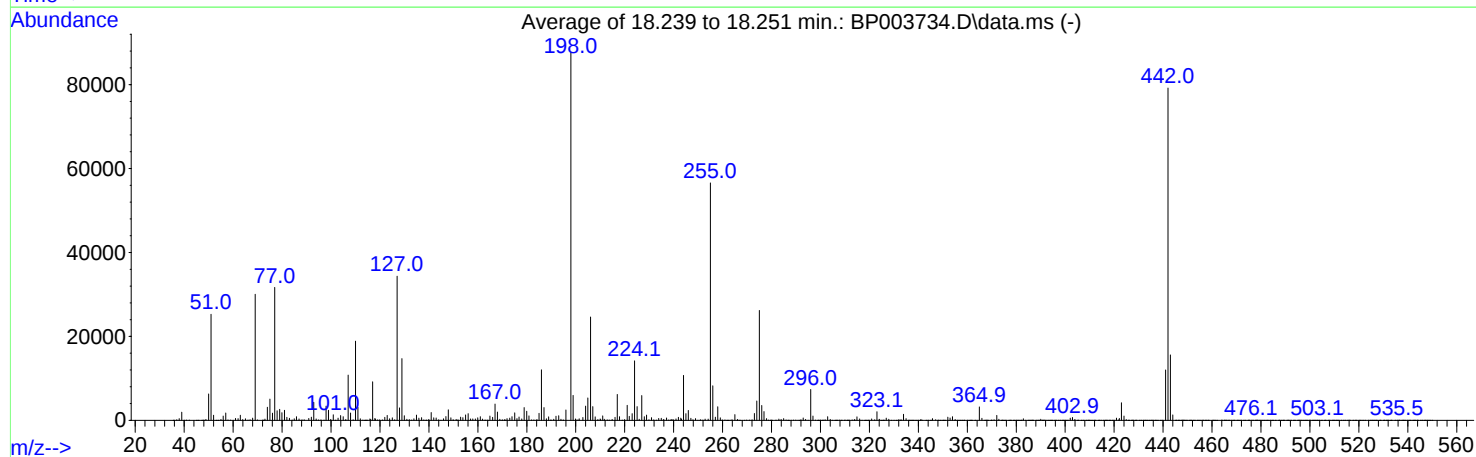


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102320\
Data File : BP003734.D
Acq On : 23 Oct 2020 23:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 19 14:54:24 2020

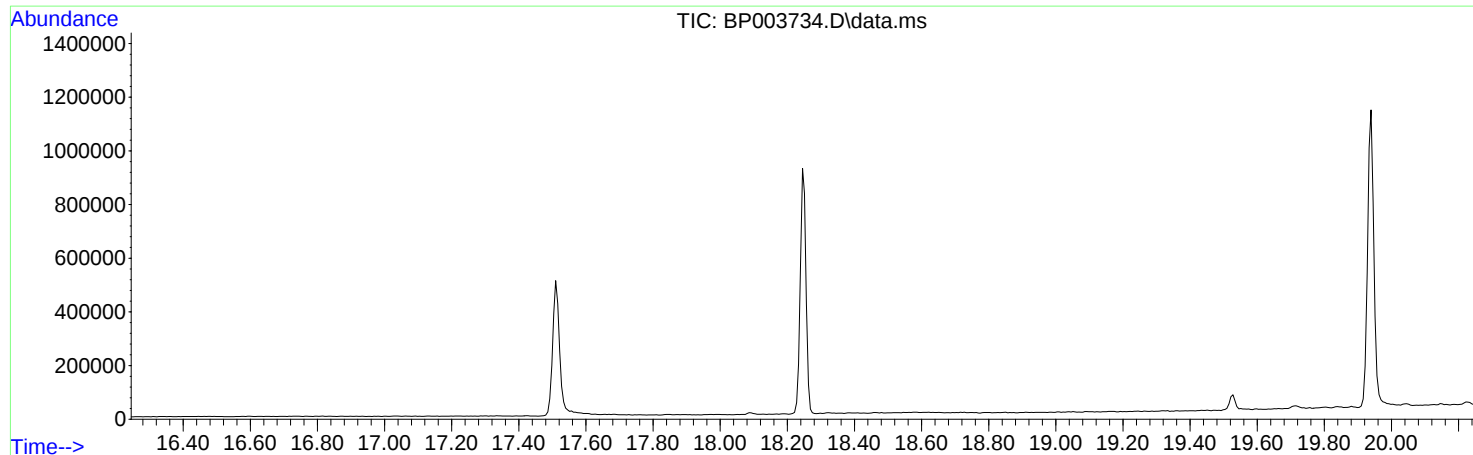

AutoFind: Scans 2610, 2611, 2612; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	25288	PASS
68	69	0.00	2	1.7	521	PASS
69	198	0.00	100	34.3	30032	PASS
70	69	0.00	2	0.4	127	PASS
127	198	10	80	39.2	34341	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87651	PASS
199	198	5	9	6.8	5943	PASS
275	198	10	60	29.9	26203	PASS
365	198	1	100	3.6	3193	PASS
441	198	0.01	100	13.7	12031	PASS
442	198	50	100	90.3	79171	PASS
443	442	15	24	19.7	15578	PASS