

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012286.D
 Acq On : 24 Oct 2022 15:38
 Operator : CG/JU
 Sample : N5070-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BQ7

Quant Time: Oct 25 06:14:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 22 01:24:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	388788	20.000	ng/u1	0.00
20) Naphthalene-d8	10.622	136	1542559	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.469	164	838513	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.227	188	1584652	20.000	ng/u1	0.00
79) Chrysene-d12	21.321	240	1654447	20.000	ng/u1	0.00
88) Perylene-d12	23.715	264	1793276	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	27485	2.861	ng/uL	0.00
4) Pyridine-d5	3.687	84	73371	2.650	ng/u1	0.00
7) Phenol-d5	6.987	99	774833	23.085	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	482008	23.679	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	611105	23.919	ng/u1	0.00
15) 4-Methylphenol-d8	8.534	113	463833	17.781	ng/u1	0.00
21) Nitrobenzene-d5	8.987	128	300551	26.322	ng/u1	0.00
24) 2-Nitrophenol-d4	9.704	143	309668	25.137	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.245	165	513940	22.241	ng/u1	0.00
31) 4-Chloroaniline-d4	10.769	131	621714	18.937	ng/u1	0.00
46) Dimethylphthalate-d6	13.881	166	1595857	27.360	ng/u1	0.00
49) Acenaphthylene-d8	14.157	160	1790399	26.891	ng/u1	0.00
54) 4-Nitrophenol-d4	14.686	143	212246	19.423	ng/u1	0.00
60) Fluorene-d10	15.463	176	1296868	25.844	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	103031	11.429	ng/u1	0.00
73) Anthracene-d10	17.327	188	1965728	28.300	ng/u1	0.00
81) Pyrene-d10	19.569	212	2495582	26.493	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.562	264	2768598	30.786	ng/u1	0.00


Target Compounds				Qvalue	
8) Phenol	7.016	94	40661	1.158 ng/u1#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012286.D
Acq On : 24 Oct 2022 15:38
Operator : CG/JU
Sample : N5070-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BQ7

Quant Time: Oct 25 06:14:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

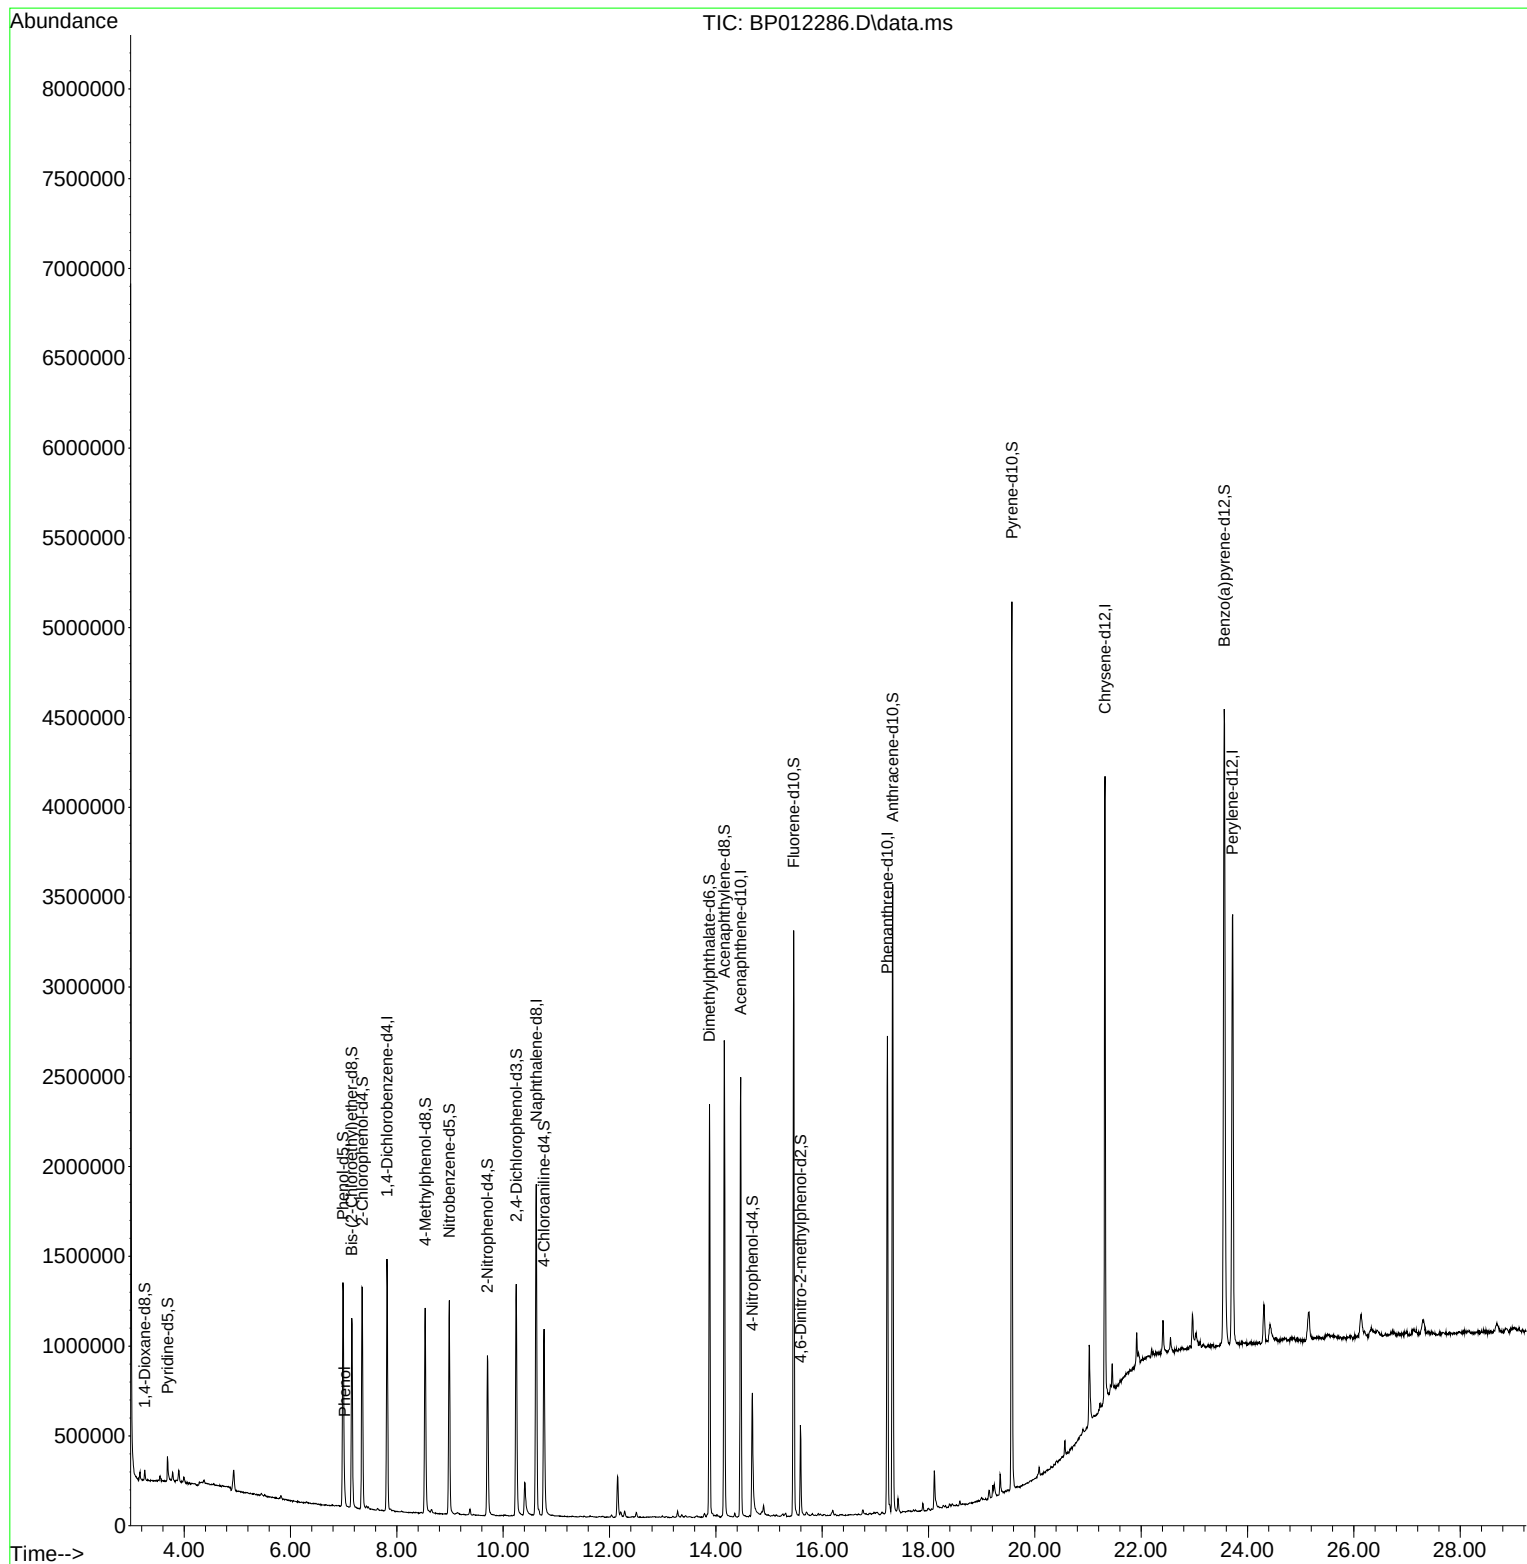

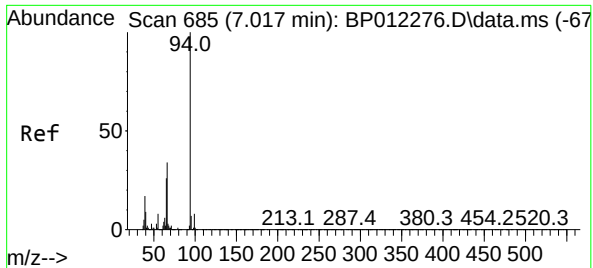

#8
Phenol
Concen: 1.158 ng/ul
RT: 7.016 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP012286.D
Acq: 24 Oct 2022 15:38

Instrument :
BNA_P
ClientSampleId :
C0BQ7

Tgt Ion: 94 Resp: 40661
Ion Ratio Lower Upper
94 100
65 31.2 20.6 31.0#
66 40.9 26.2 39.4#

