

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012291.D
 Acq On : 24 Oct 2022 18:30
 Operator : CG/JU
 Sample : N5070-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BQ6

Quant Time: Oct 25 06:31:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 22 01:24:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	355663	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	1516317	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.469	164	801774	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	1419043	20.000	ng/ul	0.00
79) Chrysene-d12	21.316	240	1395899	20.000	ng/ul	0.00
88) Perylene-d12	23.716	264	1509892	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	11066	1.259	ng/uL	0.00
4) Pyridine-d5	3.687	84	39075	1.543	ng/ul	0.00
7) Phenol-d5	6.987	99	563803	18.362	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	384132	20.629	ng/ul	0.00
11) 2-Chlorophenol-d4	7.346	132	454341	19.440	ng/ul	0.00
15) 4-Methylphenol-d8	8.534	113	218979	9.176	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	236457	21.067	ng/ul	0.00
24) 2-Nitrophenol-d4	9.705	143	239468	19.775	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	405794	17.865	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	444499	13.773	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	1348943	24.187	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1508413	23.694	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	147670	14.133	ng/ul	0.00
60) Fluorene-d10	15.463	176	1090494	22.727	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	66292	8.212	ng/ul	0.00
73) Anthracene-d10	17.328	188	1521349	24.459	ng/ul	0.00
81) Pyrene-d10	19.569	212	2067080	26.009	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.563	264	2212651	29.222	ng/ul	0.00
Target Compounds						
80) Fluoranthene	19.239	202	100582	1.024	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012291.D
Acq On : 24 Oct 2022 18:30
Operator : CG/JU
Sample : N5070-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BQ6

Quant Time: Oct 25 06:31:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

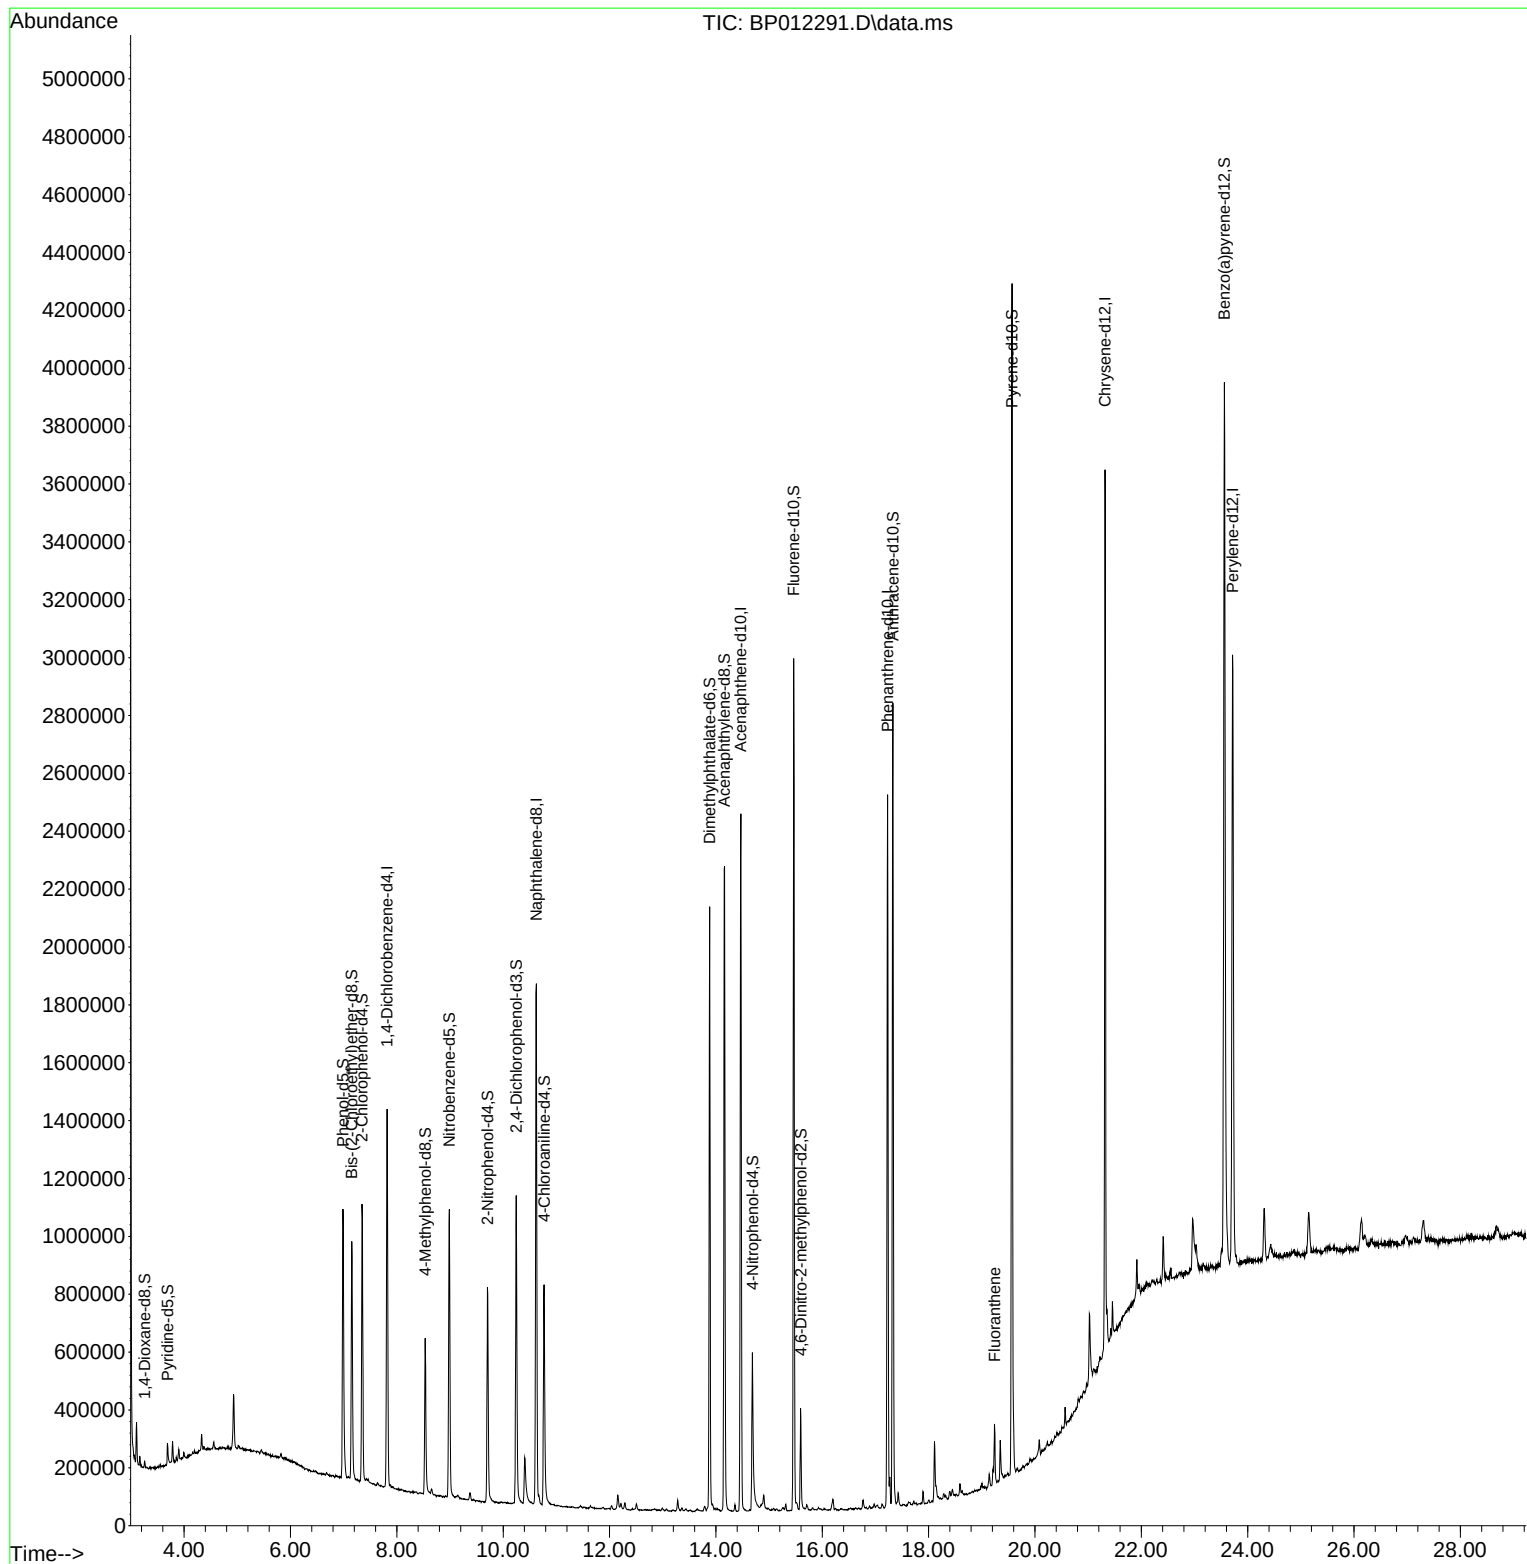

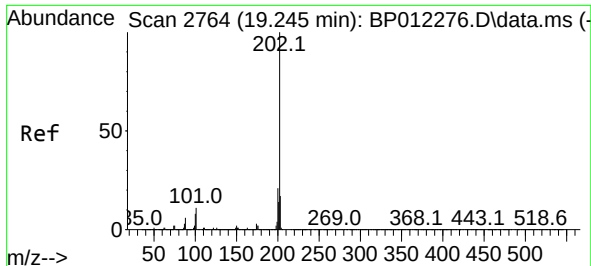

#80
 Fluoranthene
 Concen: 1.024 ng/ul
 RT: 19.239 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP012291.D
 Acq: 24 Oct 2022 18:30

Instrument :
 BNA_P
 ClientSampleId :
 C0BQ6

Tgt Ion:202 Resp: 100582
 Ion Ratio Lower Upper
 202 100
 101 12.9 10.4 15.6
 100 10.4 7.7 11.5

