

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012277.D
 Acq On : 24 Oct 2022 10:30
 Operator : CG/JU
 Sample : PB148367BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	42	46	52	rVB	95586	121216	2.18%	0.183%
2	3.681	114	118	143	rBV	1158000	1826246	32.88%	2.758%
3	3.999	168	172	178	rVB2	19388	27753	0.50%	0.042%
4	4.087	183	187	190	rBV2	4616	7009	0.13%	0.011%
5	4.116	190	192	197	rBV4	4293	6462	0.12%	0.010%
6	4.357	230	233	235	rBV2	5709	7189	0.13%	0.011%
7	5.222	378	380	384	rBV	6548	10767	0.19%	0.016%
8	5.540	431	434	437	rVV2	4513	5660	0.10%	0.009%
9	5.828	479	483	486	rBV	4142	6145	0.11%	0.009%
10	6.434	580	586	587	rBV2	5582	9448	0.17%	0.014%
11	6.593	608	613	614	rVB	6081	7235	0.13%	0.011%
12	6.698	628	631	635	rBV	5631	6065	0.11%	0.009%
13	6.993	674	681	691	rVV	1311859	2146609	38.65%	3.242%
14	7.081	694	696	699	rVV	5355	6941	0.12%	0.010%
15	7.157	702	709	720	rVV	1100516	1759677	31.68%	2.658%
16	7.351	734	742	755	rBV	1365998	2158823	38.87%	3.261%
17	7.510	766	769	772	rVB	5937	6451	0.12%	0.010%
18	7.822	812	822	833	rBV	1172040	1933623	34.82%	2.921%
19	7.904	833	836	839	rVB	5298	7777	0.14%	0.012%
20	7.993	849	851	854	rVB	6628	7866	0.14%	0.012%
21	8.075	861	865	867	rBV	5088	6778	0.12%	0.010%
22	8.534	935	943	956	rBV	1554553	2633140	47.41%	3.977%
23	8.787	983	986	988	rBV	6002	5601	0.10%	0.008%
24	8.987	1012	1020	1035	rBV	1199977	2050799	36.93%	3.098%
25	9.157	1045	1049	1050	rBV	5261	6043	0.11%	0.009%
26	9.710	1135	1143	1161	rBV	928506	1591323	28.65%	2.404%
27	10.163	1215	1220	1223	rBV	3789	6123	0.11%	0.009%
28	10.251	1227	1235	1250	rBV	1364489	2487876	44.80%	3.758%
29	10.622	1289	1298	1308	rBV	1582842	2732215	49.20%	4.127%
30	10.769	1315	1323	1337	rBV	1374000	2522060	45.41%	3.809%
31	11.063	1371	1373	1378	rVB	5860	6780	0.12%	0.010%
32	11.981	1526	1529	1534	rBV2	5289	10567	0.19%	0.016%
33	12.228	1565	1571	1578	rBV2	18981	40809	0.73%	0.062%
34	12.304	1581	1584	1587	rVB	6314	7439	0.13%	0.011%
35	12.816	1667	1671	1672	rBV	5322	5695	0.10%	0.009%
36	13.451	1774	1779	1780	rBV2	6482	8572	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012277.D
 Acq On : 24 Oct 2022 10:30
 Operator : CG/JU
 Sample : PB148367BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	13.622	1806	1808	1813	rBV2	5465	7073	0.13%	0.011%
38	13.763	1831	1832	1835	rBV2	5122	6199	0.11%	0.009%
39	13.886	1846	1853	1865	rBV	2116126	3128894	56.34%	4.726%
40	14.163	1893	1900	1912	rBV	2672072	3993716	71.91%	6.032%
41	14.469	1944	1952	1963	rVV	2151562	3200827	57.63%	4.835%
42	14.692	1983	1990	2007	rBV	493736	1062287	19.13%	1.605%
43	14.916	2026	2028	2031	rVB	8334	6402	0.12%	0.010%
44	14.963	2034	2036	2038	rBV	7363	7218	0.13%	0.011%
45	15.469	2115	2122	2132	rBV	3167643	4590168	82.65%	6.933%
46	15.598	2138	2144	2157	rBV	390187	594326	10.70%	0.898%
47	15.710	2160	2163	2167	rVB2	16507	18101	0.33%	0.027%
48	16.169	2237	2241	2242	rBV2	5619	8381	0.15%	0.013%
49	17.227	2415	2421	2430	rBV	2172729	3120971	56.20%	4.714%
50	17.327	2432	2438	2452	rVV	3085197	4464478	80.39%	6.743%
51	17.592	2481	2483	2484	rBV	8620	6138	0.11%	0.009%
52	19.145	2744	2747	2751	rBV3	38699	46444	0.84%	0.070%
53	19.215	2756	2759	2764	rVB2	37686	51405	0.93%	0.078%
54	19.568	2813	2819	2829	rBV	3839157	5033912	90.64%	7.603%
55	21.227	3098	3101	3105	rBV	164201	178490	3.21%	0.270%
56	21.321	3112	3117	3126	rBV	2670397	3382219	60.90%	5.109%
57	23.568	3492	3499	3509	rVB2	2785022	5553757	100.00%	8.389%
58	23.721	3519	3525	3538	rVB2	1679363	3554425	64.00%	5.369%




Sum of corrected areas: 66206613

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012277.D
Acq On : 24 Oct 2022 10:30
Operator : CG/JU
Sample : PB148367BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK367

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

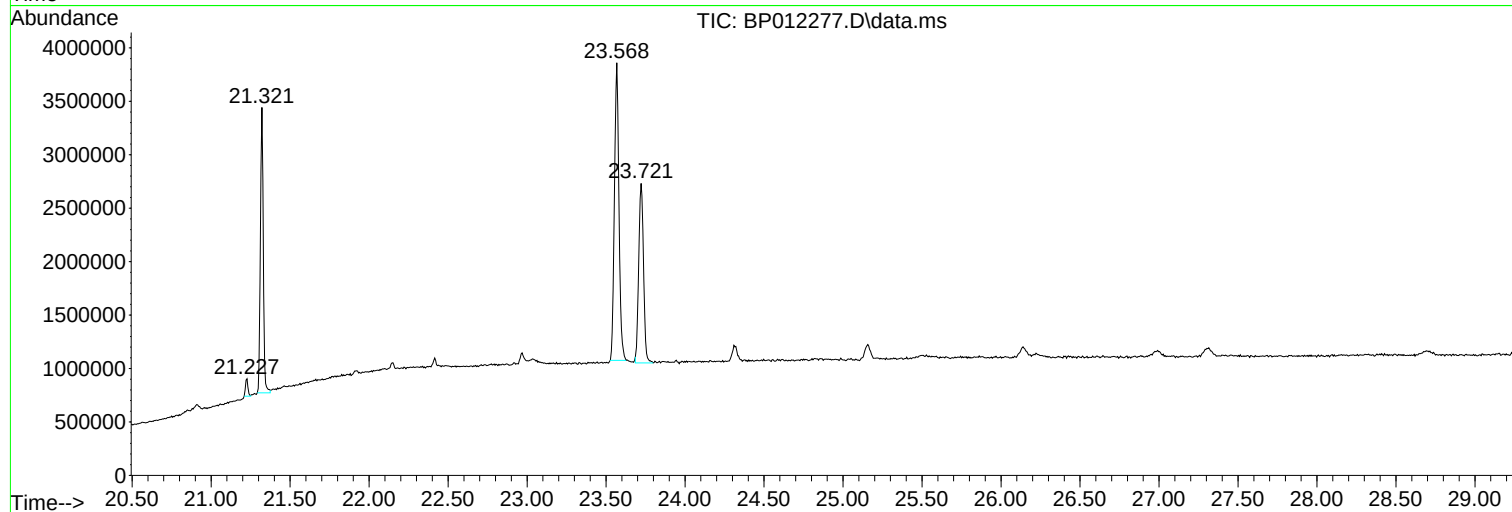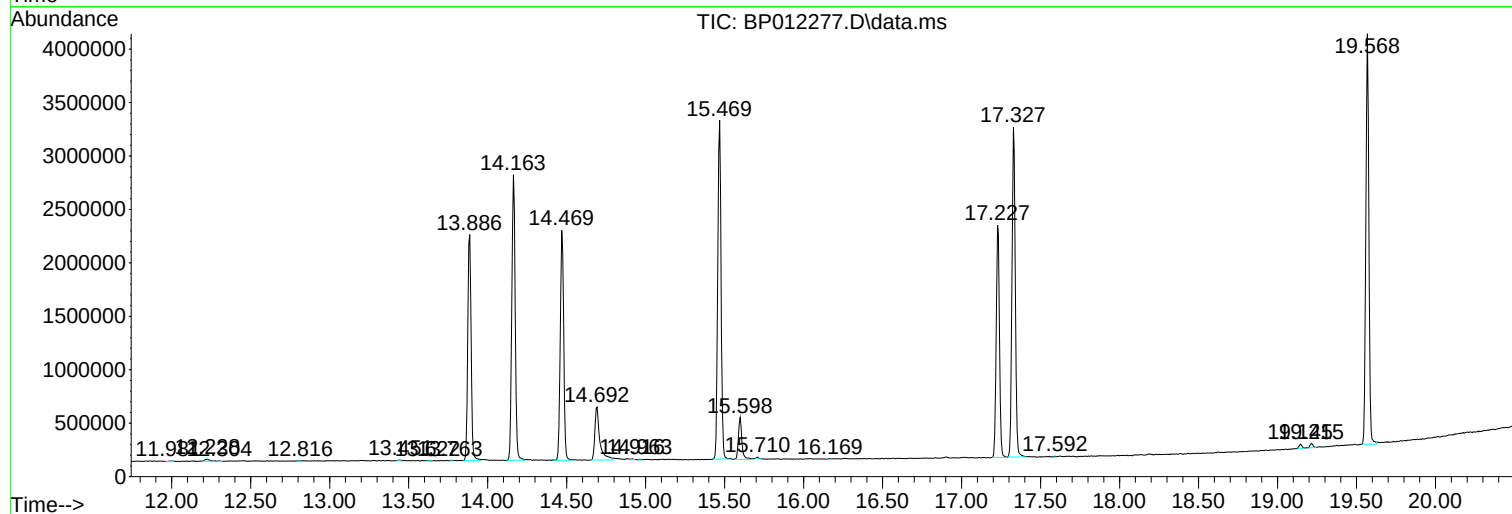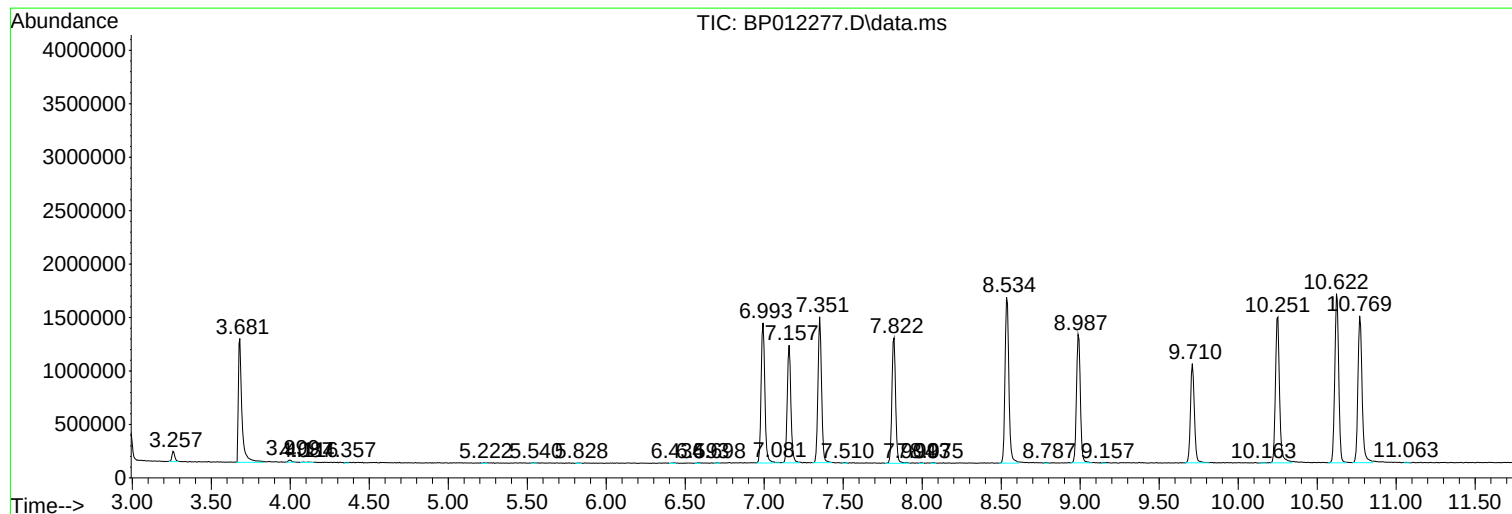

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012277.D
Acq On : 24 Oct 2022 10:30
Operator : CG/JU
Sample : PB148367BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK367

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012277.D
Acq On : 24 Oct 2022 10:30
Operator : CG/JU
Sample : PB148367BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK367

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc