

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012279.D
 Acq On : 24 Oct 2022 11:38
 Operator : CG/JU
 Sample : PB148414BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	43	46	51	rBV	78162	92614	1.46%	0.138%
2	3.687	115	119	136	rBV	368504	630705	9.91%	0.940%
3	3.993	169	171	176	rVB2	22184	30996	0.49%	0.046%
4	4.434	244	246	251	rVB2	7807	11571	0.18%	0.017%
5	6.428	582	585	590	rBV	4551	8375	0.13%	0.012%
6	6.993	674	681	695	rBV	1022837	1672402	26.29%	2.493%
7	7.158	702	709	722	rBV	873117	1387461	21.81%	2.068%
8	7.352	736	742	754	rBV	1050763	1695947	26.66%	2.528%
9	7.817	812	821	832	rVV	1138703	1906254	29.96%	2.842%
10	8.534	936	943	958	rBV	1202774	2060659	32.39%	3.072%
11	8.987	1012	1020	1032	rBV	972721	1656198	26.03%	2.469%
12	9.258	1062	1066	1069	rVB	6808	9415	0.15%	0.014%
13	9.369	1084	1085	1089	rVV	6926	7652	0.12%	0.011%
14	9.711	1135	1143	1158	rBV	764528	1283843	20.18%	1.914%
15	10.246	1227	1234	1250	rBV	1075624	2017218	31.70%	3.007%
16	10.622	1290	1298	1310	rBV	1596374	2761754	43.41%	4.117%
17	10.769	1316	1323	1339	rBV	1112156	2107805	33.13%	3.142%
18	10.946	1351	1353	1357	rVB	5325	6439	0.10%	0.010%
19	11.516	1446	1450	1451	rBV	5550	7240	0.11%	0.011%
20	11.640	1469	1471	1475	rBV	5619	8540	0.13%	0.013%
21	12.216	1566	1569	1577	rBV3	16714	37312	0.59%	0.056%
22	12.734	1654	1657	1662	rVB	5301	7746	0.12%	0.012%
23	13.199	1732	1736	1741	rBV2	4025	7355	0.12%	0.011%
24	13.446	1775	1778	1782	rVB3	6660	8742	0.14%	0.013%
25	13.887	1846	1853	1862	rBV	1920199	2865042	45.03%	4.271%
26	13.987	1868	1870	1874	rVB	5561	6795	0.11%	0.010%
27	14.163	1892	1900	1914	rBV	2471579	3663365	57.58%	5.461%
28	14.469	1945	1952	1969	rBV	2381639	3517724	55.29%	5.244%
29	14.687	1983	1989	2012	rBV	555645	1228411	19.31%	1.831%
30	15.075	2052	2055	2058	rBV	6524	9715	0.15%	0.014%
31	15.469	2114	2122	2133	rBV	3031884	4461063	70.11%	6.650%
32	15.598	2138	2144	2153	rBV	447383	672898	10.58%	1.003%
33	15.710	2158	2163	2166	rVB2	14837	23582	0.37%	0.035%
34	15.969	2205	2207	2211	rBV	5664	7027	0.11%	0.010%
35	16.493	2293	2296	2298	rBV	4440	6363	0.10%	0.009%
36	16.887	2360	2363	2365	rBV4	7411	9666	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012279.D
 Acq On : 24 Oct 2022 11:38
 Operator : CG/JU
 Sample : PB148414BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	17.016	2381	2385	2388	rBV2	9092	10773	0.17%	0.016%
38	17.087	2394	2397	2399	rBV	6965	10440	0.16%	0.016%
39	17.228	2415	2421	2432	rBV	2888395	4094447	64.35%	6.103%
40	17.328	2432	2438	2451	rVB2	3508789	5049897	79.37%	7.528%
41	19.145	2743	2747	2752	rBV3	42618	61523	0.97%	0.092%
42	19.210	2755	2758	2764	rBV2	42629	68557	1.08%	0.102%
43	19.569	2813	2819	2829	rBV	4368737	5920839	93.06%	8.826%
44	21.228	3098	3101	3105	rBV	212498	226681	3.56%	0.338%
45	21.322	3112	3117	3125	rBV	3738625	4689565	73.71%	6.990%
46	23.569	3492	3499	3510	rVB2	3051933	6362544	100.00%	9.484%
47	23.722	3519	3525	3534	rVB2	2394734	4694718	73.79%	6.998%




Sum of corrected areas: 67085878

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012279.D
Acq On : 24 Oct 2022 11:38
Operator : CG/JU
Sample : PB148414BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

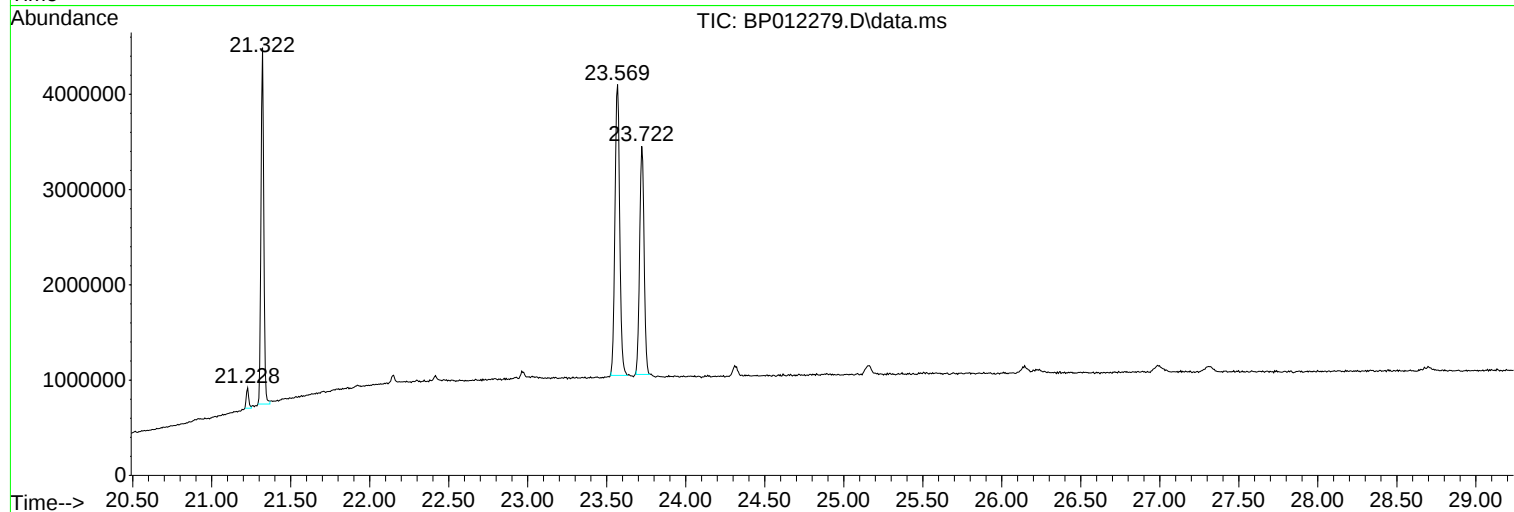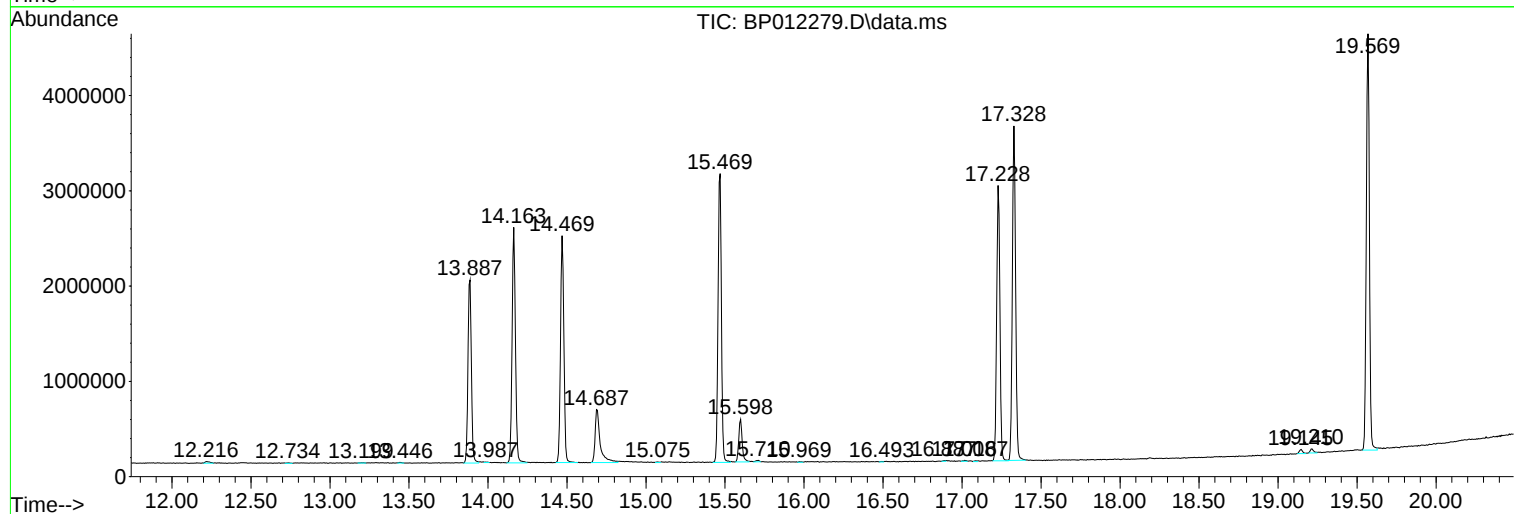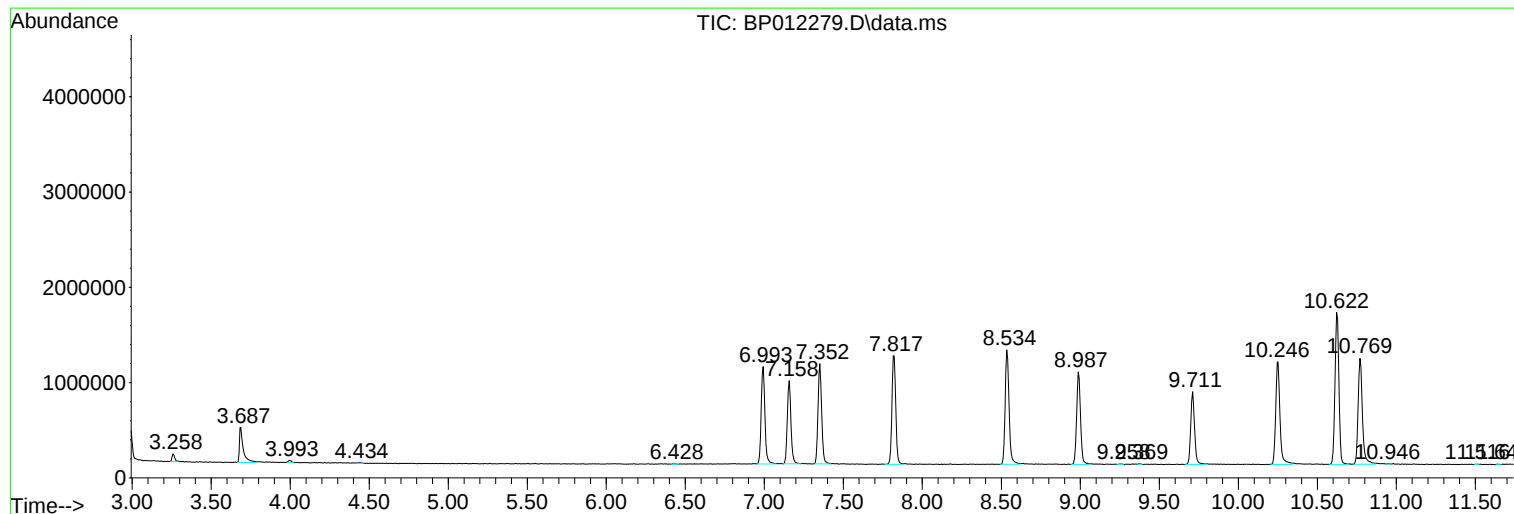

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012279.D
Acq On : 24 Oct 2022 11:38
Operator : CG/JU
Sample : PB148414BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012279.D
Acq On : 24 Oct 2022 11:38
Operator : CG/JU
Sample : PB148414BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc