

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012283.D
 Acq On : 24 Oct 2022 13:56
 Operator : CG/JU
 Sample : N5070-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	56	rVB	67282	87650	1.66%	0.148%
2	3.510	85	89	91	rBV5	9517	12208	0.23%	0.021%
3	3.681	115	118	123	rVB2	29417	39780	0.75%	0.067%
4	3.722	123	125	126	rBV	13600	12350	0.23%	0.021%
5	3.781	131	135	142	rVV	123265	157433	2.98%	0.265%
6	3.858	145	148	150	rVV2	17338	20483	0.39%	0.035%
7	3.899	150	155	161	rVB	77149	108305	2.05%	0.183%
8	3.999	167	172	177	rVB	63564	87943	1.67%	0.148%
9	4.369	232	235	242	rVB3	18086	27867	0.53%	0.047%
10	4.557	263	267	272	rVB3	32321	46646	0.88%	0.079%
11	4.934	323	331	337	rBV2	120968	229603	4.35%	0.387%
12	5.028	343	347	356	rVB3	16252	32310	0.61%	0.054%
13	5.322	393	397	402	rBV3	9148	12050	0.23%	0.020%
14	5.452	414	419	427	rBV2	27133	53093	1.01%	0.089%
15	5.822	476	482	489	rBV2	42427	66528	1.26%	0.112%
16	6.299	556	563	570	rBV7	12153	25921	0.49%	0.044%
17	6.687	622	629	632	rBV8	8019	14818	0.28%	0.025%
18	6.793	642	647	653	rBV	9649	17817	0.34%	0.030%
19	6.987	674	680	697	rVB	866557	1529454	28.96%	2.578%
20	7.151	702	708	722	rBV	837033	1395637	26.43%	2.352%
21	7.351	735	742	752	rBV	932001	1515129	28.69%	2.554%
22	7.434	752	756	757	rVV4	15761	23981	0.45%	0.040%
23	7.457	757	760	766	rVB2	23805	37355	0.71%	0.063%
24	7.646	784	792	796	rBV2	9033	18673	0.35%	0.031%
25	7.816	811	821	830	rBV	1255632	2041595	38.66%	3.441%
26	7.922	837	839	847	rVB4	9072	14472	0.27%	0.024%
27	8.463	926	931	934	rBV5	7055	12961	0.25%	0.022%
28	8.534	936	943	954	rBV	629863	1096563	20.76%	1.848%
29	8.651	959	963	972	rVB2	25801	47178	0.89%	0.080%
30	8.987	1013	1020	1033	rBV	935123	1576446	29.85%	2.657%
31	9.151	1046	1048	1056	rVB8	10159	21353	0.40%	0.036%
32	9.375	1080	1086	1091	rBV	37226	57450	1.09%	0.097%
33	9.710	1135	1143	1158	rBV	670382	1192964	22.59%	2.011%
34	10.028	1191	1197	1201	rBV6	6991	13165	0.25%	0.022%
35	10.245	1226	1234	1247	rBV	961555	1703981	32.26%	2.872%
36	10.410	1257	1262	1278	rBV2	68016	196622	3.72%	0.331%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012283.D
 Acq On : 24 Oct 2022 13:56
 Operator : CG/JU
 Sample : N5070-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	10.622	1288	1298	1304	rBV	1667753	2824477	53.48%	4.761%
38	10.669	1304	1306	1313	rVV	65691	96230	1.82%	0.162%
39	10.769	1316	1323	1342	rVB	261806	535461	10.14%	0.903%
40	11.645	1466	1472	1477	rBV3	12194	25473	0.48%	0.043%

41	11.869	1507	1510	1519	rVB6	7049	14217	0.27%	0.024%
42	12.039	1535	1539	1543	rBV3	19513	29976	0.57%	0.051%
43	12.163	1554	1560	1564	rBV3	21060	39491	0.75%	0.067%
44	12.216	1564	1569	1575	rVV	21726	39976	0.76%	0.067%
45	12.286	1575	1581	1590	rVB	65481	113247	2.14%	0.191%

46	12.510	1612	1619	1626	rVB	57016	99563	1.89%	0.168%
47	12.992	1695	1701	1706	rBV3	12899	24083	0.46%	0.041%
48	13.063	1708	1713	1718	rBV8	7373	15924	0.30%	0.027%
49	13.281	1743	1750	1758	rBV3	45480	85590	1.62%	0.144%
50	13.363	1758	1764	1770	rVB2	20043	33439	0.63%	0.056%

51	13.433	1772	1776	1781	rVB4	9005	14541	0.28%	0.025%
52	13.633	1805	1810	1816	rBV5	14843	39286	0.74%	0.066%
53	13.786	1830	1836	1841	rBV2	40672	73312	1.39%	0.124%
54	13.845	1841	1846	1847	rVV	28949	41182	0.78%	0.069%
55	13.881	1847	1852	1860	rVV	1887708	2644797	50.08%	4.458%

56	13.939	1860	1862	1866	rVB2	27565	32382	0.61%	0.055%
57	14.022	1873	1876	1879	rBV3	19038	23328	0.44%	0.039%
58	14.057	1880	1882	1888	rVB2	14770	18048	0.34%	0.030%
59	14.163	1888	1900	1917	rBV2	2192722	3439100	65.12%	5.797%
60	14.357	1927	1933	1940	rVB2	30862	47584	0.90%	0.080%

61	14.469	1940	1952	1959	rBV	2228932	3276614	62.04%	5.523%
62	14.692	1984	1990	2011	rBV	142623	403144	7.63%	0.680%
63	14.869	2014	2020	2024	rBV3	26911	56137	1.06%	0.095%
64	14.986	2037	2040	2047	rVB7	10994	22711	0.43%	0.038%
65	15.092	2052	2058	2062	rVV4	12511	22714	0.43%	0.038%

66	15.139	2062	2066	2069	rVV3	11974	13600	0.26%	0.023%
67	15.257	2079	2086	2089	rBV7	22036	45125	0.85%	0.076%
68	15.310	2092	2095	2099	rVB2	28036	39722	0.75%	0.067%
69	15.463	2114	2121	2127	rBV	2824912	4038100	76.46%	6.807%
70	15.598	2138	2144	2156	rVV	259995	410791	7.78%	0.692%

71	15.710	2159	2163	2174	rVB10	21745	54866	1.04%	0.092%
72	15.816	2177	2181	2187	rVB	17981	27264	0.52%	0.046%
73	15.927	2197	2200	2203	rBV4	10638	16224	0.31%	0.027%
74	15.963	2203	2206	2213	rVV3	19083	31425	0.60%	0.053%
75	16.039	2215	2219	2227	rVB8	11444	26461	0.50%	0.045%

76	16.204	2239	2247	2252	rBV2	57133	117463	2.22%	0.198%
----	--------	------	------	------	------	-------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012283.D
 Acq On : 24 Oct 2022 13:56
 Operator : CG/JU
 Sample : N5070-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

77	16.339	2266	2270	2275	rBV6	8393	20703	0.39%	0.035%
78	16.769	2337	2343	2351	rBV7	33804	76891	1.46%	0.130%
79	16.880	2359	2362	2371	rBV6	14455	28919	0.55%	0.049%
80	16.951	2371	2374	2375	rBV3	11469	12095	0.23%	0.020%
81	16.980	2375	2379	2382	rVB	20194	27602	0.52%	0.047%
82	17.122	2400	2403	2410	rVB5	23047	44679	0.85%	0.075%
83	17.227	2411	2421	2426	rBV	2321558	3377052	63.94%	5.692%
84	17.269	2426	2428	2432	rVV	163215	194370	3.68%	0.328%
85	17.327	2432	2438	2449	rVB	2609667	3791555	71.79%	6.391%
86	17.721	2502	2505	2508	rBV2	17445	20194	0.38%	0.034%
87	17.898	2531	2535	2541	rVB	45114	60912	1.15%	0.103%
88	18.110	2565	2571	2575	rBV2	148732	246865	4.67%	0.416%
89	18.145	2575	2577	2582	rVB	59116	71936	1.36%	0.121%
90	18.280	2596	2600	2604	rBV3	31049	55752	1.06%	0.094%
91	18.398	2616	2620	2624	rBV3	32646	57036	1.08%	0.096%
92	18.592	2649	2653	2657	rBV3	28728	43072	0.82%	0.073%
93	19.216	2755	2759	2760	rBV2	46255	64747	1.23%	0.109%
94	19.239	2760	2763	2771	rVB	253830	357193	6.76%	0.602%
95	19.345	2778	2781	2788	rBV3	86797	138446	2.62%	0.233%
96	19.568	2813	2819	2832	rBV	3420211	4923766	93.23%	8.299%
97	21.021	3063	3066	3075	rBV4	254353	435969	8.25%	0.735%
98	21.321	3112	3117	3121	rBV	2834843	3744383	70.90%	6.311%
99	23.562	3492	3498	3513	rVB2	2465036	5281303	100.00%	8.902%
100	23.715	3519	3524	3534	rVB2	1863861	3750619	71.02%	6.322%




Sum of corrected areas: 59326911

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012283.D
Acq On : 24 Oct 2022 13:56
Operator : CG/JU
Sample : N5070-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BL7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

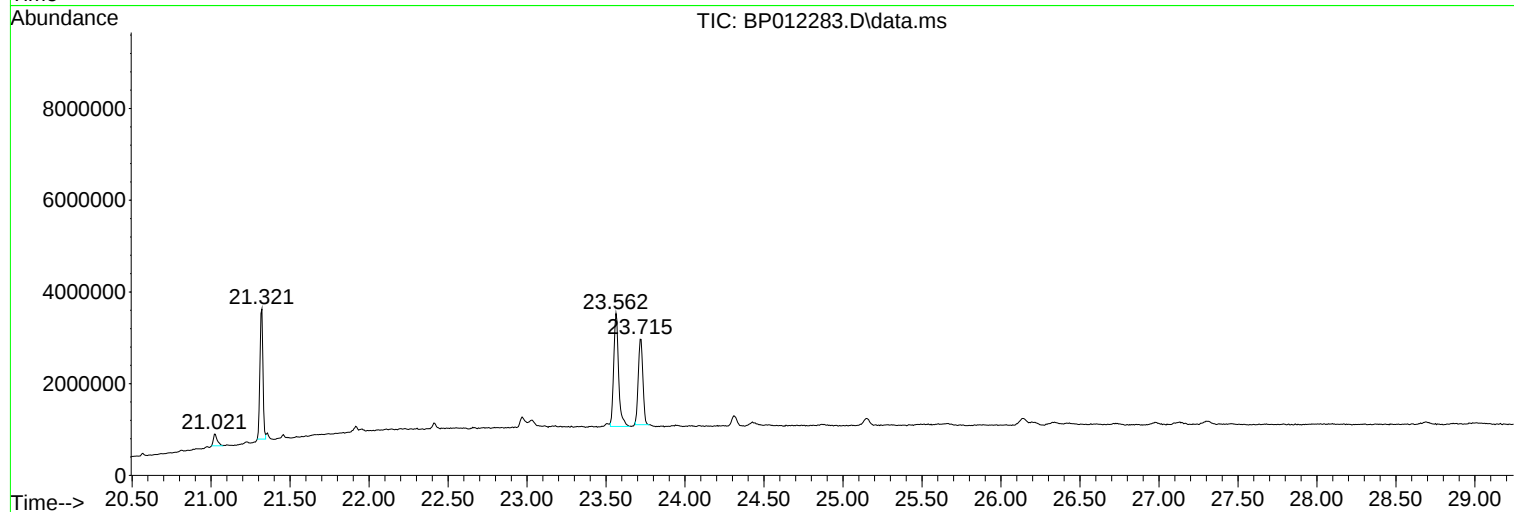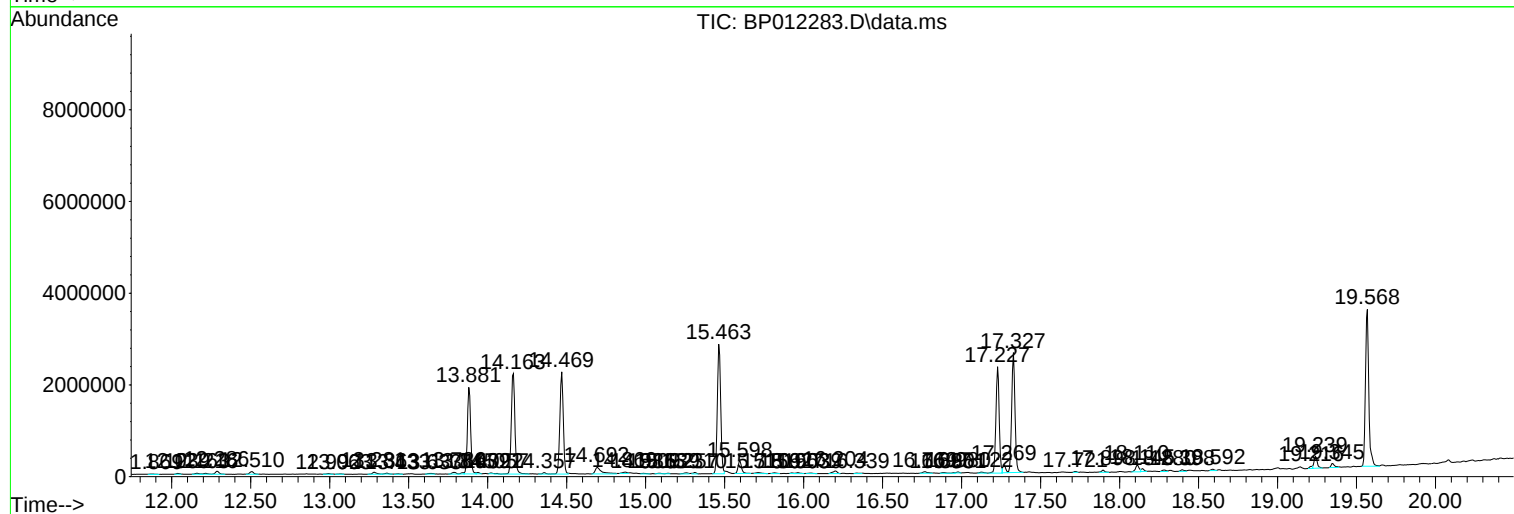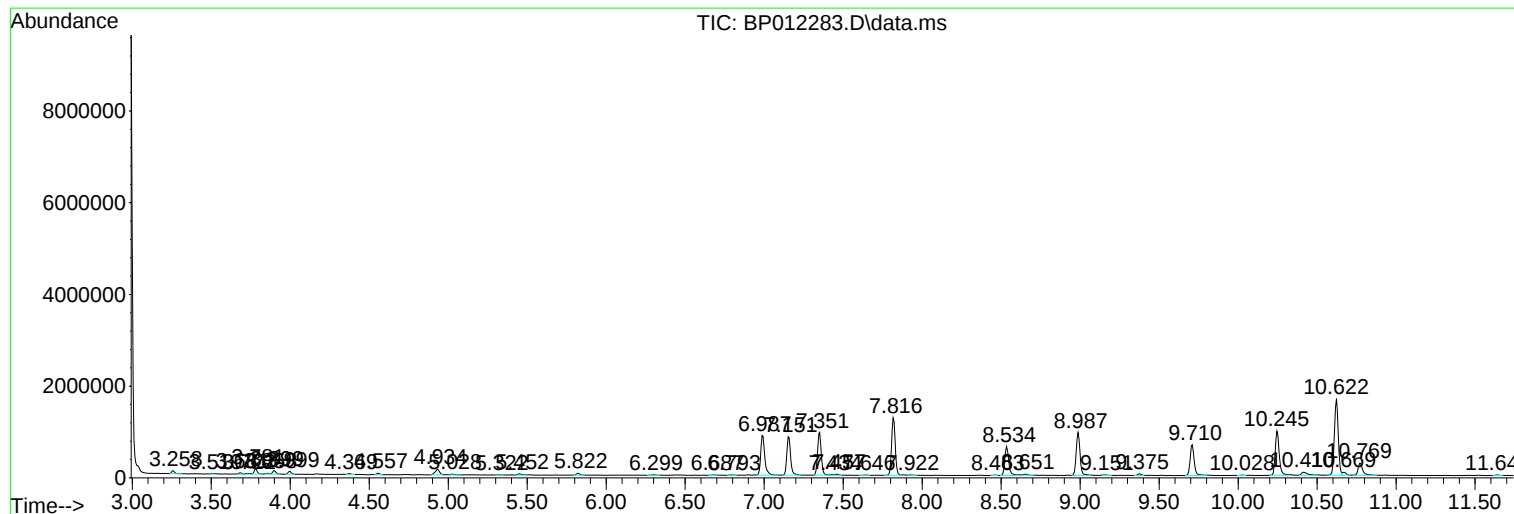

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012283.D
Acq On : 24 Oct 2022 13:56
Operator : CG/JU
Sample : N5070-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BL7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.934	2.25 ng/ul	229603	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
3	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
4	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	37		
5	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	36		

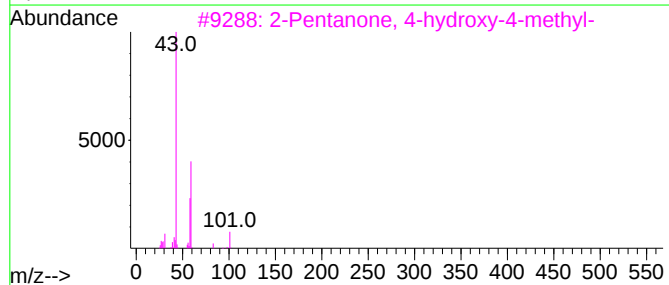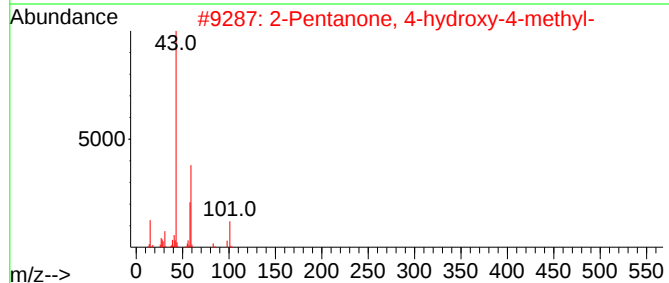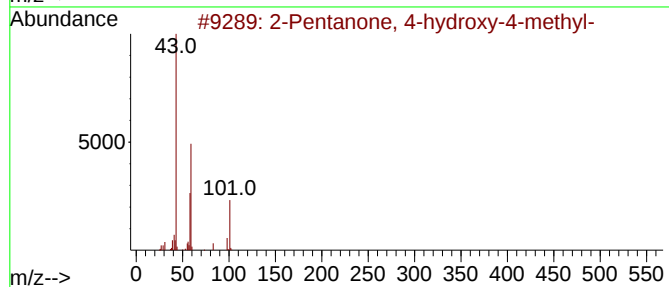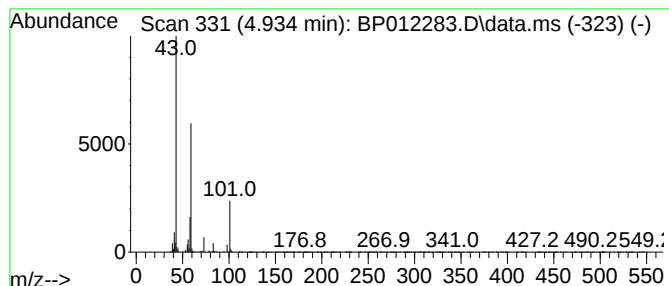

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012283.D
Acq On : 24 Oct 2022 13:56
Operator : CG/JU
Sample : N5070-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BL7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Oxalic acid, hexadecyl prop... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.021	2.33 ng/ul	435969	Chrysene-d12	21.321

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxalic acid, hexadecyl propyl ester	356	C21H40O4	1000309-26-9	91
2			Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	91
3			Oxalic acid, isobutyl octadecyl ...	398	C24H46O4	1000309-38-3	87
4			Oxalic acid, isobutyl heptadecyl...	384	C23H44O4	1000309-38-2	87
5			Cyclotetracosane	336	C24H48	000297-03-0	86

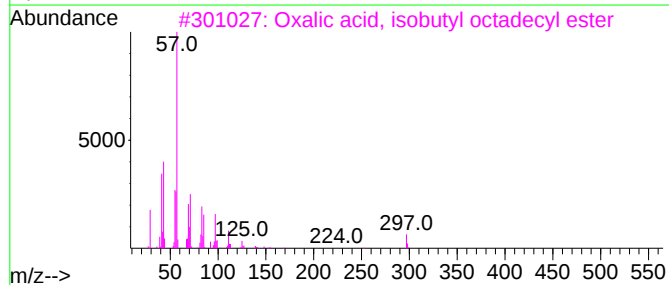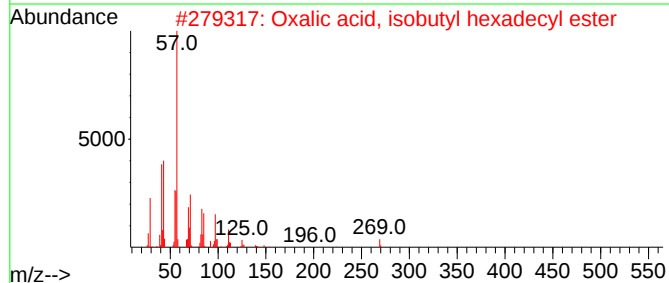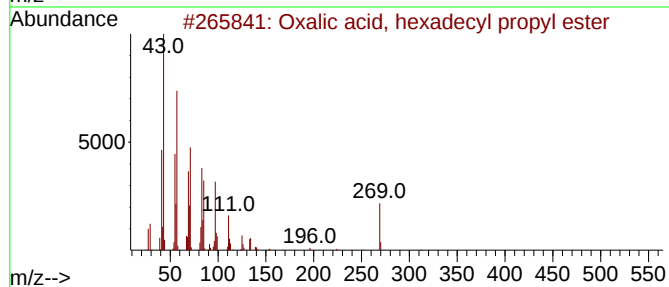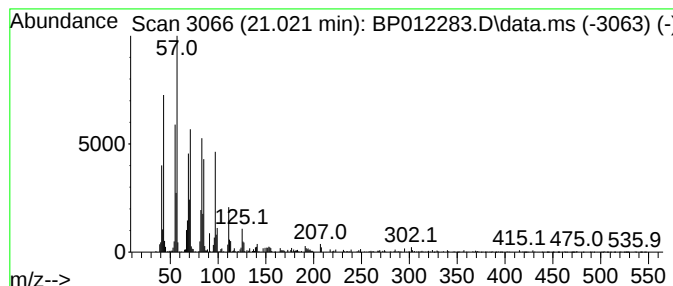

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012283.D
Acq On : 24 Oct 2022 13:56
Operator : CG/JU
Sample : N5070-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BL7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.934	2.3	ng/ul	229603	1	7.816	2041600	20.0
Oxalic acid, he...	21.021	2.3	ng/ul	435969	5	21.321	3744380	20.0