

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012289.D
 Acq On : 24 Oct 2022 17:22
 Operator : CG/JU
 Sample : N5070-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	117	119	127	rBV	85912	133327	2.97%	0.239%
2	6.987	675	680	693	rVB	854999	1469711	32.77%	2.629%
3	7.152	703	708	721	rVB	829613	1344217	29.97%	2.405%
4	7.346	735	741	753	rBV	929499	1521764	33.93%	2.722%
5	7.816	815	821	830	rVB	1269883	2005552	44.72%	3.588%
6	8.534	937	943	953	rBV	880515	1533878	34.20%	2.744%
7	8.987	1013	1020	1030	rBV	1023036	1736478	38.72%	3.106%
8	9.369	1083	1085	1091	rVB3	24405	36137	0.81%	0.065%
9	9.705	1136	1142	1152	rBV	686574	1178316	26.27%	2.108%
10	10.246	1227	1234	1256	rBV	1046489	1880343	41.93%	3.364%
11	10.410	1257	1262	1276	rVV	66963	175804	3.92%	0.315%
12	10.622	1290	1298	1310	rVB	1805112	3052659	68.07%	5.461%
13	10.769	1316	1323	1335	rBV	726760	1312956	29.28%	2.349%
14	11.805	1496	1499	1504	rBV	5606	8230	0.18%	0.015%
15	11.869	1507	1510	1516	rVB5	7649	13633	0.30%	0.024%
16	12.040	1534	1539	1543	rBV6	7524	13893	0.31%	0.025%
17	12.216	1564	1569	1576	rVB4	17084	32240	0.72%	0.058%
18	12.287	1578	1581	1587	rVV7	7029	12647	0.28%	0.023%
19	12.504	1616	1618	1623	rVB	5104	6603	0.15%	0.012%
20	12.669	1642	1646	1647	rBV3	4172	4559	0.10%	0.008%
21	12.816	1668	1671	1674	rBV5	4797	6617	0.15%	0.012%
22	12.852	1674	1677	1680	rVB3	4715	5850	0.13%	0.010%
23	12.993	1698	1701	1708	rVV4	5323	9951	0.22%	0.018%
24	13.069	1708	1714	1719	rVB7	5960	10774	0.24%	0.019%
25	13.193	1730	1735	1739	rBV6	6499	8564	0.19%	0.015%
26	13.281	1745	1750	1755	rBV2	24131	37927	0.85%	0.068%
27	13.357	1758	1763	1769	rVV4	13758	23064	0.51%	0.041%
28	13.428	1773	1775	1780	rVB6	5749	8577	0.19%	0.015%
29	13.881	1846	1852	1865	rBV	1601143	2223174	49.57%	3.977%
30	13.981	1867	1869	1874	rVB5	5817	9049	0.20%	0.016%
31	14.157	1886	1899	1910	rBV2	2186088	3332469	74.31%	5.962%
32	14.363	1927	1934	1939	rVB3	13741	23244	0.52%	0.042%
33	14.469	1945	1952	1965	rVB	2346066	3474819	77.48%	6.216%
34	14.634	1976	1980	1984	rBV7	4704	7258	0.16%	0.013%
35	14.693	1984	1990	2012	rVV	243577	592683	13.22%	1.060%
36	14.875	2018	2021	2022	rBV3	6609	4953	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
 Data File : BP012289.D
 Acq On : 24 Oct 2022 17:22
 Operator : CG/JU
 Sample : N5070-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	14.904	2022	2026	2029	rVB6	9402	15458	0.34%	0.028%
38	15.263	2080	2087	2090	rBV2	11061	17404	0.39%	0.031%
39	15.310	2092	2095	2100	rVB4	17229	22591	0.50%	0.040%
40	15.463	2115	2121	2137	rBV	2565938	3710212	82.73%	6.637%

41	15.593	2137	2143	2158	rVV	206146	336094	7.49%	0.601%
42	15.704	2158	2162	2167	rVB6	16035	26996	0.60%	0.048%
43	15.875	2186	2191	2195	rVB5	4909	9992	0.22%	0.018%
44	15.922	2195	2199	2203	rBV7	6903	12159	0.27%	0.022%
45	16.093	2226	2228	2231	rBV4	3254	4565	0.10%	0.008%

46	16.175	2239	2242	2251	rVB9	10211	20941	0.47%	0.037%
47	16.251	2251	2255	2257	rBV5	6193	5332	0.12%	0.010%
48	16.345	2267	2271	2272	rBV4	4582	5370	0.12%	0.010%
49	16.369	2272	2275	2278	rVB5	3985	5691	0.13%	0.010%
50	16.528	2295	2302	2305	rBV8	5584	11612	0.26%	0.021%

51	16.569	2307	2309	2314	rVB5	2544	4745	0.11%	0.008%
52	16.634	2314	2320	2324	rBV7	4945	9855	0.22%	0.018%
53	16.687	2324	2329	2330	rBV4	4847	4950	0.11%	0.009%
54	16.734	2333	2337	2338	rBV2	9771	11051	0.25%	0.020%
55	16.975	2374	2378	2382	rVV5	6654	9865	0.22%	0.018%

56	17.022	2382	2386	2393	rVB7	8791	19495	0.43%	0.035%
57	17.134	2403	2405	2413	rVB8	6549	11650	0.26%	0.021%
58	17.228	2413	2421	2432	rBV	2474317	3480840	77.61%	6.227%
59	17.328	2432	2438	2450	rVV	2426442	3398621	75.78%	6.080%
60	17.716	2502	2504	2508	rVB5	4314	4487	0.10%	0.008%

61	17.892	2531	2534	2538	rBV	33165	38329	0.85%	0.069%
62	17.998	2550	2552	2554	rBV3	5220	5094	0.11%	0.009%
63	18.063	2558	2563	2566	rBV7	10618	17355	0.39%	0.031%
64	18.110	2566	2571	2579	rBV2	113471	186975	4.17%	0.334%
65	18.404	2617	2621	2623	rBV5	8007	12224	0.27%	0.022%

66	18.592	2650	2653	2656	rBV5	10871	15029	0.34%	0.027%
67	19.139	2743	2746	2750	rBV4	30356	44213	0.99%	0.079%
68	19.210	2755	2758	2761	rBV2	26716	38000	0.85%	0.068%
69	19.345	2778	2781	2787	rBV3	65140	103894	2.32%	0.186%
70	19.563	2813	2818	2828	rBV	3088418	3968249	88.48%	7.099%

71	20.563	2986	2988	2992	rVB2	55358	56030	1.25%	0.100%
72	21.022	3063	3066	3076	rBV2	205988	325197	7.25%	0.582%
73	21.316	3112	3116	3124	rBV	3053246	3847977	85.80%	6.884%
74	21.457	3137	3140	3146	rVB3	142196	162183	3.62%	0.290%
75	23.563	3491	3498	3510	rVB	2173275	4484839	100.00%	8.023%

76	23.716	3518	3524	3537	rVB2	2127473	4182031	93.25%	7.481%
----	--------	------	------	------	------	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012289.D
Acq On : 24 Oct 2022 17:22
Operator : CG/JU
Sample : N5070-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BS5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Title : SVOA CALIBRATION




Sum of corrected areas: 55899515

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012289.D
Acq On : 24 Oct 2022 17:22
Operator : CG/JU
Sample : N5070-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

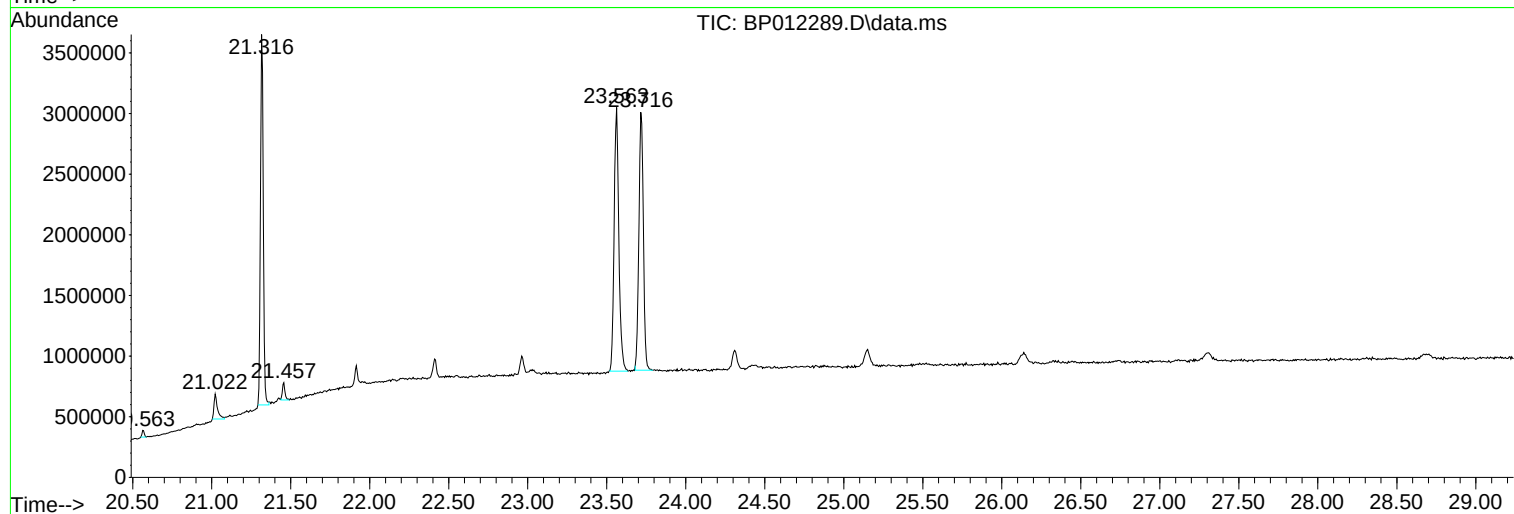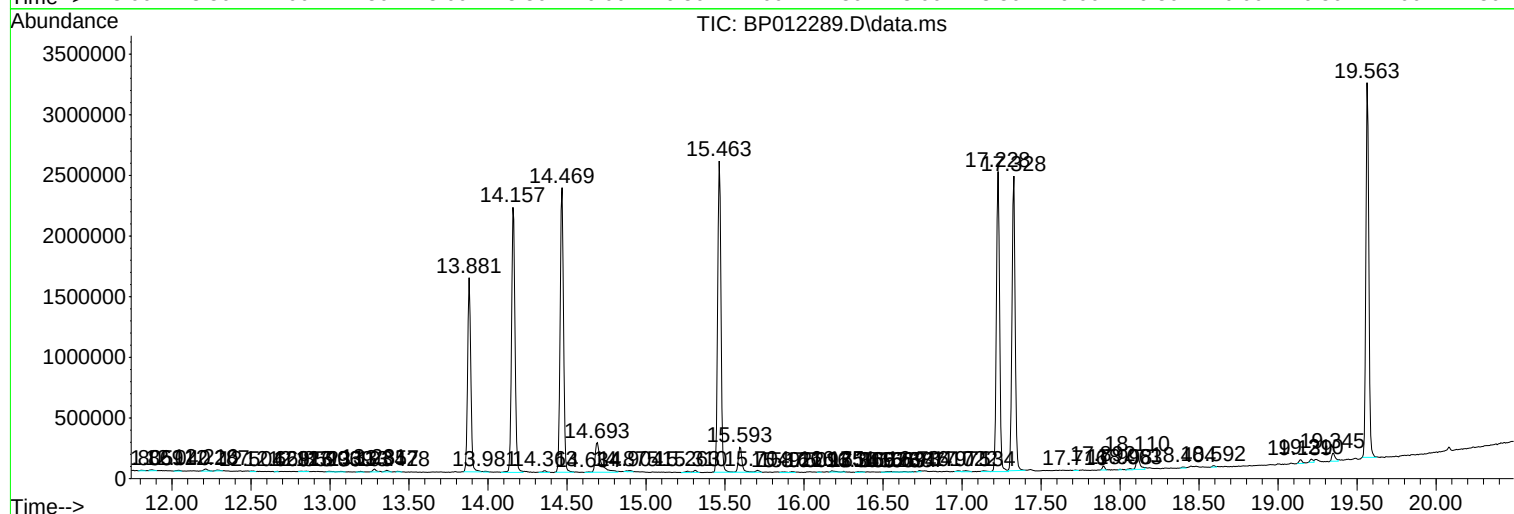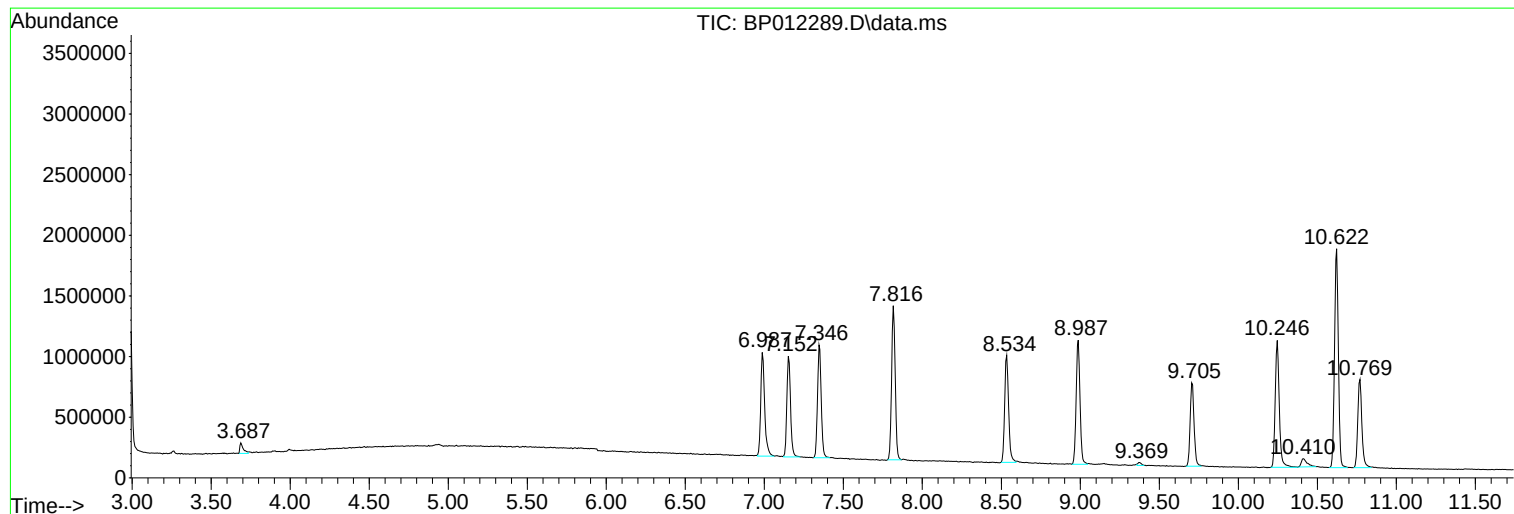

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012289.D
Acq On : 24 Oct 2022 17:22
Operator : CG/JU
Sample : N5070-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102422\
Data File : BP012289.D
Acq On : 24 Oct 2022 17:22
Operator : CG/JU
Sample : N5070-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------